

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072916\
 Data File : BG023327.D
 Acq On : 29 Jul 2016 5:45
 Operator : UM/SJ
 Sample : H4213-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 L-1

Quant Time: Jul 29 07:30:30 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 27 17:30:33 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	166000	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	731203	20.00	ng	0.00
38) Acenaphthene-d10	14.81	164	522813	20.00	ng	0.00
63) Phenanthrene-d10	17.57	188	1216723	20.00	ng	0.00
75) Chrysene-d12	21.89	240	1246195	20.00	ng	0.00
86) Perylene-d12	25.30	264	1270163	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	1222751	125.75	ng	0.00
7) Phenol-d6	7.29	99	1670986	111.93	ng	0.00
23) Nitrobenzene-d5	9.31	82	1283623	85.85	ng	0.00
41) 2,4,6-Tribromophenol	16.31	330	878907	162.42	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	2612306	93.52	ng	0.00
78) Terphenyl-d14	20.18	244	3261524	85.08	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.46	79	21187	2.11	ng	Qvalue # 53
31) Naphthalene	11.02	128	139040	4.09	ng	97
32) Benzoic acid	10.03	122	64	8.12	ng	85
76) Benzidine	19.81	184	265118	7.56	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG072916\
Data File : BG023327.D
Acq On : 29 Jul 2016 5:45
Operator : UM/SJ
Sample : H4213-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
L-1

Quant Time: Jul 29 07:30:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

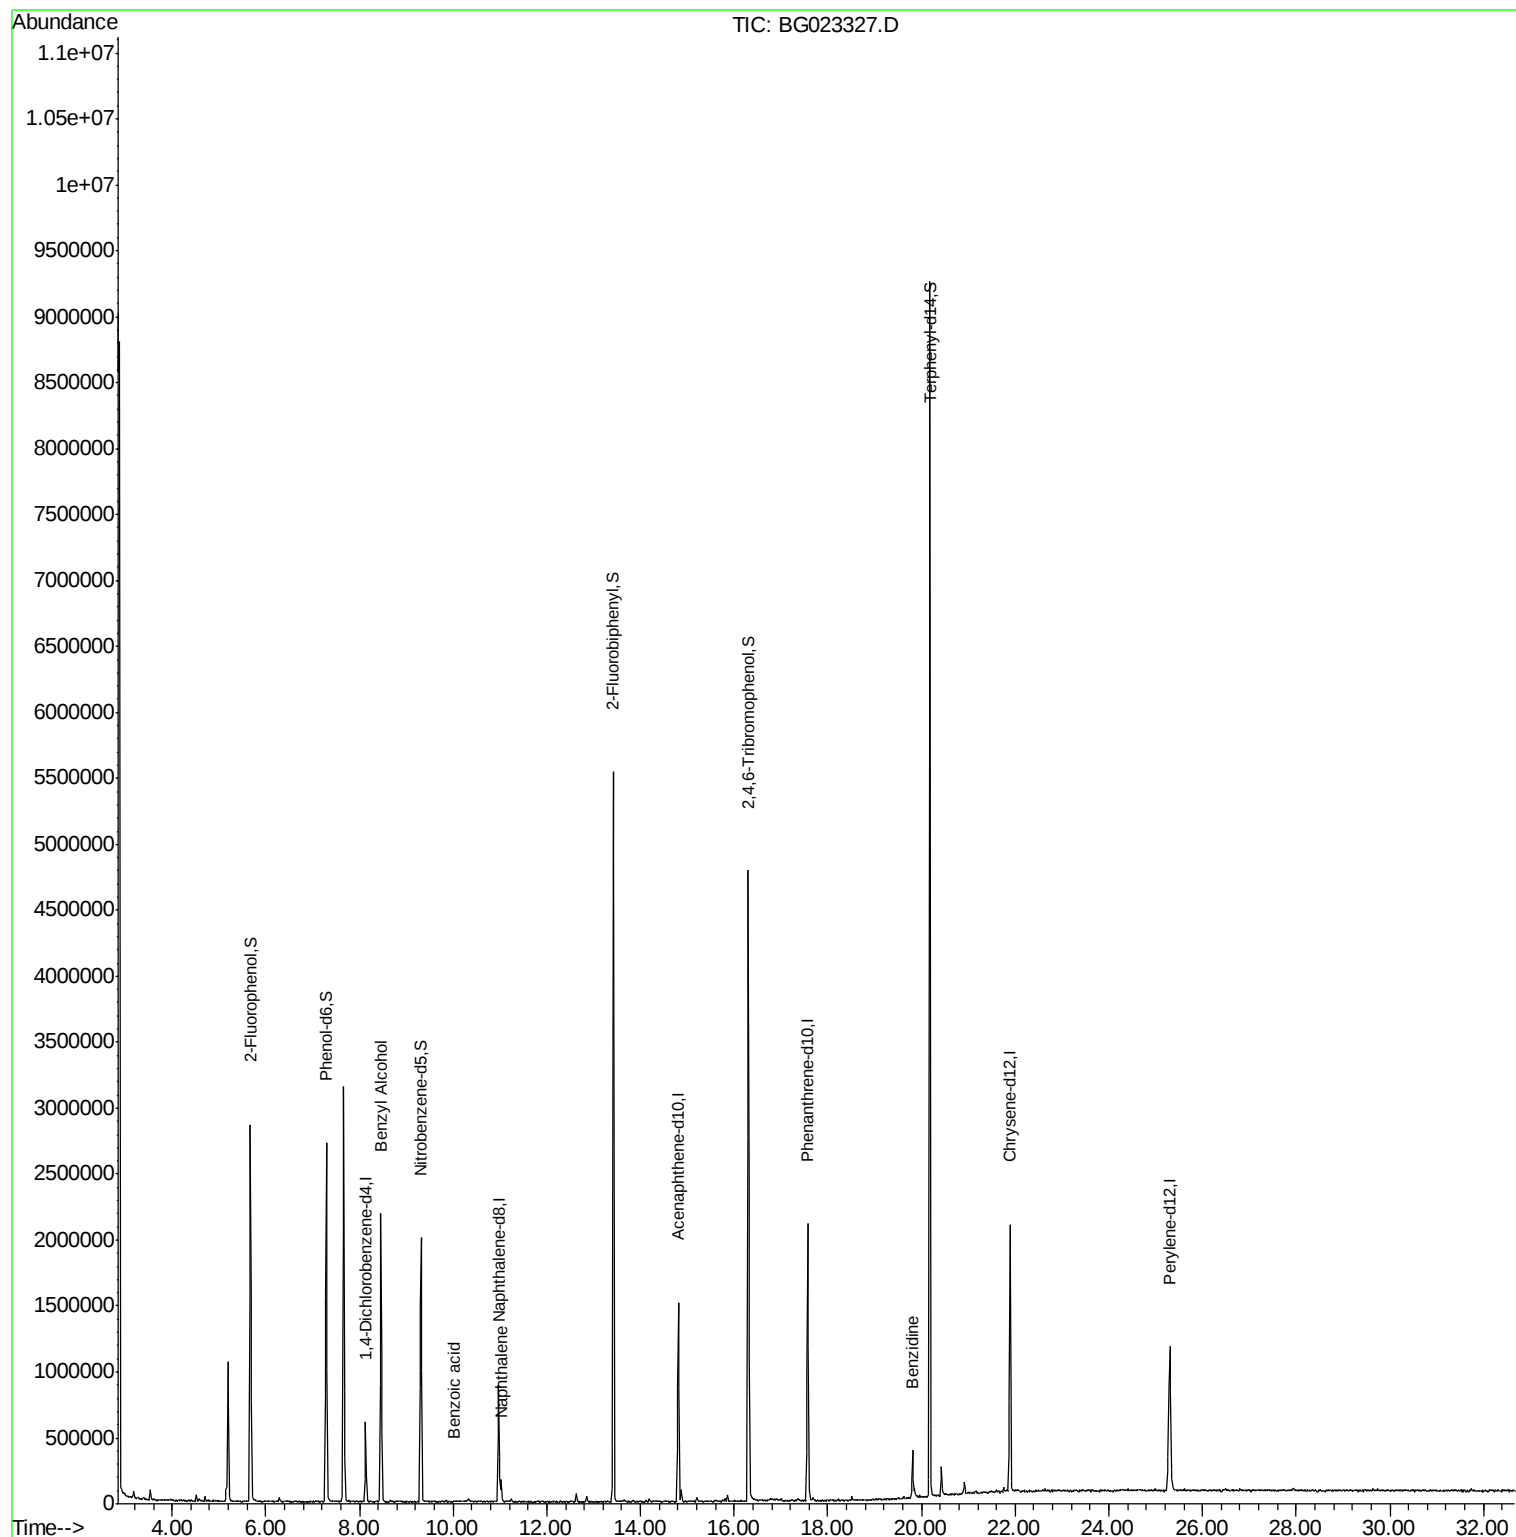



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.13 min Scan# 901

Delta R.T. -0.01 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampleId :

L-1


Tgt Ion:152 Resp: 166000

Ion Ratio Lower Upper

152 100

150 150.2 144.7 217.1




115 53.6 64.0 96.0#

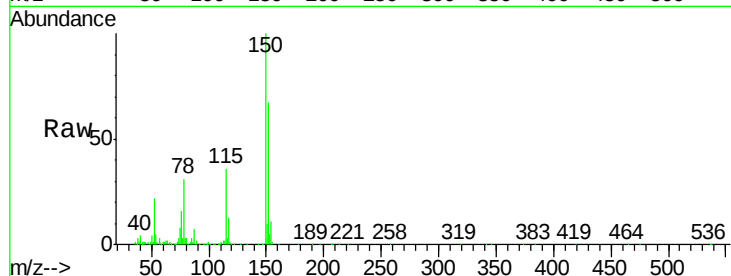

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

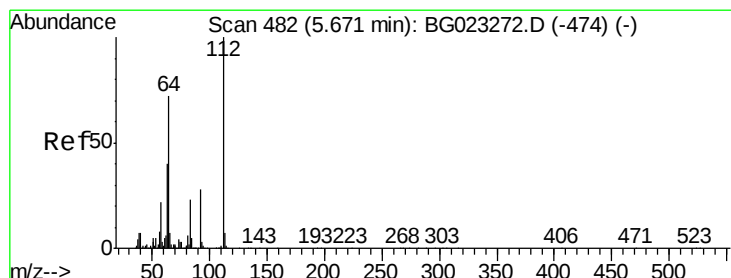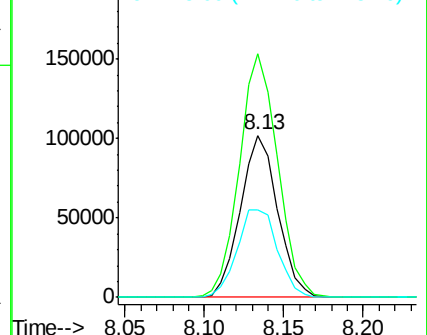

#5

2-Fluorophenol

Concen: 125.75 ng

RT: 5.67 min Scan# 482

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45


Tgt Ion:112 Resp: 1222751

Ion Ratio Lower Upper

112 100

64 71.7 59.0 88.4



63 37.4 37.8 56.8#

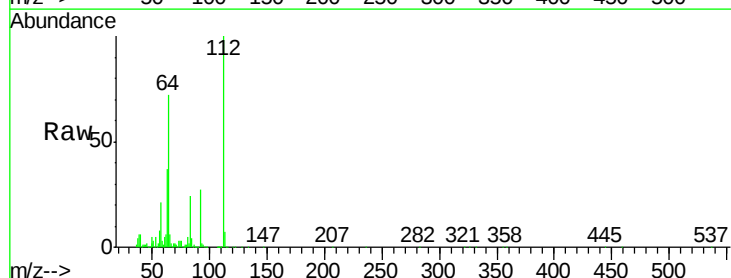


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

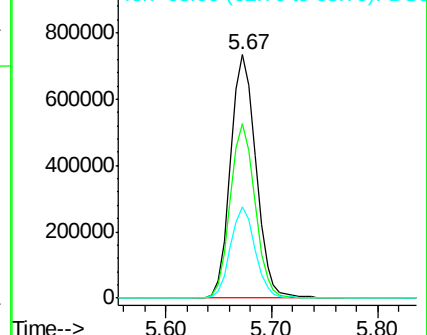

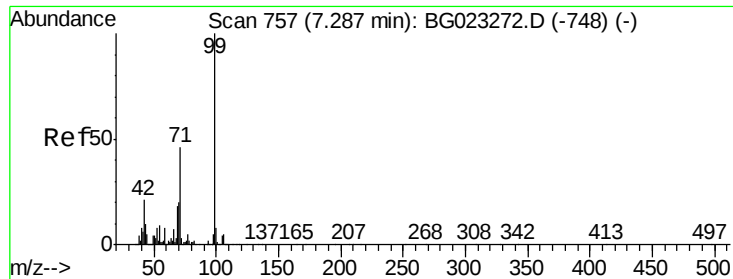

#7

Phenol-d6

Concen: 111.93 ng

RT: 7.29 min Scan# 757

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampleId :

L-1





Tgt Ion: 99 Resp: 1670986

Ion Ratio Lower Upper

99 100

42 18.1 17.8 26.6

71 41.0 41.5 62.3#

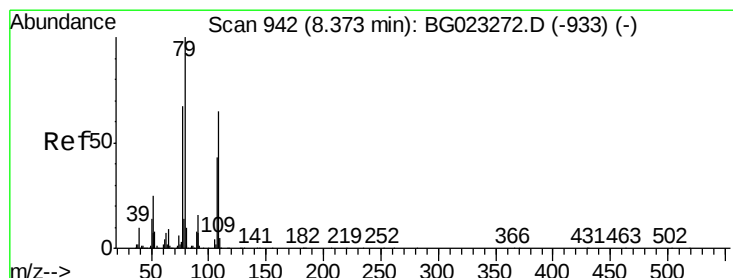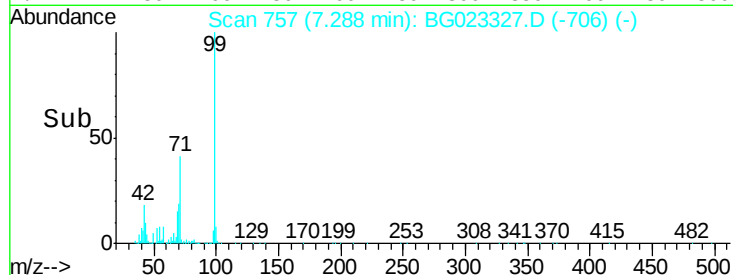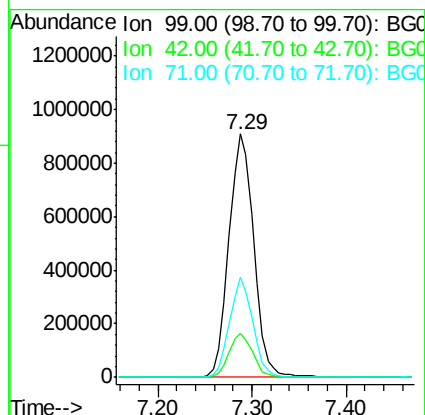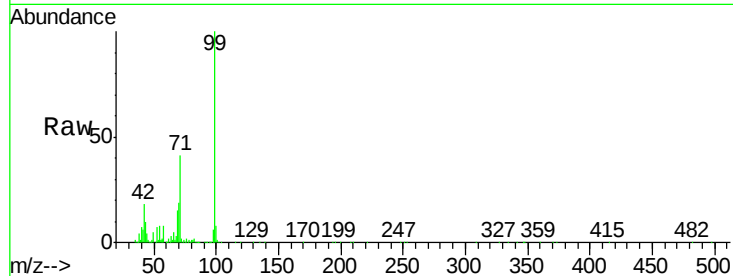

#15

Benzyl Alcohol

Concen: 2.11 ng

RT: 8.46 min Scan# 956

Delta R.T. 0.08 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45




Tgt Ion: 79 Resp: 21187


Ion Ratio Lower Upper

79 100

108 21.3 46.5 69.7#

77 101.0 52.3 78.5#


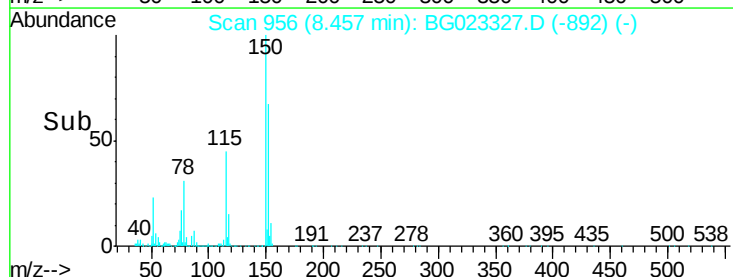
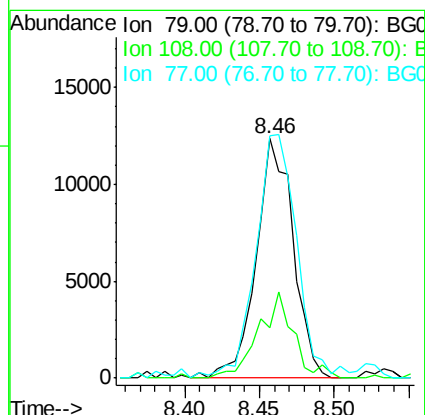
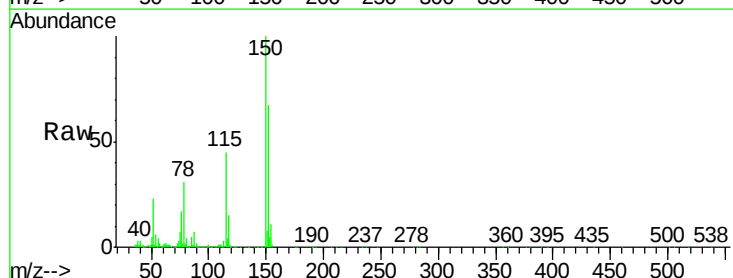




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.97 min Scan# 1384
Delta R.T. -0.01 min
Lab File: BG023327.D
Acq: 29 Jul 2016 5:45




Instrument :
BNA_G
ClientSampleId :
L-1


Tgt Ion:	136	Resp:	731203
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.6	14.4
54	9.6	7.3	10.9
68	8.2	5.3	7.9#

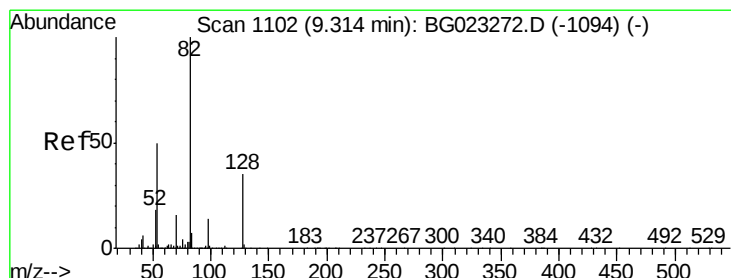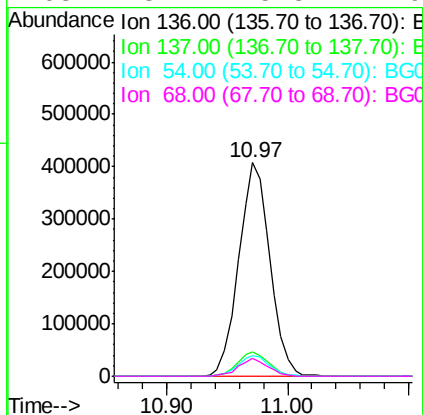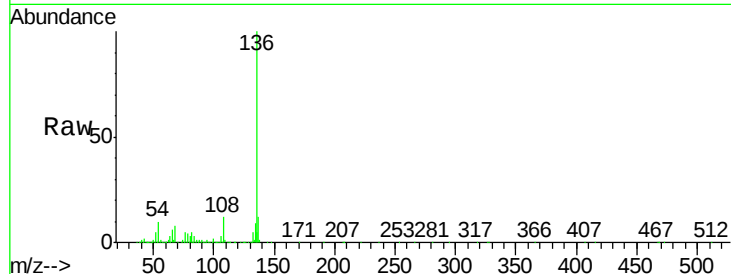

#23
Nitrobenzene-d5
Concen: 85.85 ng
RT: 9.31 min Scan# 1102
Delta R.T. 0.01 min
Lab File: BG023327.D
Acq: 29 Jul 2016 5:45

Tgt Ion:	82	Resp:	1283623
Ion	Ratio	Lower	Upper
82	100		
128	40.0	24.4	36.6#
54	50.3	41.4	62.0



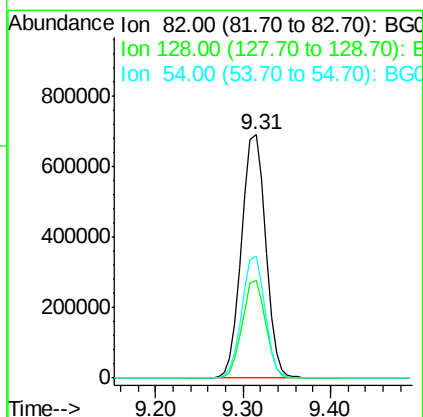
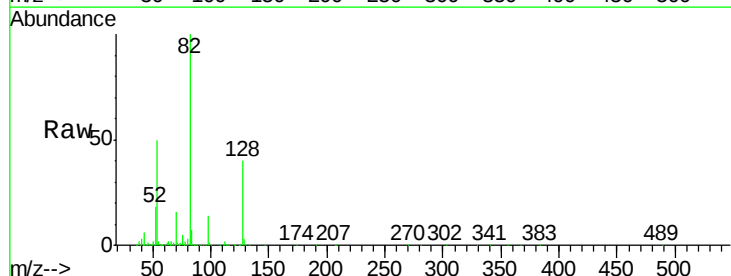


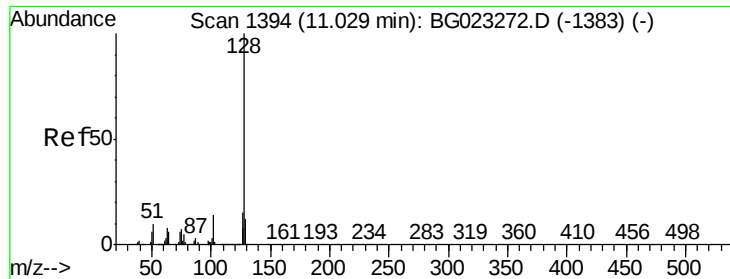

#31
Naphthalene
Concen: 4.09 ng
RT: 11.02 min Scan# 1393
Delta R.T. -0.01 min
Lab File: BG023327.D
Acq: 29 Jul 2016 5:45




Instrument :
BNA_G
ClientSampleId :
L-1


Tgt Ion:128 Resp: 139040
Ion Ratio Lower Upper
128 100
129 10.6 9.4 14.0
127 15.5 11.3 16.9

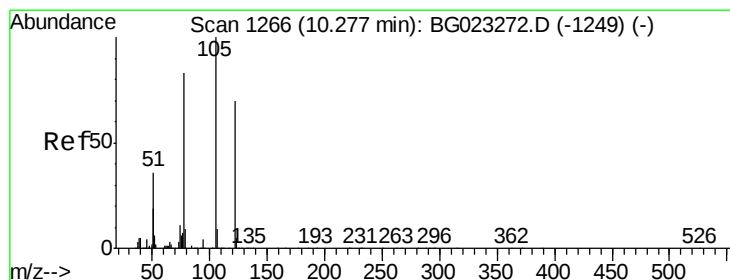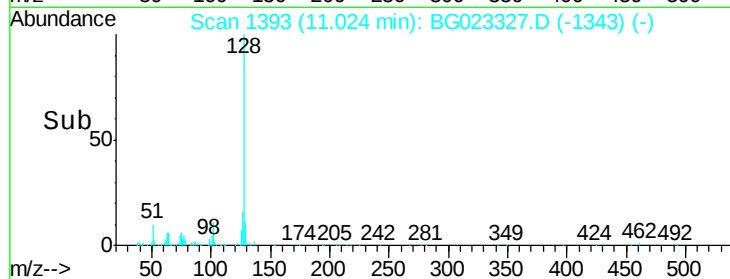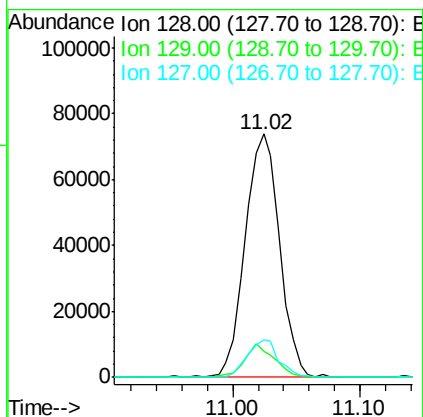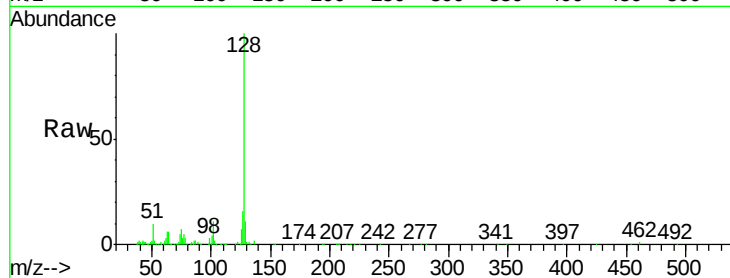

#32
Benzoic acid
Concen: 8.12 ng
RT: 10.03 min Scan# 1223
Delta R.T. -0.25 min
Lab File: BG023327.D
Acq: 29 Jul 2016 5:45

Tgt Ion:122 Resp: 64
Ion Ratio Lower Upper
122 100
105 119.2 117.2 157.2
77 146.7 109.2 149.2

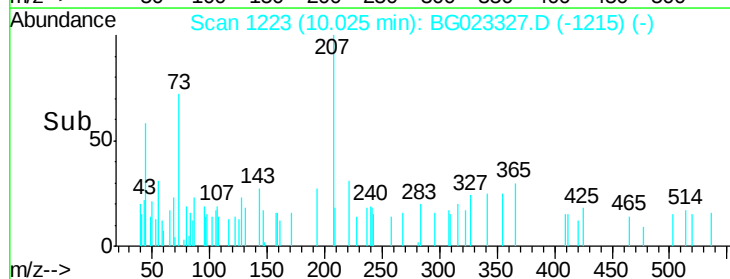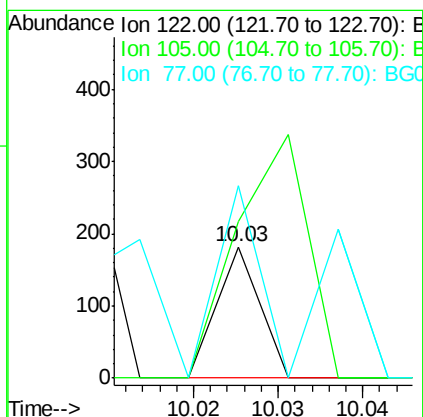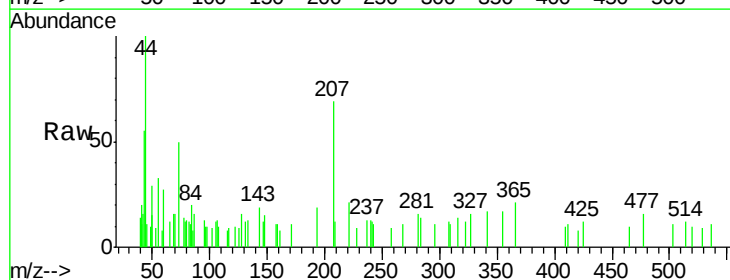

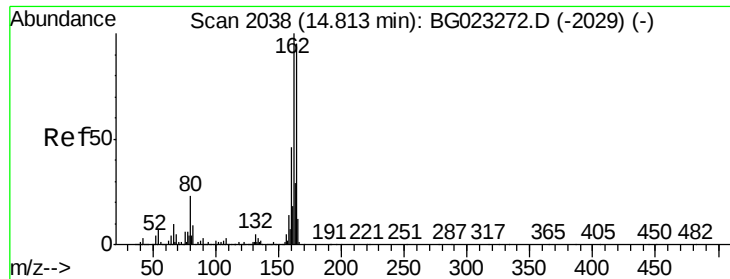

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.81 min Scan# 2037

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampleId :

L-1


Tgt Ion:164 Resp: 522813

Ion Ratio Lower Upper

164 100

162 101.3 87.7 131.5




160 45.3 37.2 55.8

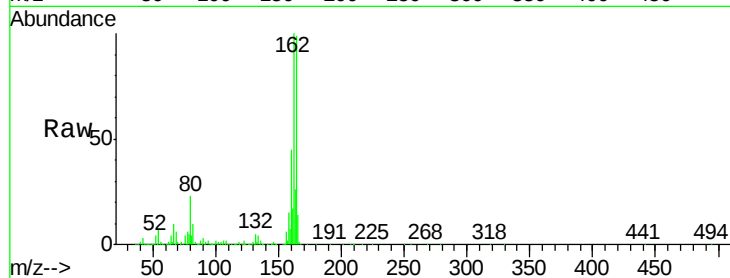

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

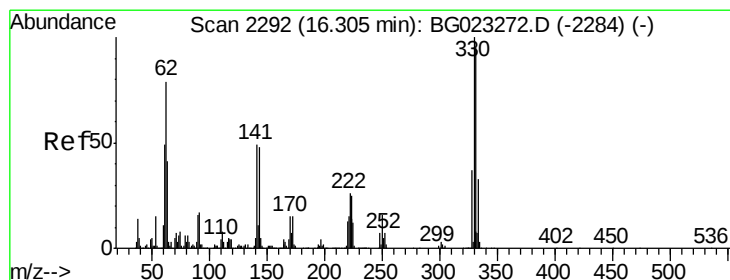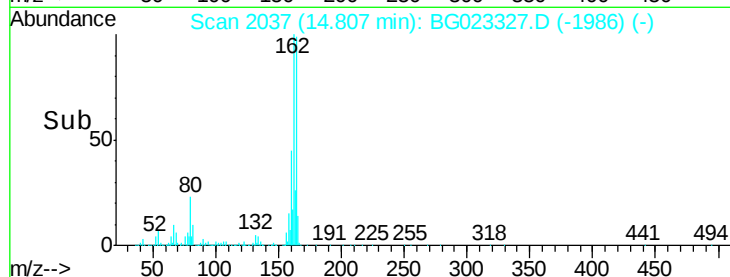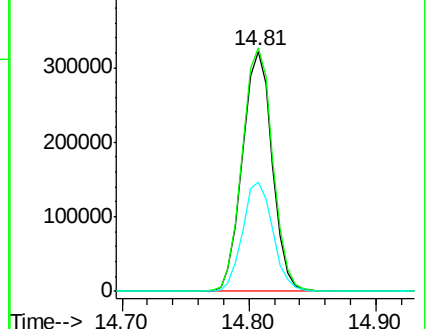

#41

2,4,6-Tribromophenol

Concen: 162.42 ng

RT: 16.31 min Scan# 2292

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45


Tgt Ion:330 Resp: 878907

Ion Ratio Lower Upper

330 100

332 100.3 77.4 116.2



141 39.4 31.7 47.5

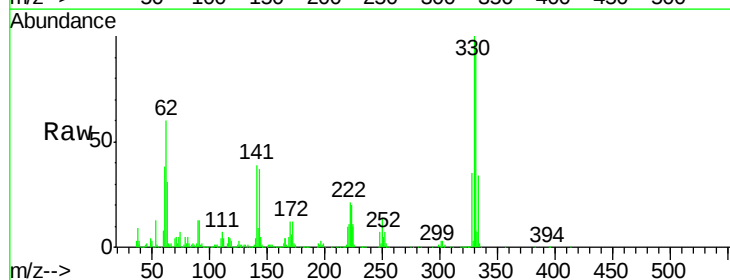


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

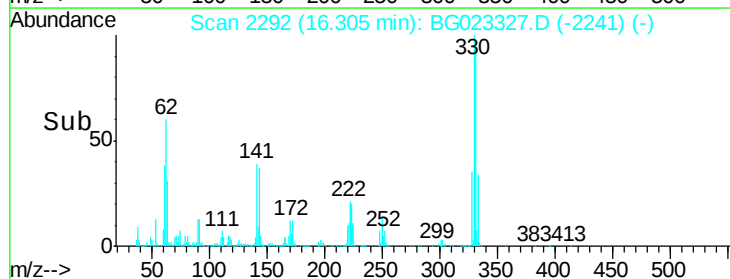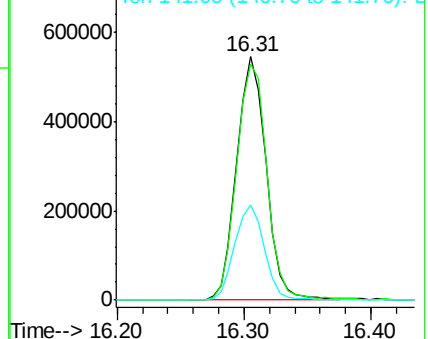



#44

2-Fluorobiphenyl

Concen: 93.52 ng

RT: 13.42 min Scan# 1801

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampleId :

L-1


Tgt Ion:172 Resp: 2612306

Ion Ratio Lower Upper

172 100

171 44.1 31.6 47.4




170 30.3 21.3 31.9

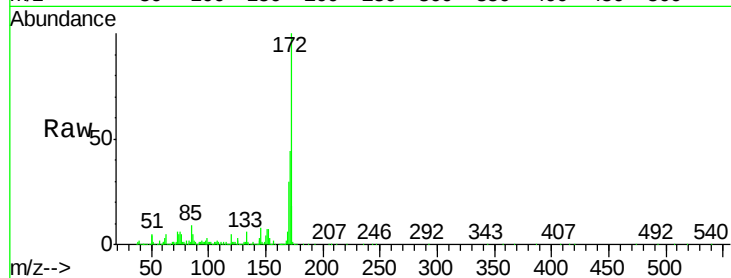

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

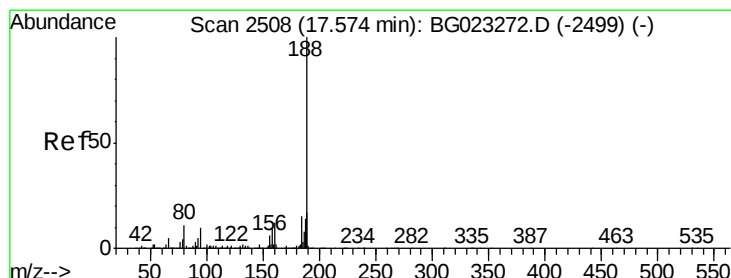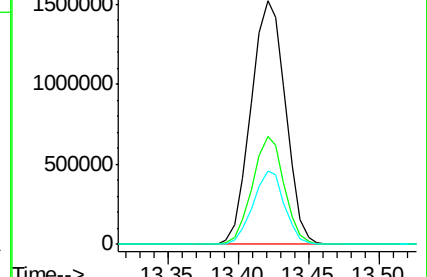

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.57 min Scan# 2507

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45


Tgt Ion:188 Resp: 1216723

Ion Ratio Lower Upper

188 100

94 10.1 5.2 7.8#



80 12.5 7.2 10.8#

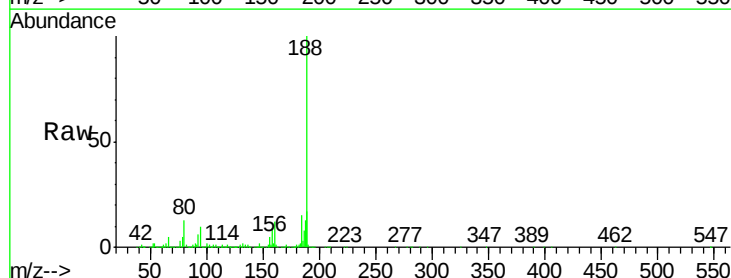


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

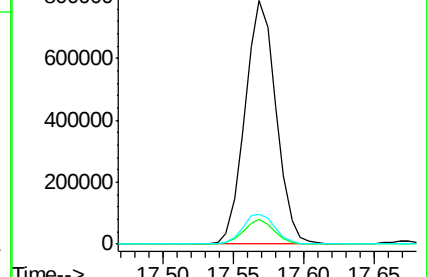

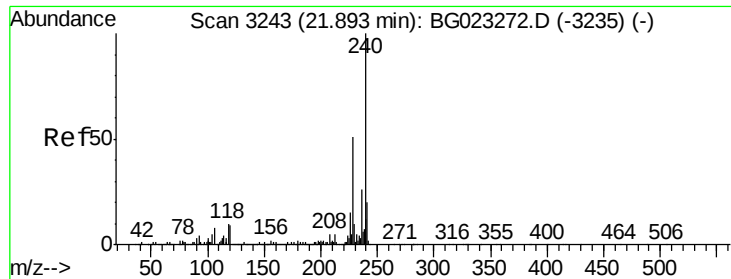

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.89 min Scan# 3243

Delta R.T. 0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampleId :

L-1


Tgt Ion:240 Resp: 1246195

Ion Ratio Lower Upper

240 100

120 10.0 4.1 6.1#




236 26.9 21.1 31.7

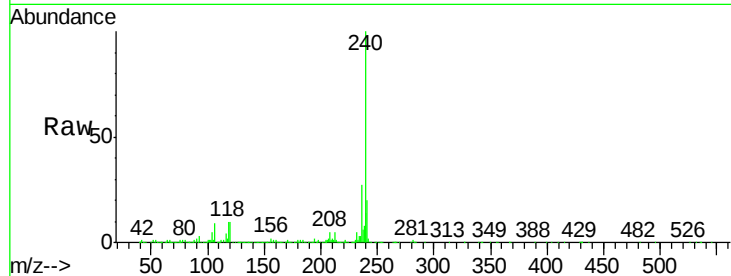

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

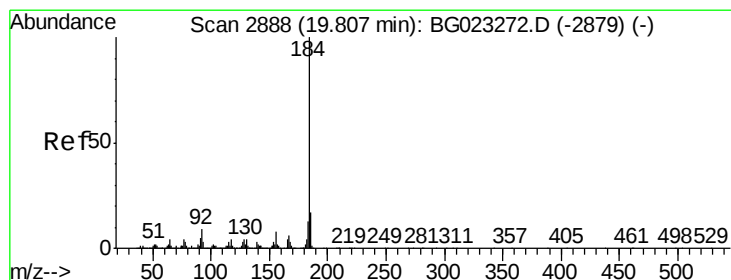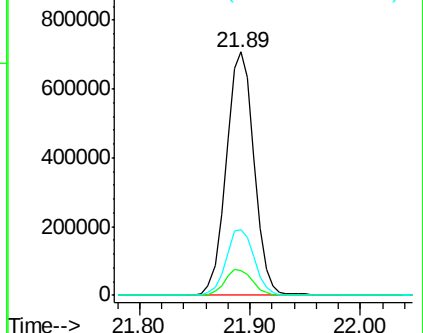

#76

Benzidine

Concen: 7.56 ng

RT: 19.81 min Scan# 2888

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45


Tgt Ion:184 Resp: 265118

Ion Ratio Lower Upper

184 100

185 13.4 12.6 19.0



183 12.4 10.7 16.1

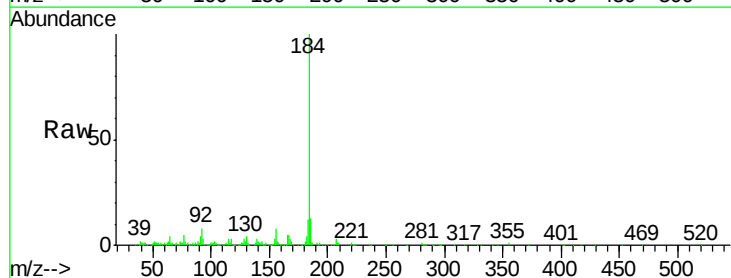


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

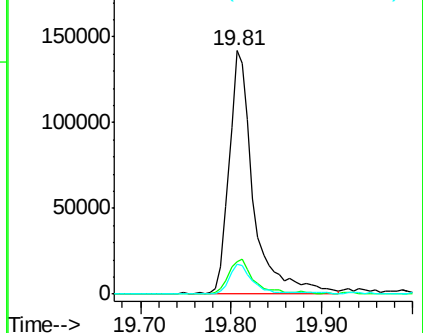

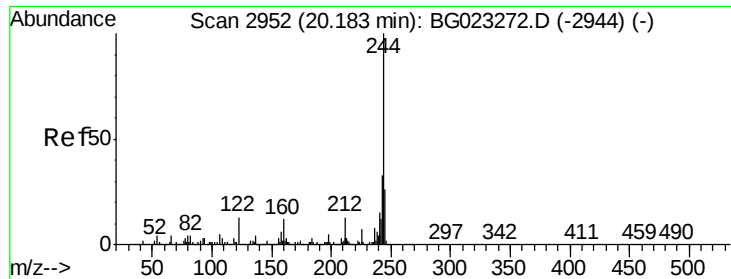

#78

Terphenyl-d14

Concen: 85.08 ng

RT: 20.18 min Scan# 2951

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45

Instrument :

BNA_G

ClientSampled :

L-1


Tgt Ion:244 Resp: 3261524

Ion Ratio Lower Upper

244 100

212 13.7 10.8 16.2




122 16.6 8.0 12.0#

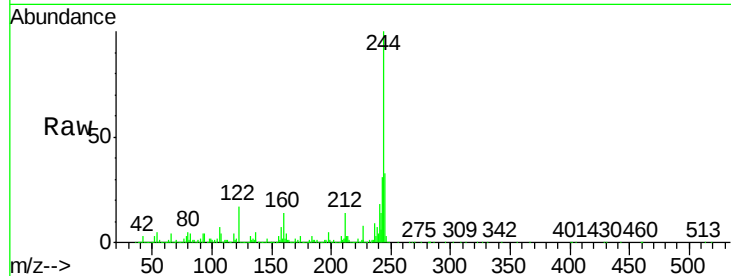

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

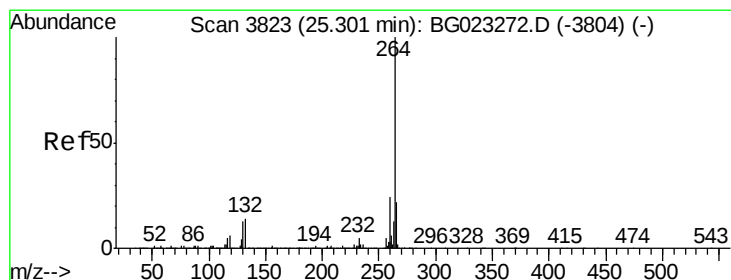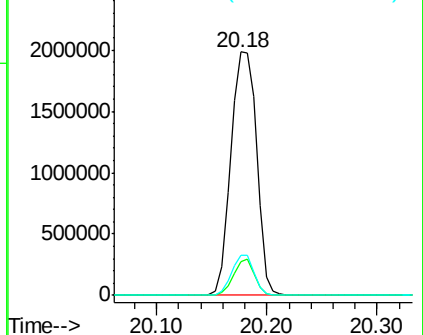

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.30 min Scan# 3823

Delta R.T. -0.00 min

Lab File: BG023327.D

Acq: 29 Jul 2016 5:45


Tgt Ion:264 Resp: 1270163

Ion Ratio Lower Upper

264 100

260 24.9 18.4 27.6

265 22.7 18.9 28.3

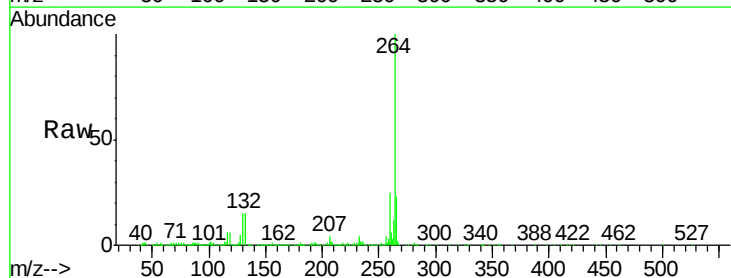

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

