
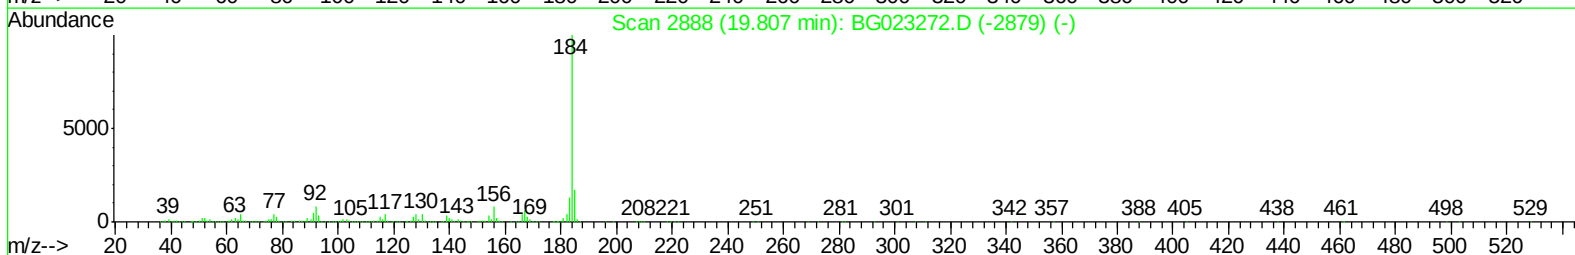
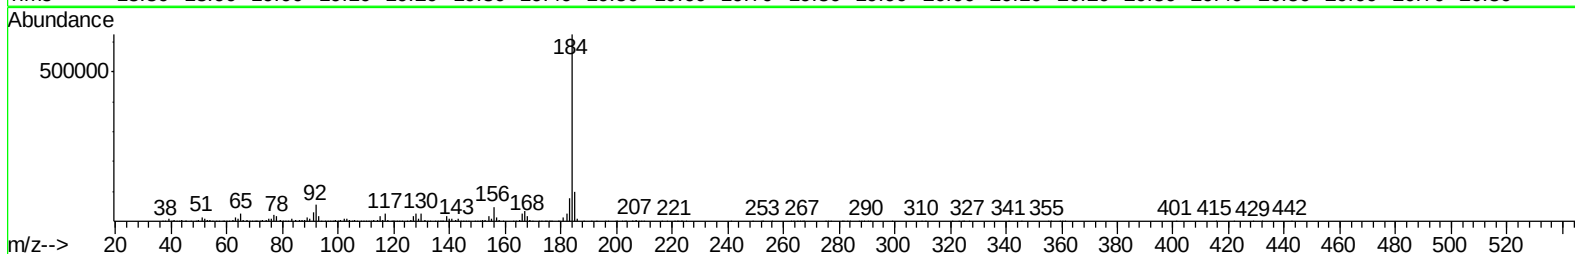


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072916\
Data File : BG023320.D
Acq On : 29 Jul 2016 1:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 08:11:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

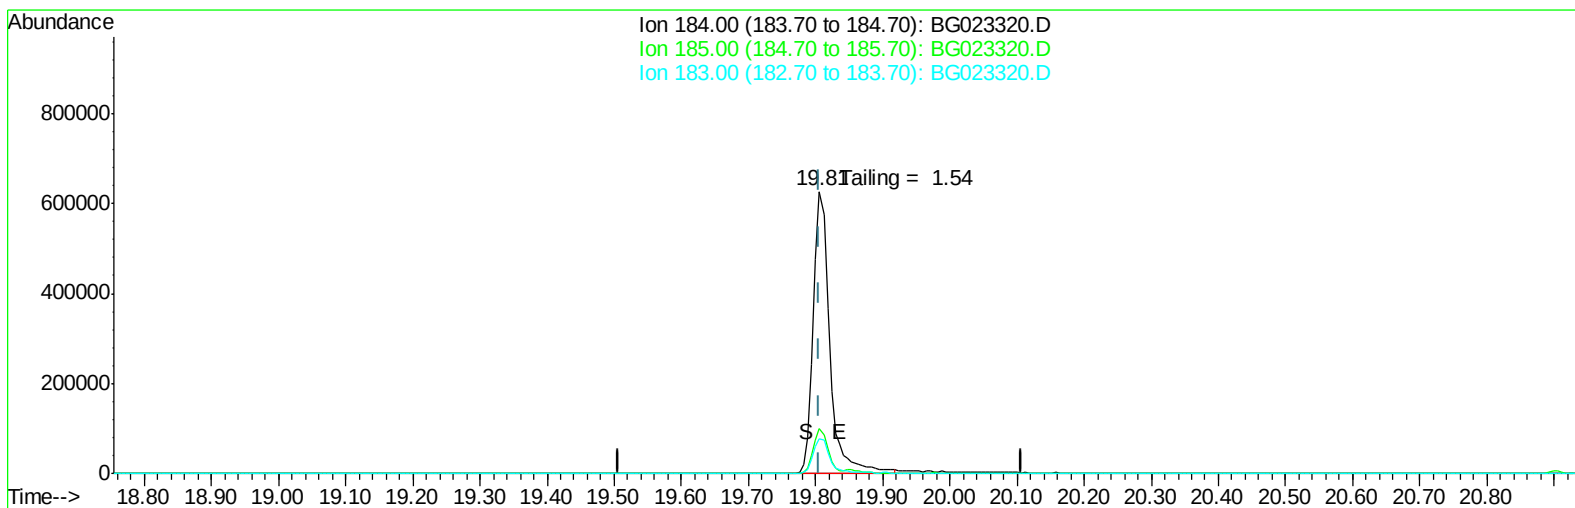

TIC: BG023320.D

(76) Benzidine




19.806min (-0.001) 27866.93ng

response 1048703

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.03
183.00	13.40	12.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072916\
Data File : BG023320.D
Acq On : 29 Jul 2016 1:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 08:11:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

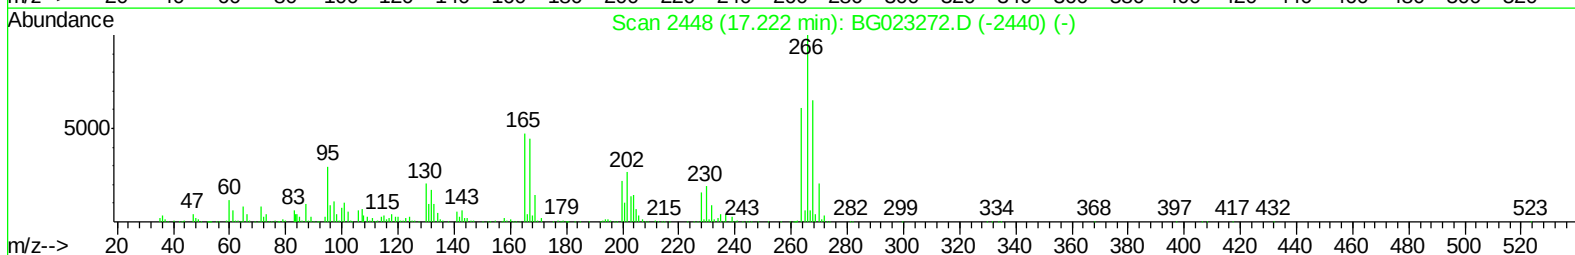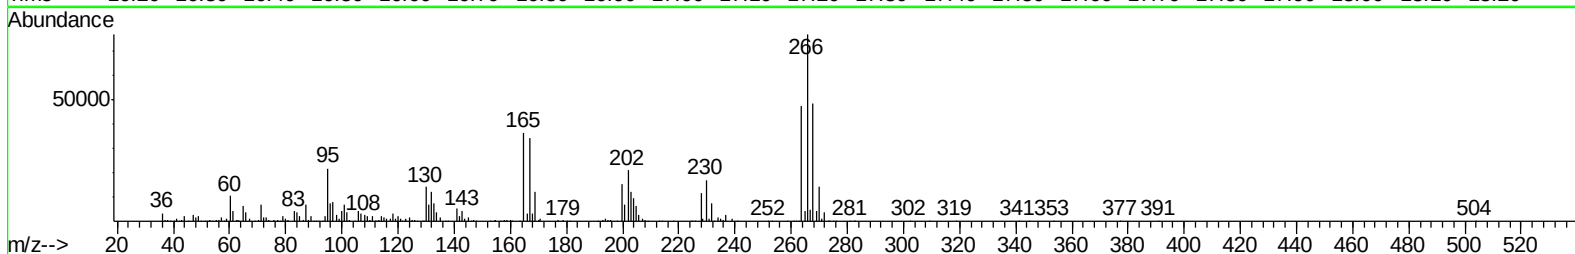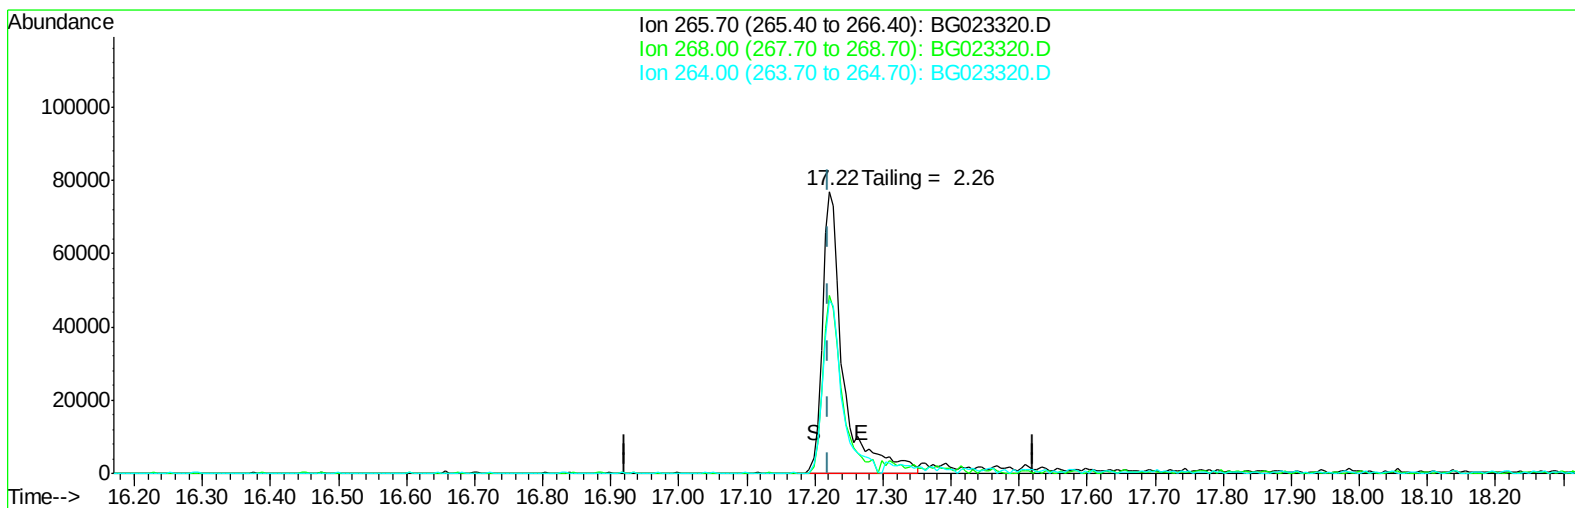

TIC: BG023320.D

(69) Pentachlorophenol (C)

17.221min (+0.000) 40400.77ng

response 160208

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.27
264.00	63.20	61.50
0.00	0.00	0.00