


Data Path : Z:\HPCHEM1\BNA G\Data\BG072916\
 Data File : BG023320.D
 Acq On : 29 Jul 2016 1:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

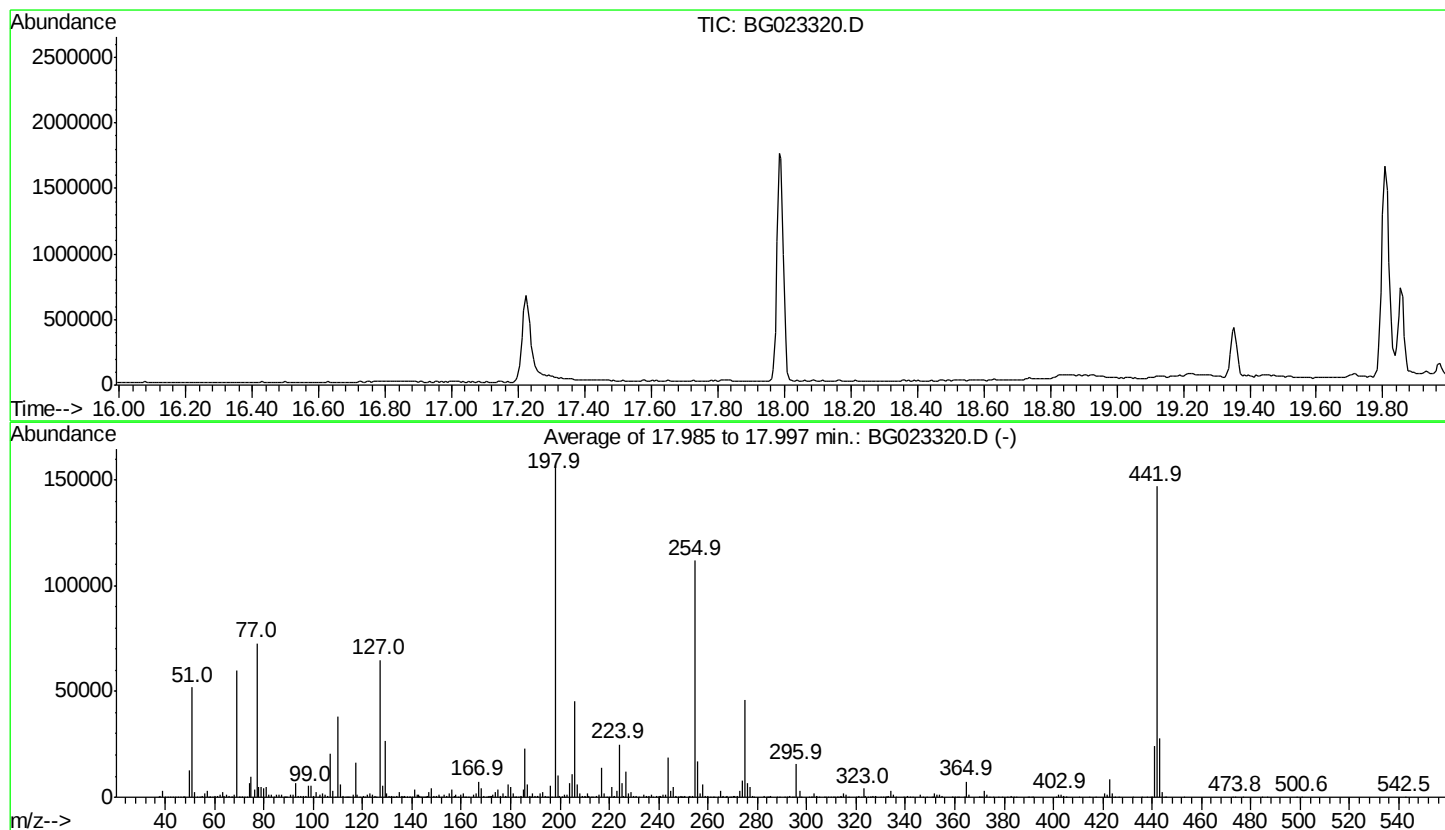

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	51782	PASS
68	69	0.00	2	1.9	1133	PASS
69	198	0.00	100	38.2	59953	PASS
70	69	0.00	2	0.2	121	PASS
127	198	10	80	41.5	65000	PASS
197	198	0.00	2	0.2	250	PASS
198	198	100	100	100.0	156746	PASS
199	198	5	9	6.7	10573	PASS
275	198	10	60	29.3	45901	PASS
365	198	1	100	4.7	7312	PASS
441	442	0.01	24	16.5	24224	PASS
442	198	50	100	93.6	146792	PASS
443	442	15	24	18.9	27762	PASS