
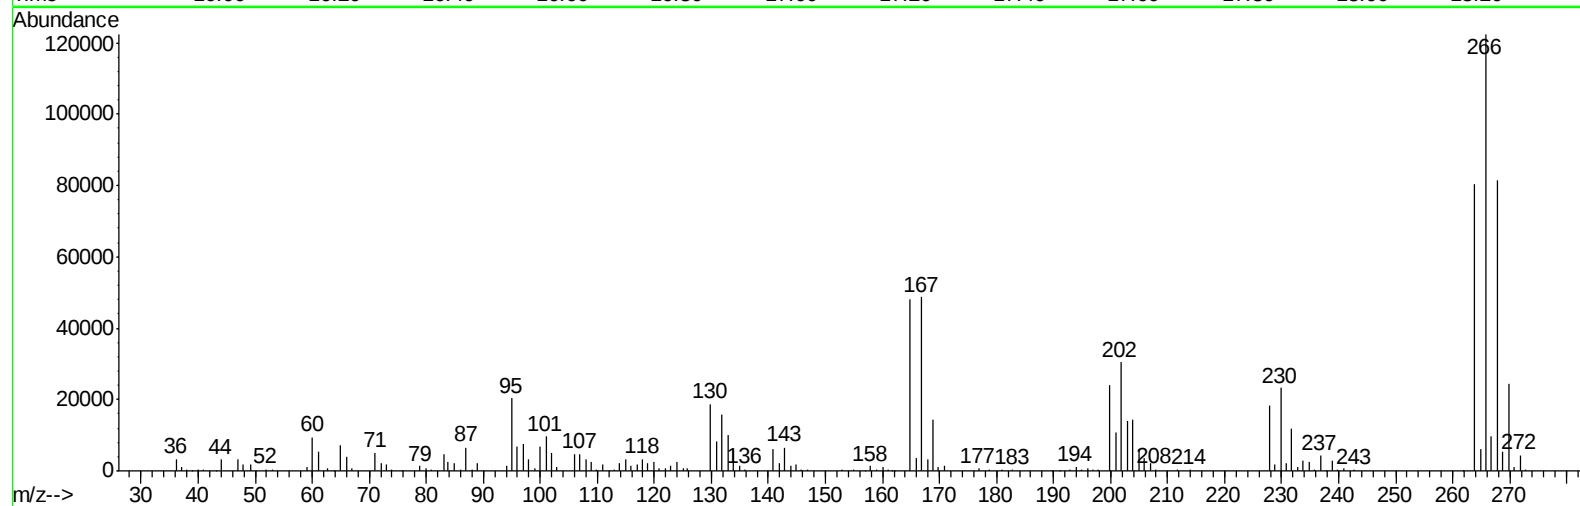


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072919\
Data File : BG041783.D
Acq On : 29 Jul 2019 8:28
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 09:15:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 07:53:52 2019
Response via : Initial Calibration

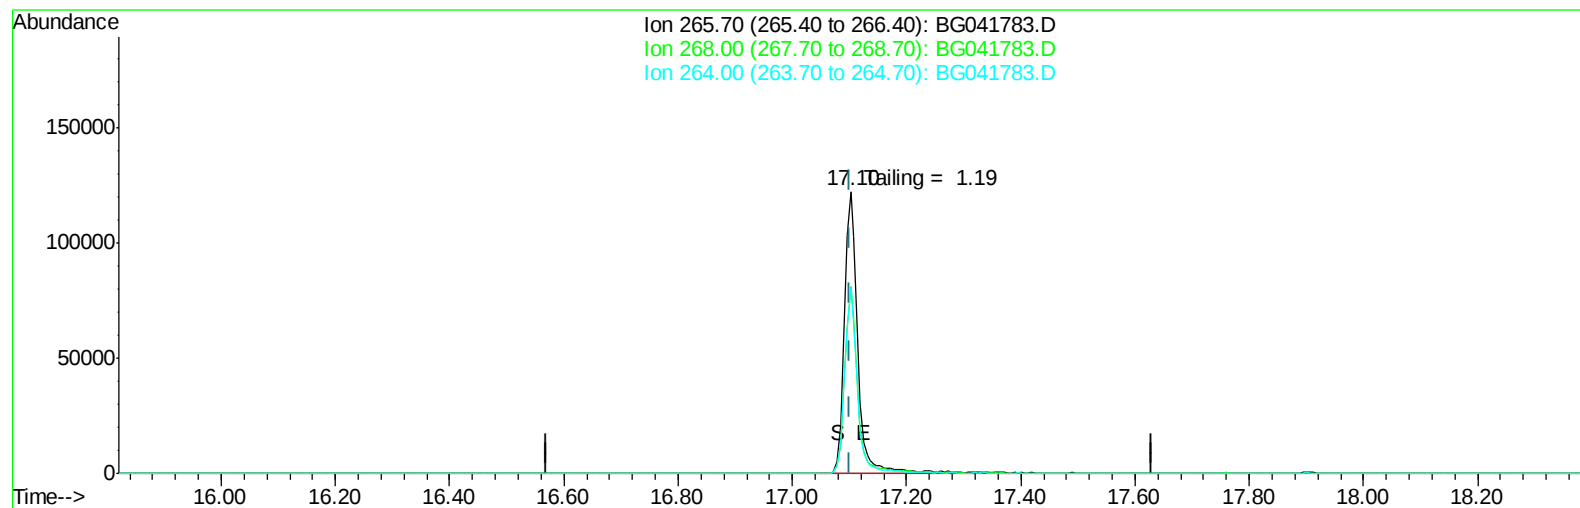

TIC: BG041783.D

(70) Pentachlorophenol (C)



17.102min (+0.001) 68070.45ng

response 196840

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	66.52
264.00	64.30	65.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072919\
Data File : BG041783.D
Acq On : 29 Jul 2019 8:28
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 09:15:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 07:53:52 2019
Response via : Initial Calibration

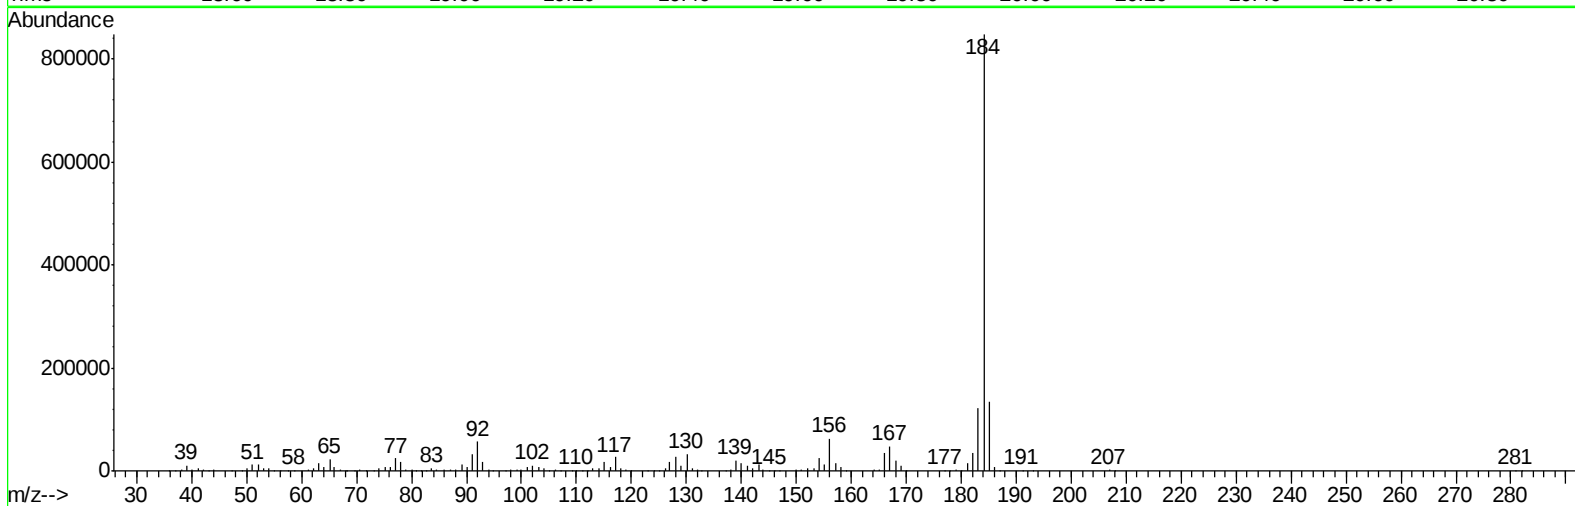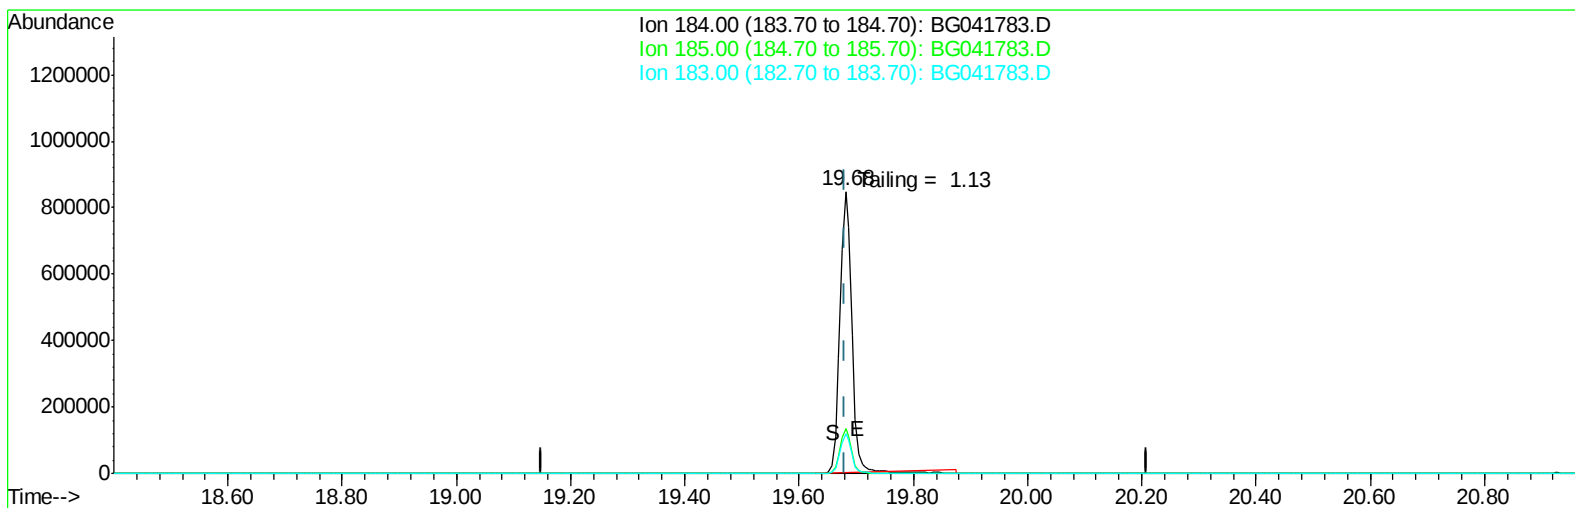

TIC: BG041783.D

(77) Benzidine

19.681min (+0.001) 120589.32ng

response 1243792

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.81
183.00	14.70	14.25
0.00	0.00	0.00