


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072919\
 Data File : BG041783.D
 Acq On : 29 Jul 2019 8:28
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 30 07:53:52 2019

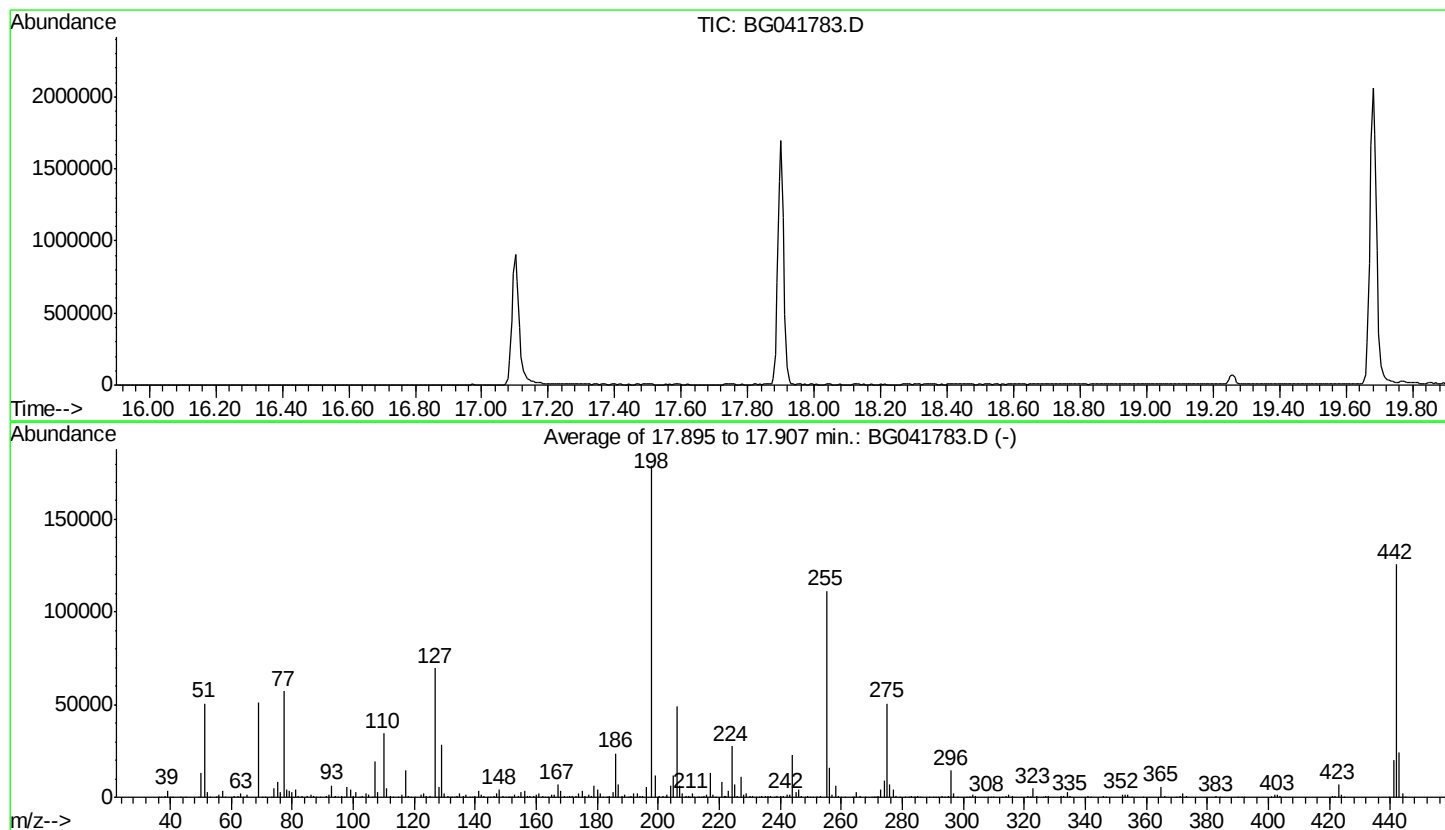

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	50480	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.4	50834	PASS
70	69	0.00	2	0.5	232	PASS
127	198	10	80	39.0	69746	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	178986	PASS
199	198	5	9	6.5	11615	PASS
275	198	10	60	28.2	50533	PASS
365	198	1	100	3.2	5749	PASS
441	198	0.01	100	11.1	19814	PASS
442	198	50	100	70.2	125706	PASS
443	442	15	24	19.3	24229	PASS