

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072921\
 Data File : BG049571.D
 Acq On : 29 Jul 2021 22:49
 Operator : CG/JU
 Sample : M3141-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGEQ9

Quant Time: Jul 30 05:27:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 11:36:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	17753	20.000	ng/ul	0.00
20) Naphthalene-d8	10.866	136	74167	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.696	164	57489	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	138083	20.000	ng/ul	0.00
79) Chrysene-d12	21.728	240	129688	20.000	ng/ul	0.00
88) Perylene-d12	25.006	264	130587	20.000	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.429	96	1090	2.809	ng/uL	0.00
4) Pyridine-d5	3.858	84	13237	11.877	ng/ul	0.00
7) Phenol-d5	7.201	99	34564	22.005	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.371	67	19650	22.089	ng/ul	0.00
11) 2-Chlorophenol-d4	7.577	132	25640	22.773	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	26014	21.973	ng/ul	0.00
21) Nitrobenzene-d5	9.215	128	12175	21.351	ng/ul	0.00
24) 2-Nitrophenol-d4	9.944	143	15283	22.872	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.484	165	26950	22.176	ng/ul	0.00
31) 4-Chloroaniline-d4	11.001	131	31378	18.526	ng/ul	0.00
46) Dimethylphthalate-d6	14.091	166	98875	22.453	ng/ul	0.00
49) Acenaphthylene-d8	14.391	160	115297	22.542	ng/ul	0.00
54) 4-Nitrophenol-d4	14.896	143	12444	17.159	ng/ul	0.00
60) Fluorene-d10	15.689	176	88583	23.349	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.807	200	12238	14.302	ng/ul	0.00
73) Anthracene-d10	17.545	188	144360	22.494	ng/ul	0.00
81) Pyrene-d10	19.836	212	154411	23.285	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.777	264	123889	18.050	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.230	94	3402	2.217	ng/ul#	83
86) Bis(2-ethylhexyl)phtha...	21.605	149	7111	1.539	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072921\
Data File : BG049571.D
Acq On : 29 Jul 2021 22:49
Operator : CG/JU
Sample : M3141-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGEQ9

Quant Time: Jul 30 05:27:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 11:36:47 2021
Response via : Initial Calibration




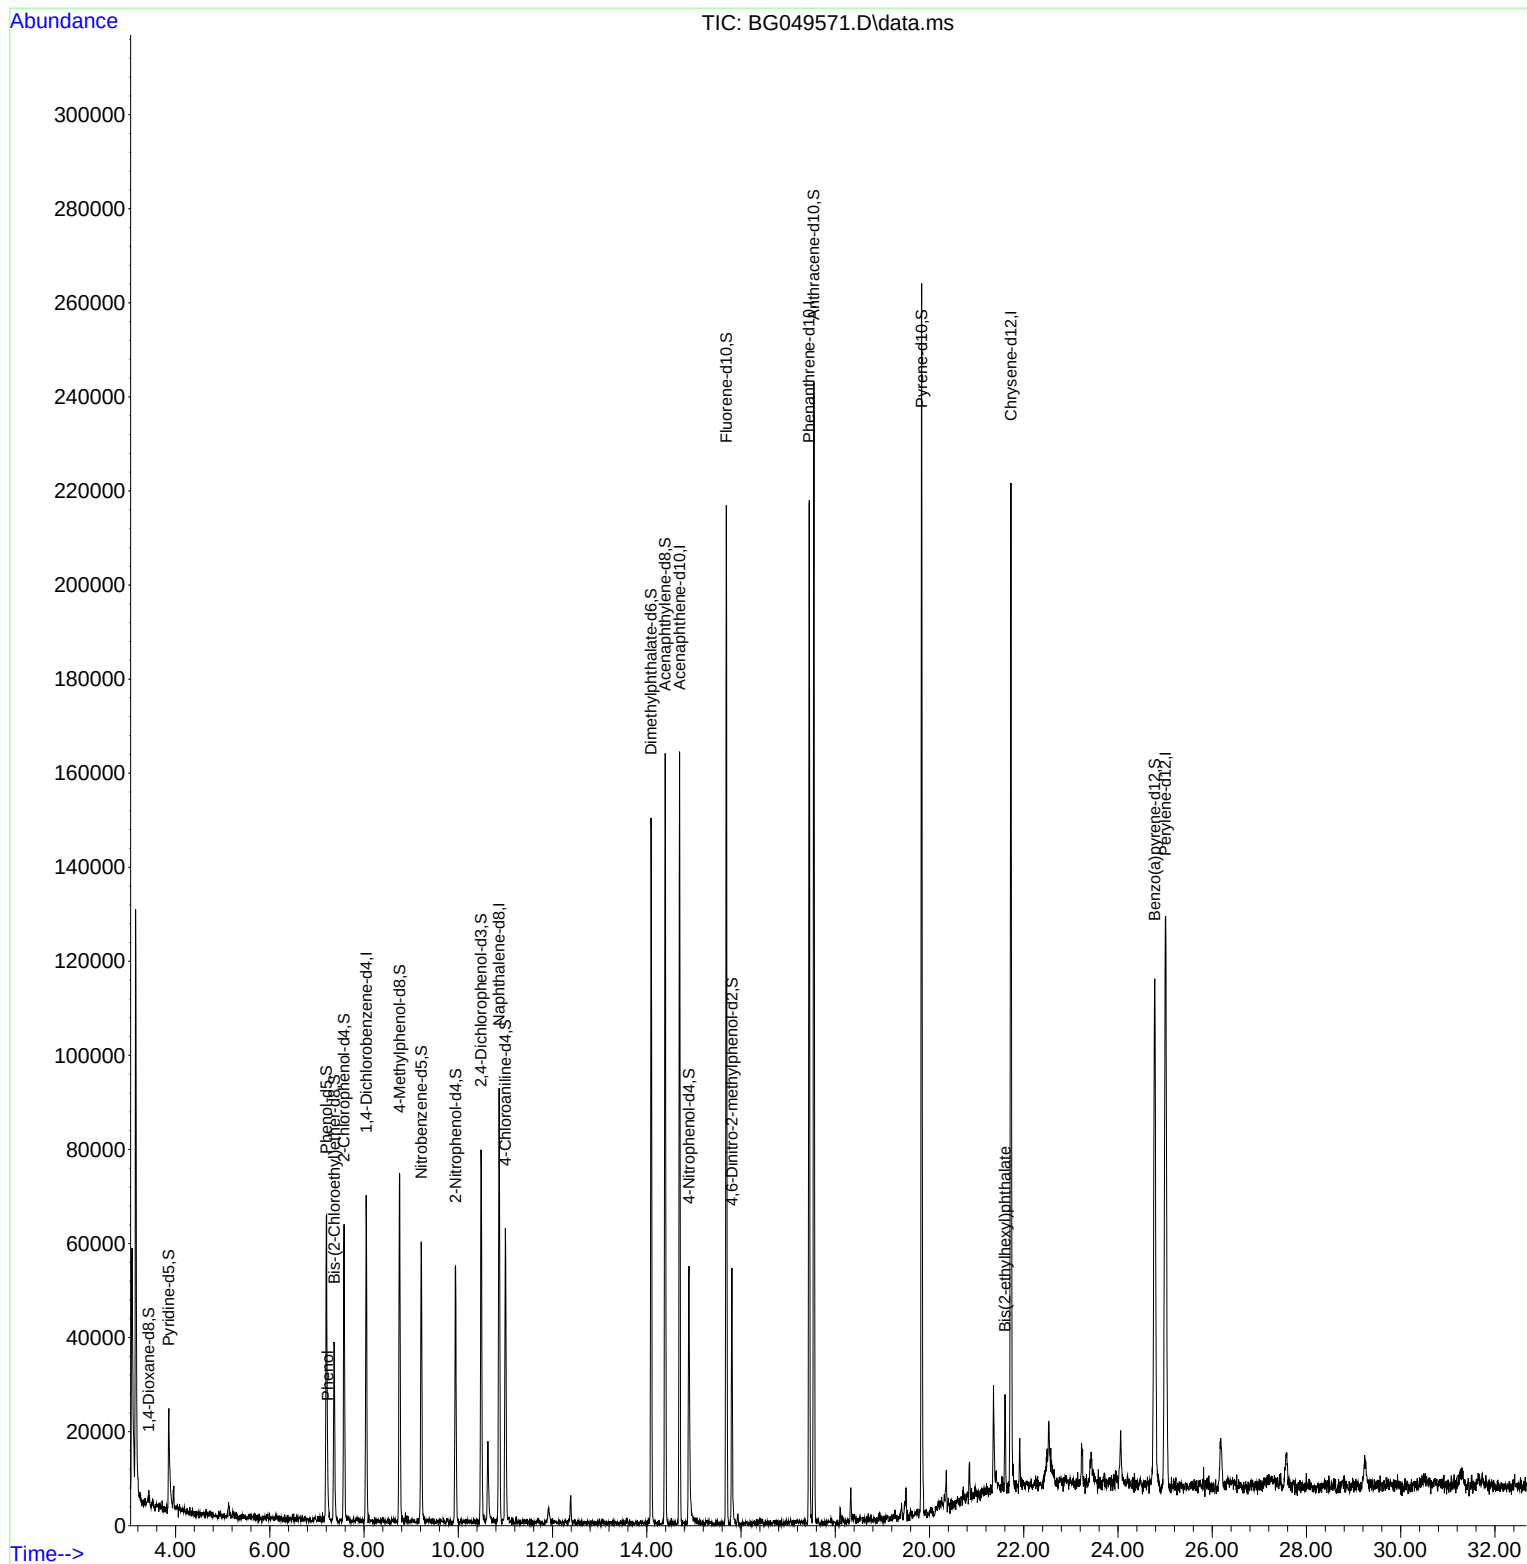


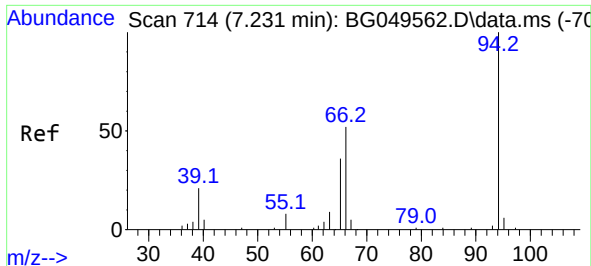

#8
Phenol
Concen: 2.217 ng/ul
RT: 7.230 min Scan# 713
Delta R.T. 0.003 min
Lab File: BG049571.D
Acq: 29 Jul 2021 22:49

Instrument :
BNA_G
ClientSampled :
BGEQ9

Tgt Ion: 94 Resp: 3402
Ion Ratio Lower Upper
94 100
65 34.9 28.8 43.2
66 69.2 40.3 60.5#

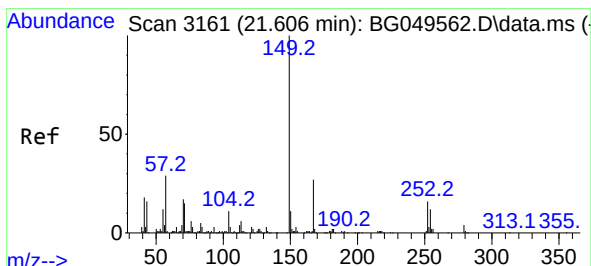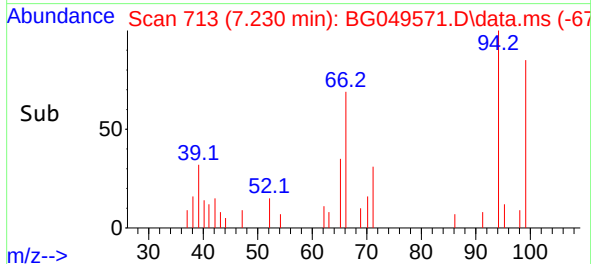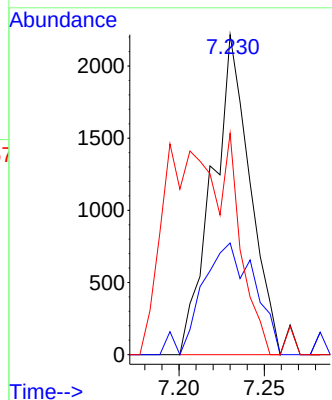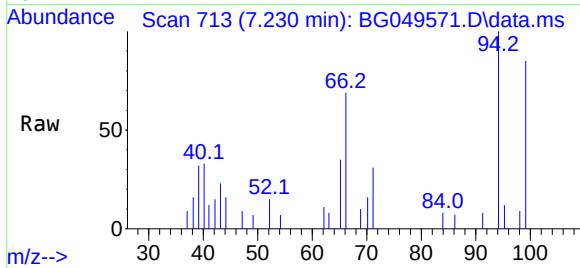

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.539 ng/ul
RT: 21.605 min Scan# 3160
Delta R.T. 0.003 min
Lab File: BG049571.D
Acq: 29 Jul 2021 22:49

Tgt Ion: 149 Resp: 7111
Ion Ratio Lower Upper
149 100
167 26.8 20.9 31.3
279 5.1 3.6 5.4

