
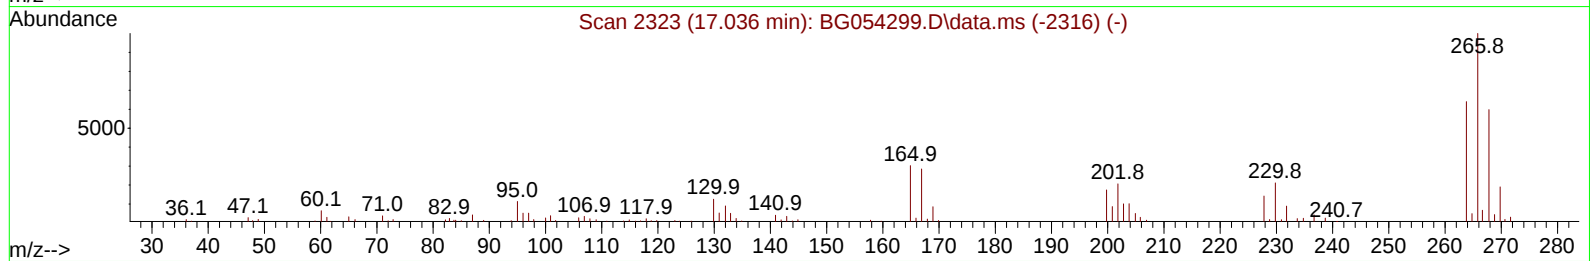
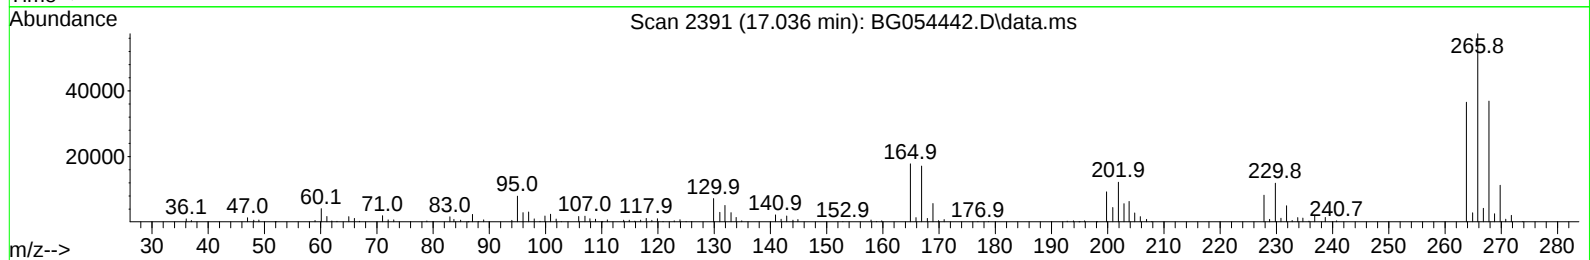


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054442.D
Acq On : 29 Jul 2022 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 09:44:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

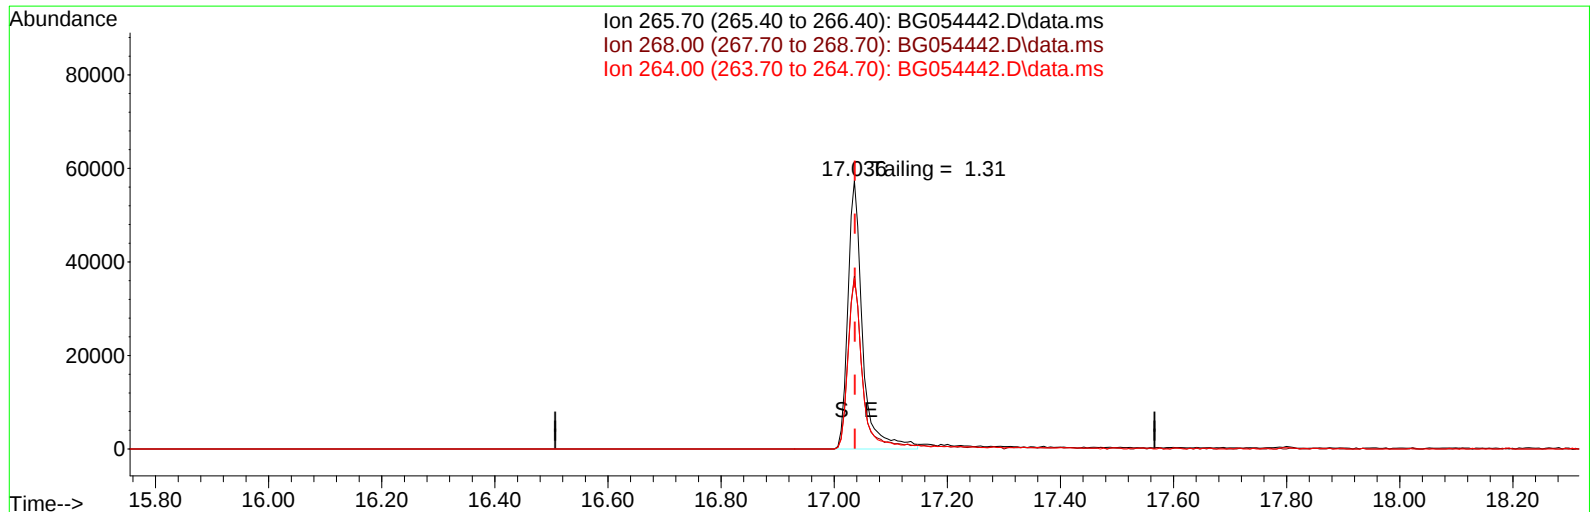

TIC: BG054442.D\data.ms

(70) Pentachlorophenol (C)




17.036min (-0.001) 19757.93 ng

response 103564

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.28
264.00	66.20	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054442.D
Acq On : 29 Jul 2022 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 09:44:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

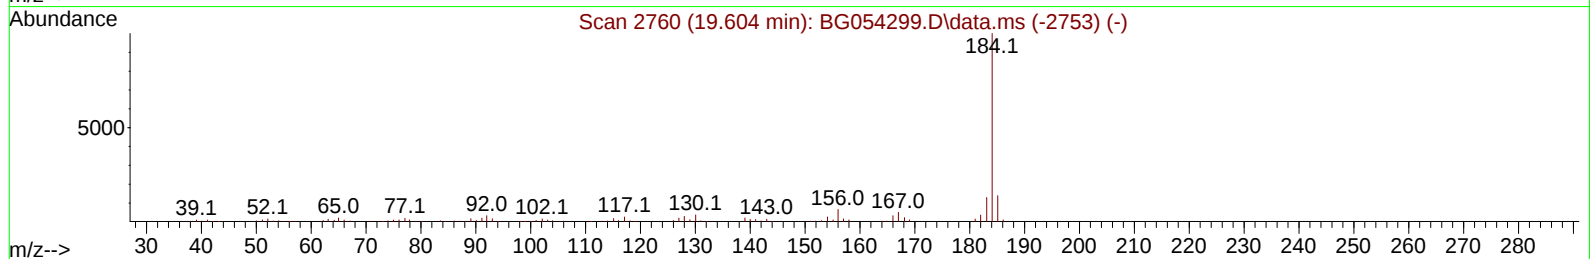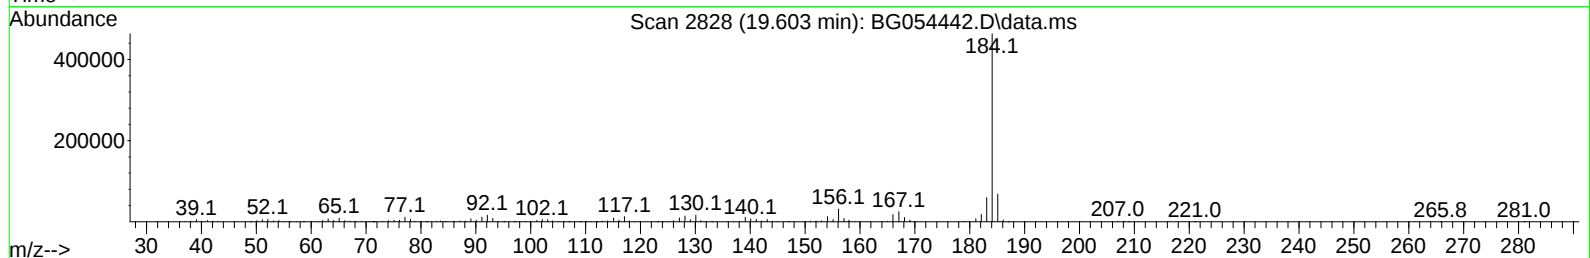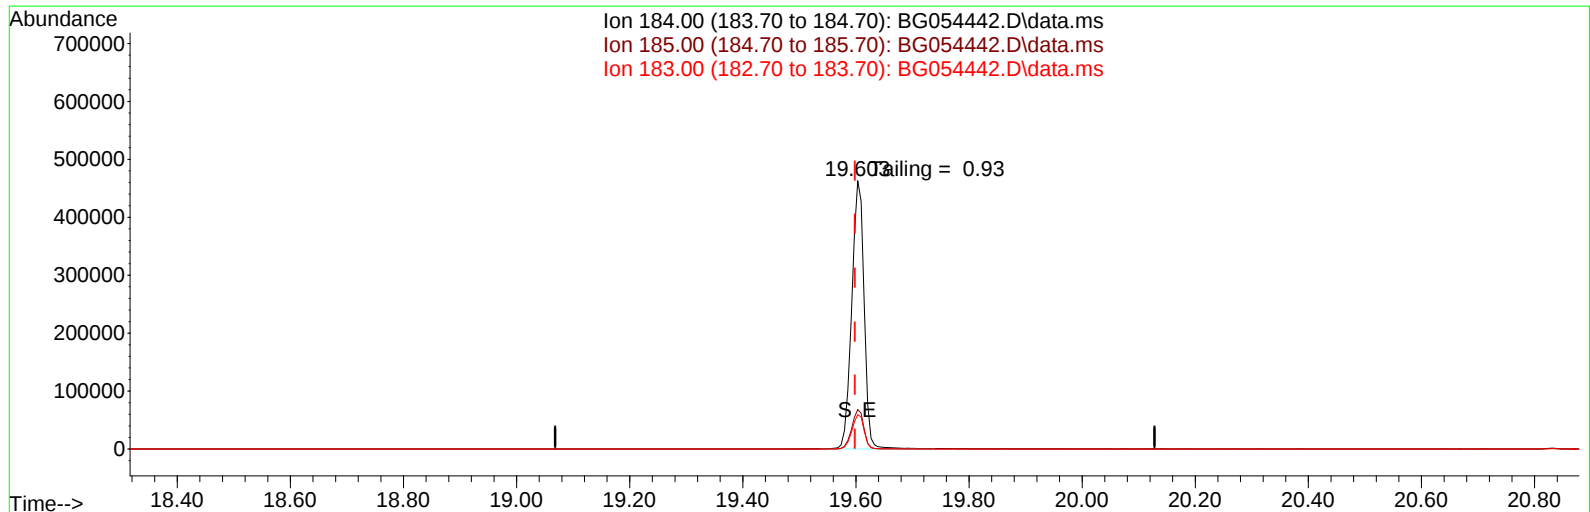

TIC: BG054442.D\data.ms

(77) Benzidine**19.603min (+ 0.005) 549844.35 ng****response 707025**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.77
183.00	11.10	12.84
0.00	0.00	0.00