

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
 Data File : BG054445.D
 Acq On : 29 Jul 2022 12:02
 Operator : CG/JU
 Sample : N3895-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RVE-47

Quant Time: Jul 30 03:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	15915	20.000	ng	0.00
21) Naphthalene-d8	10.794	136	55283	20.000	ng	# 0.00
39) Acenaphthene-d10	14.619	164	45054	20.000	ng	0.00
64) Phenanthrene-d10	17.369	188	124060	20.000	ng	# 0.00
76) Chrysene-d12	21.634	240	147339	20.000	ng	# 0.00
86) Perylene-d12	24.836	264	158720	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.565	112	94125	123.482	ng	0.00
7) Phenol-d6	7.175	99	124357	119.061	ng	0.00
23) Nitrobenzene-d5	9.149	82	79044	77.863	ng	0.00
42) 2,4,6-Tribromophenol	16.117	330	124038	131.123	ng	0.00
45) 2-Fluorobiphenyl	13.244	172	232037	72.654	ng	0.00
79) Terphenyl-d14	19.977	244	568453	76.538	ng	0.00
Target Compounds						
						Qvalue
75) Fluoranthene	19.425	202	29227	3.470	ng	97
78) Pyrene	19.783	202	27019	3.196	ng	95
88) Benzo(b)fluoranthene	23.826	252	27828	2.965	ng	98
90) Benzo(a)pyrene	24.684	252	17560	2.191	ng	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054445.D
Acq On : 29 Jul 2022 12:02
Operator : CG/JU
Sample : N3895-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RVE-47

Quant Time: Jul 30 03:17:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration




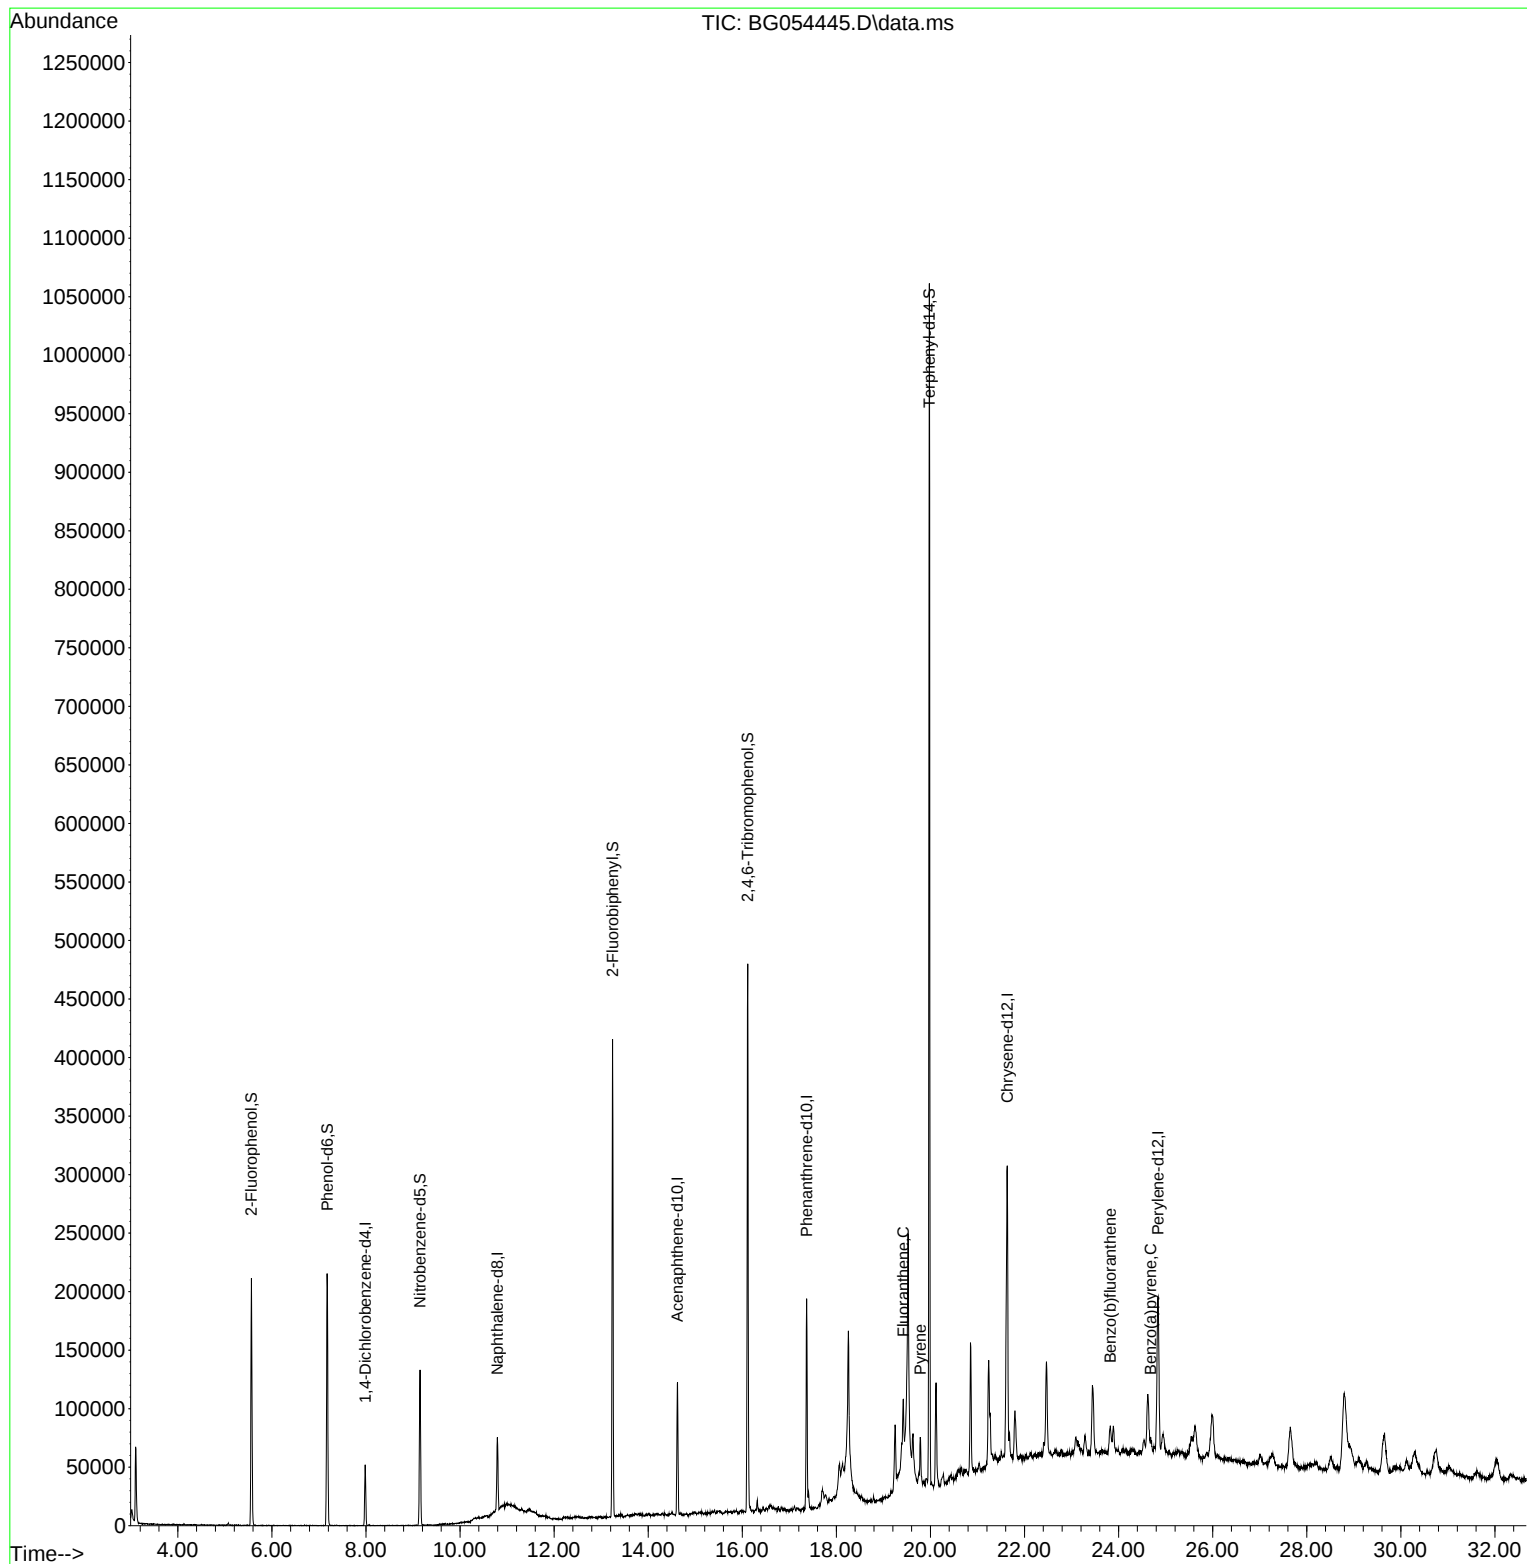




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.985 min Scan# 81
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02




Instrument :
BNA_G
ClientSampleId :
RVE-47


Tgt Ion:152 Resp: 15915
Ion Ratio Lower Upper
152 100
150 148.0 131.6 197.4
115 52.2 50.9 76.3

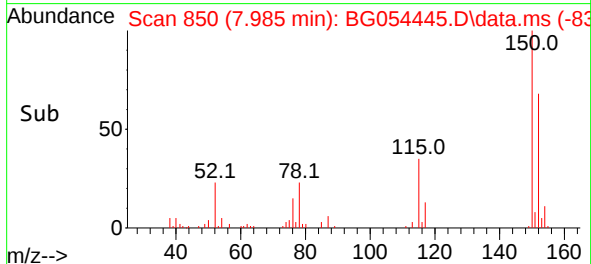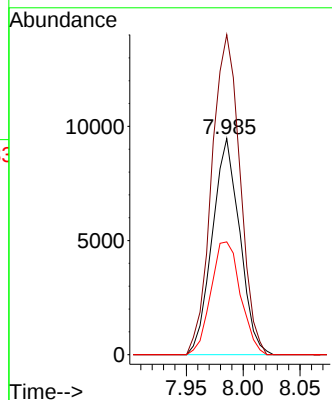

#5
2-Fluorophenol
Concen: 123.482 ng
RT: 5.565 min Scan# 438
Delta R.T. 0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02

Tgt Ion:112 Resp: 94125
Ion Ratio Lower Upper
112 100
64 61.6 55.1 82.7
63 35.3 30.4 45.6


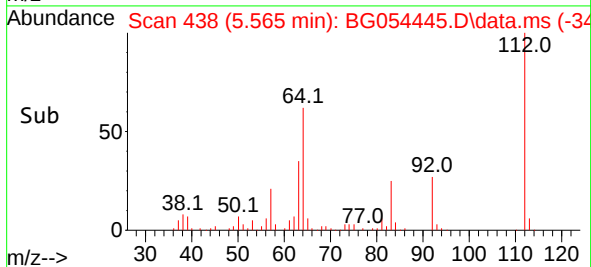
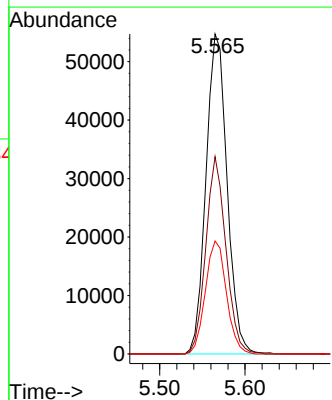
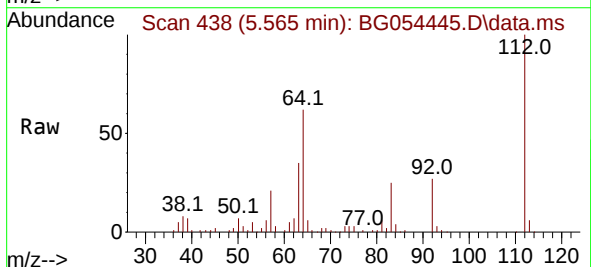




#7
Phenol-d6
Concen: 119.061 ng
RT: 7.175 min Scan# 71
Delta R.T. 0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02




Instrument :
BNA_G
ClientSampleId :
RVE-47


Tgt Ion: 99 Resp: 124357
Ion Ratio Lower Upper
99 100
42 20.6 17.0 25.6
71 44.0 33.8 50.8

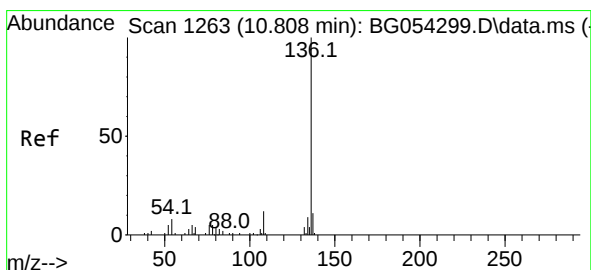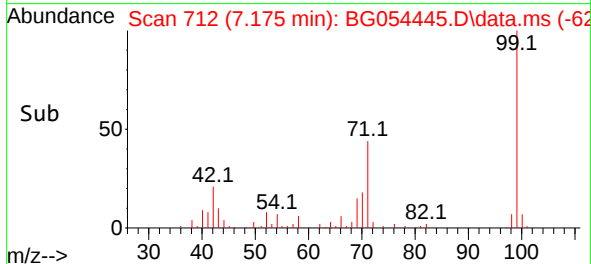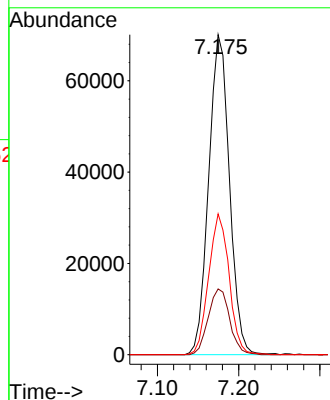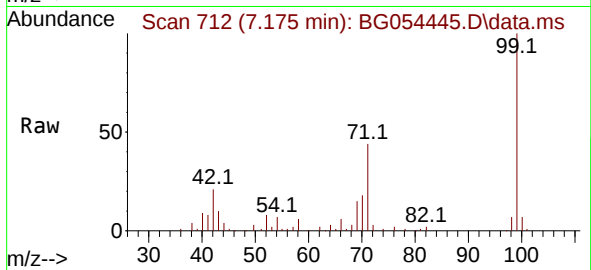

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.794 min Scan# 1328
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02

Tgt Ion: 136 Resp: 55283
Ion Ratio Lower Upper
136 100
137 9.4 8.5 12.7
54 6.7 7.4 11.2#
68 4.5 4.9 7.3#


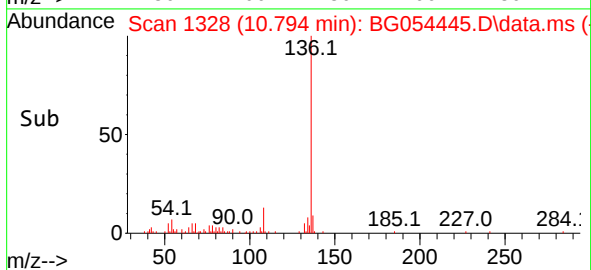
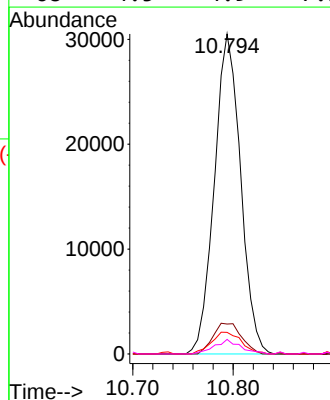
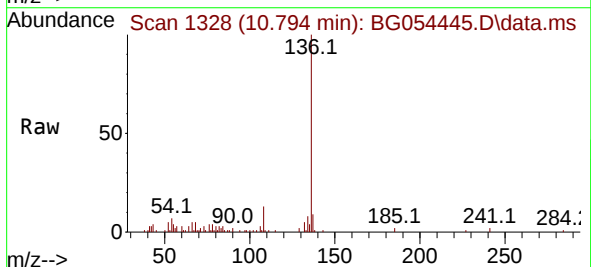




#23
Nitrobenzene-d5
Concen: 77.863 ng
RT: 9.149 min Scan# 1
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02




Instrument :
BNA_G
ClientSampleId :
RVE-47


Tgt Ion: 82 Resp: 79044
Ion Ratio Lower Upper
82 100
128 42.2 27.9 41.9#
54 54.8 41.2 61.8

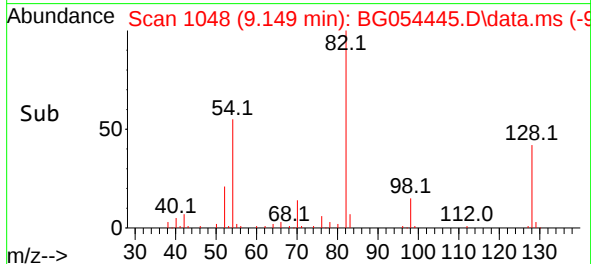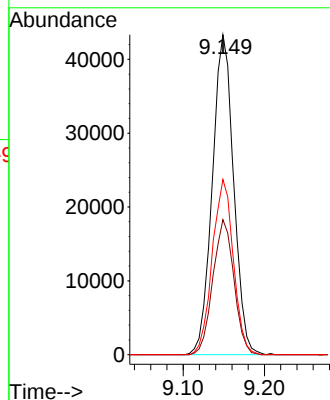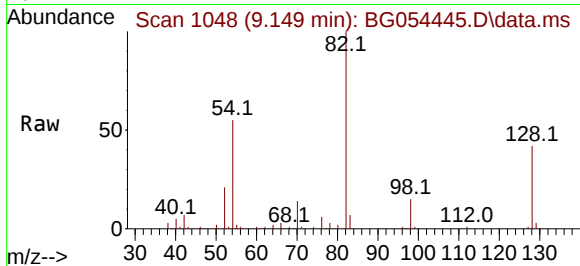

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.619 min Scan# 1979
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02

Tgt Ion: 164 Resp: 45054
Ion Ratio Lower Upper
164 100
162 105.9 82.3 123.5
160 42.6 34.2 51.2


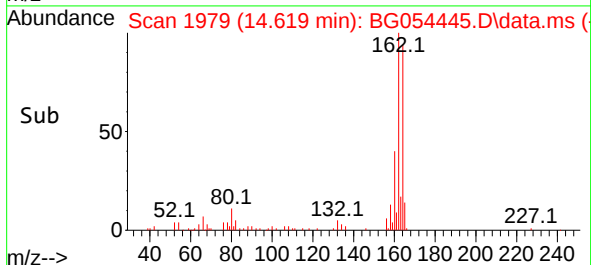
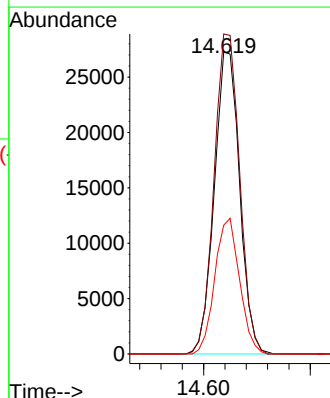
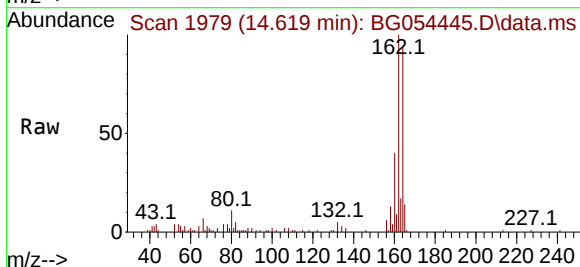




#42
 2,4,6-Tribromophenol
 Concen: 131.123 ng
 RT: 16.117 min Scan# 2168
 Delta R.T. 0.003 min
 Lab File: BG054445.D
 Acq: 29 Jul 2022 12:02




Instrument :
 BNA_G
 ClientSampleId :
 RVE-47


Tgt Ion:330 Resp: 124038
 Ion Ratio Lower Upper
 330 100
 332 97.1 76.0 114.0
 141 20.3 27.1 40.7#

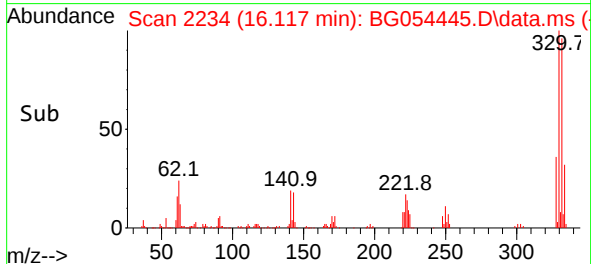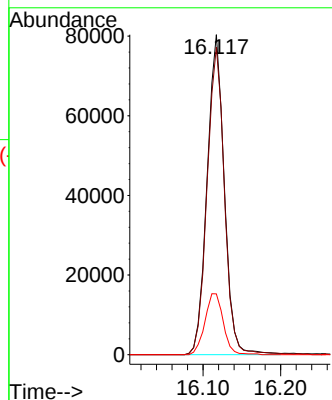

#45
 2-Fluorobiphenyl
 Concen: 72.654 ng
 RT: 13.244 min Scan# 1745
 Delta R.T. -0.003 min
 Lab File: BG054445.D
 Acq: 29 Jul 2022 12:02

Tgt Ion:172 Resp: 232037
 Ion Ratio Lower Upper
 172 100
 171 36.4 28.5 42.7
 170 23.6 18.9 28.3


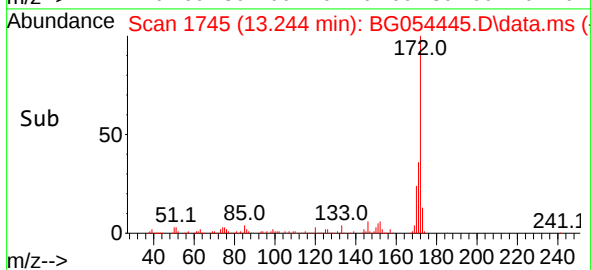
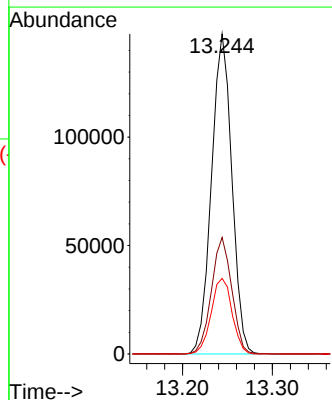
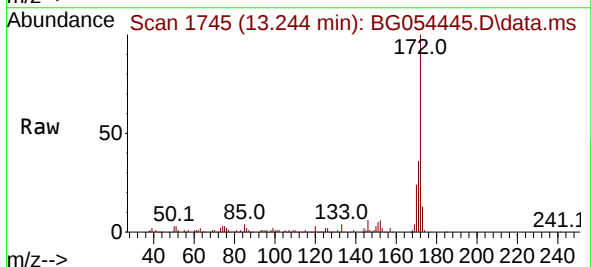




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.369 min Scan# 241
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02




Instrument :
BNA_G
ClientSampleId :
RVE-47


Tgt Ion:188 Resp: 124060
Ion Ratio Lower Upper
188 100
94 4.0 5.4 8.0#
80 4.5 6.8 10.2#

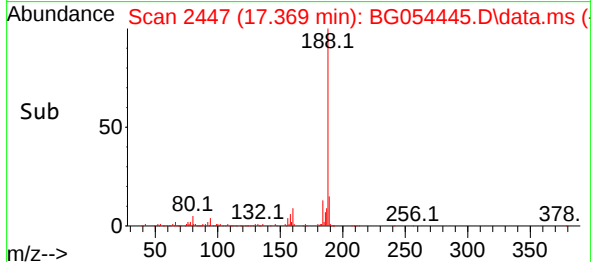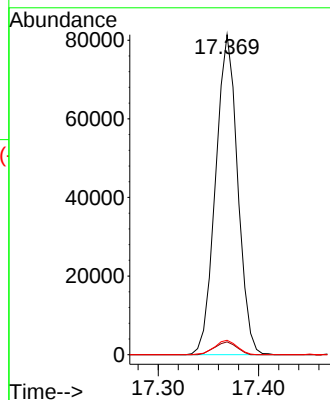

#75
Fluoranthene
Concen: 3.470 ng
RT: 19.425 min Scan# 2797
Delta R.T. 0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02

Tgt Ion:202 Resp: 29227
Ion Ratio Lower Upper
202 100
101 5.2 0.0 26.9
203 18.2 0.0 37.2


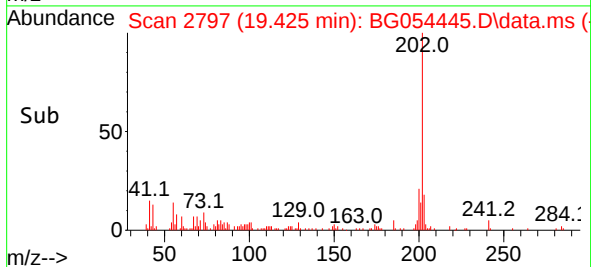
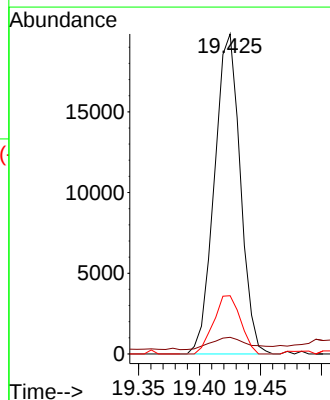
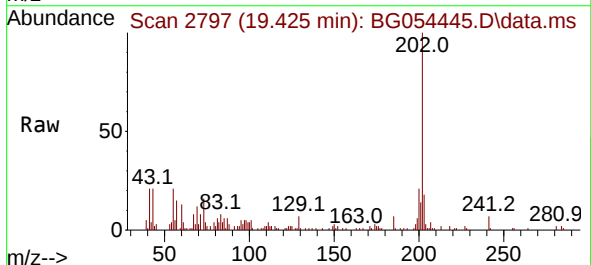




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.634 min Scan# 31
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02




Instrument :
BNA_G
ClientSampleId :
RVE-47


Tgt Ion:240 Resp: 147339
Ion Ratio Lower Upper
240 100
120 3.4 4.6 7.0#
236 25.9 20.2 30.4

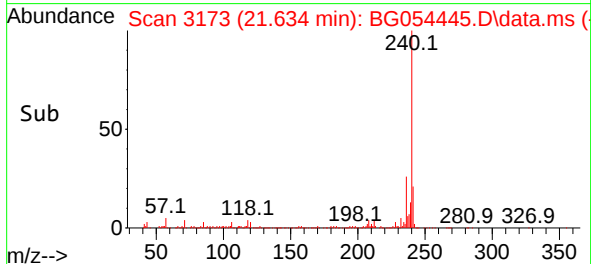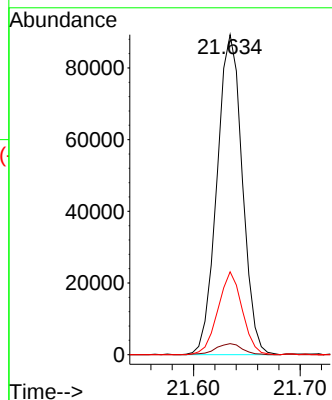

#78
Pyrene
Concen: 3.196 ng
RT: 19.783 min Scan# 2858
Delta R.T. -0.003 min
Lab File: BG054445.D
Acq: 29 Jul 2022 12:02

Tgt Ion:202 Resp: 27019
Ion Ratio Lower Upper
202 100
200 23.5 16.6 24.8
203 19.6 14.6 21.8


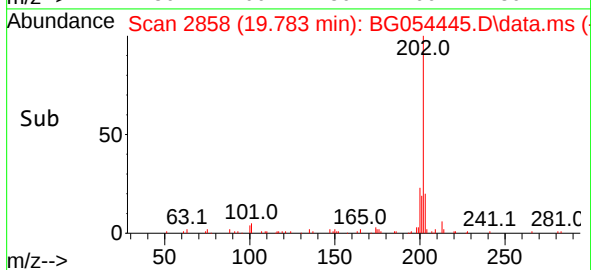
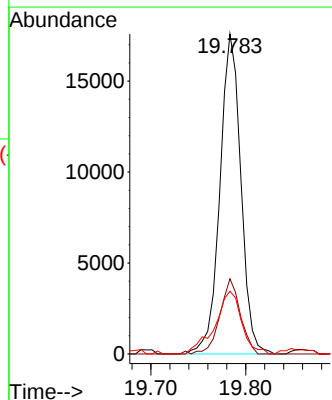
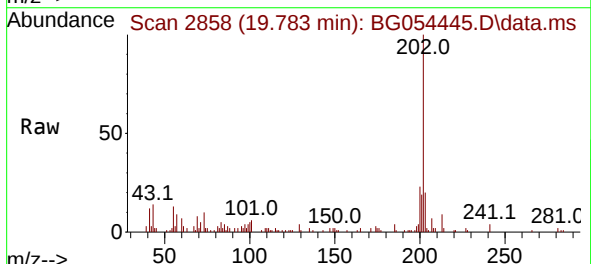




#79
 Terphenyl-d14
 Concen: 76.538 ng
 RT: 19.977 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG054445.D
 Acq: 29 Jul 2022 12:02




Instrument :
 BNA_G
 ClientSampleId :
 RVE-47


Tgt Ion:244 Resp: 568453
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.5 9.7
 122 4.3 5.0 7.4#

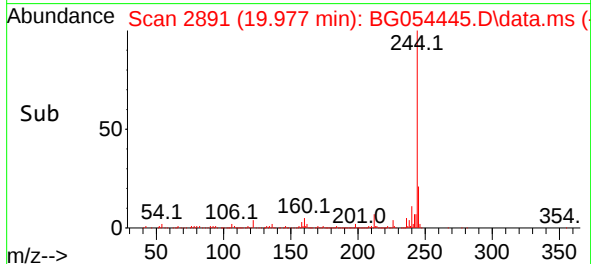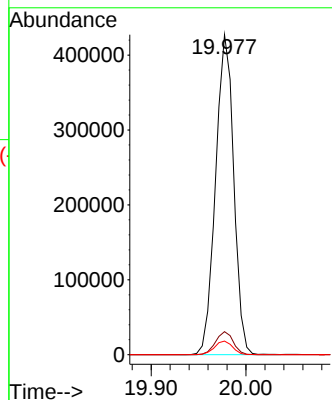

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.836 min Scan# 3718
 Delta R.T. 0.003 min
 Lab File: BG054445.D
 Acq: 29 Jul 2022 12:02

Tgt Ion:264 Resp: 158720
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.0 28.6
 265 22.8 17.4 26.2

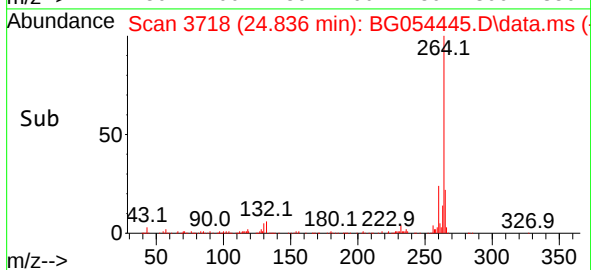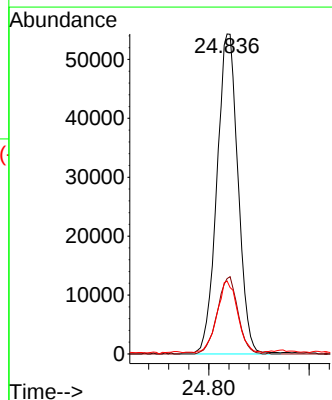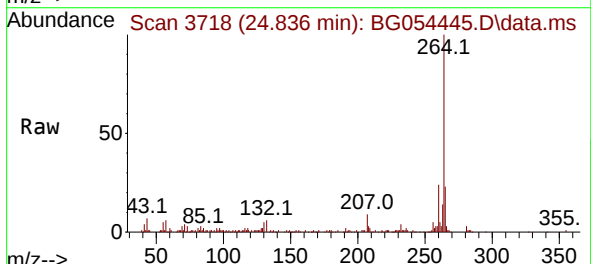



#88

Benzo(b)fluoranthene

Concen: 2.965 ng

RT: 23.826 min Scan# 31

Delta R.T. 0.003 min

Lab File: BG054445.D

Acq: 29 Jul 2022 12:02

Instrument :

BNA_G

ClientSampleId :

RVE-47





Tgt Ion:252 Resp: 27828

Ion Ratio Lower Upper

252 100

253 23.3 18.0 27.0

125 6.6 4.6 6.8

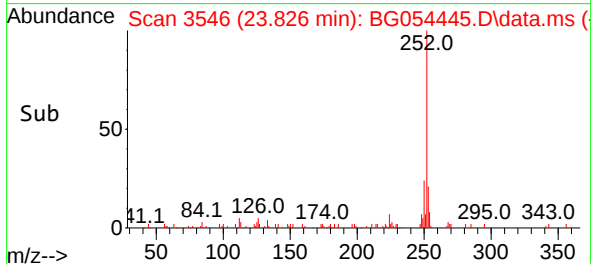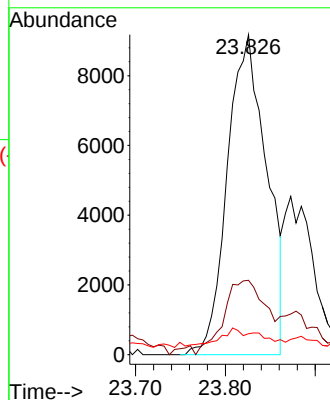

#90

Benzo(a)pyrene

Concen: 2.191 ng

RT: 24.684 min Scan# 3692

Delta R.T. -0.003 min

Lab File: BG054445.D

Acq: 29 Jul 2022 12:02

Tgt Ion:252 Resp: 17560

Ion Ratio Lower Upper

252 100

253 30.3 17.8 26.8#

125 7.7 4.3 6.5#

