

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
 Data File : BG054444.D
 Acq On : 29 Jul 2022 11:15
 Operator : CG/JU
 Sample : PB146540BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB146540BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.562	431	438	449	rBB	233216	385255	20.95%	6.625%
2	7.171	703	712	729	rBV	228868	411930	22.40%	7.084%
3	7.982	843	850	857	rBV2	44027	76503	4.16%	1.316%
4	9.146	1041	1048	1061	rBB	141963	268581	14.60%	4.619%
5	10.797	1321	1329	1338	rBV	57275	105540	5.74%	1.815%
6	13.241	1738	1745	1754	rBV	470142	760350	41.34%	13.076%
7	14.622	1974	1980	1988	rBB	109708	172616	9.38%	2.968%
8	16.114	2228	2234	2251	rBV	445102	711684	38.69%	12.239%
9	17.365	2441	2447	2458	rBV	165682	265274	14.42%	4.562%
10	19.980	2884	2892	2898	rBV	1345325	1839297	100.00%	31.630%
11	21.631	3167	3173	3182	rBV	233730	385288	20.95%	6.626%
12	24.839	3708	3719	3731	rVB2	140159	403005	21.91%	6.930%
13	25.949	3900	3908	3917	rVB10	8641	29652	1.61%	0.510%




Sum of corrected areas: 5814975

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054444.D
Acq On : 29 Jul 2022 11:15
Operator : CG/JU
Sample : PB146540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146540BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

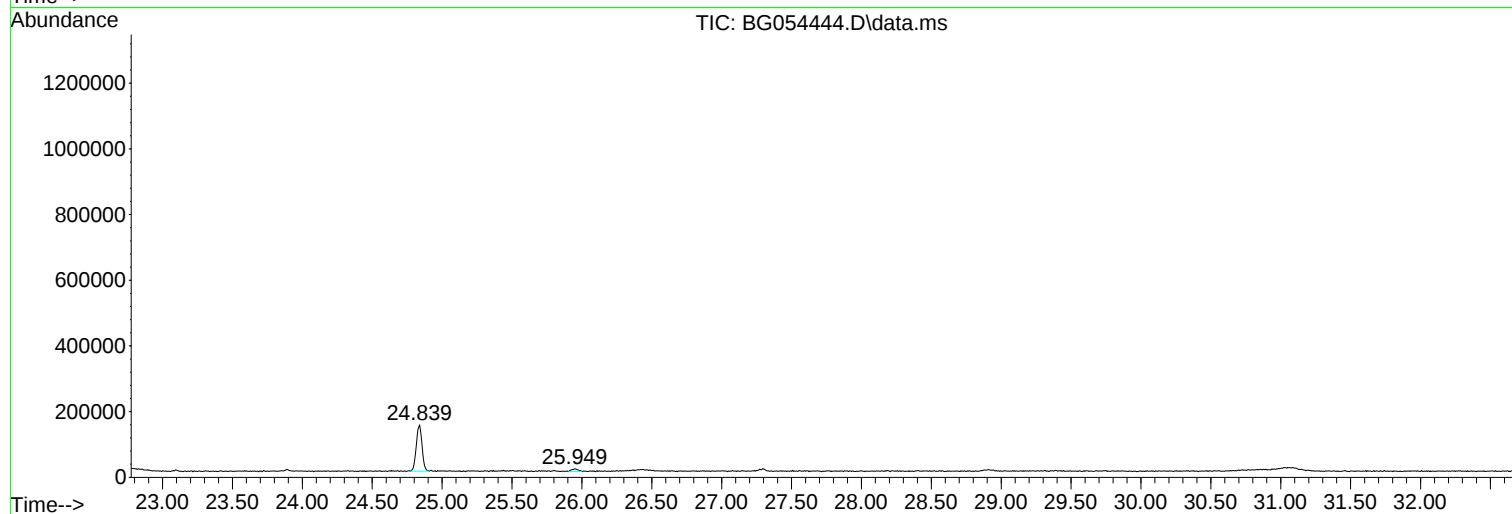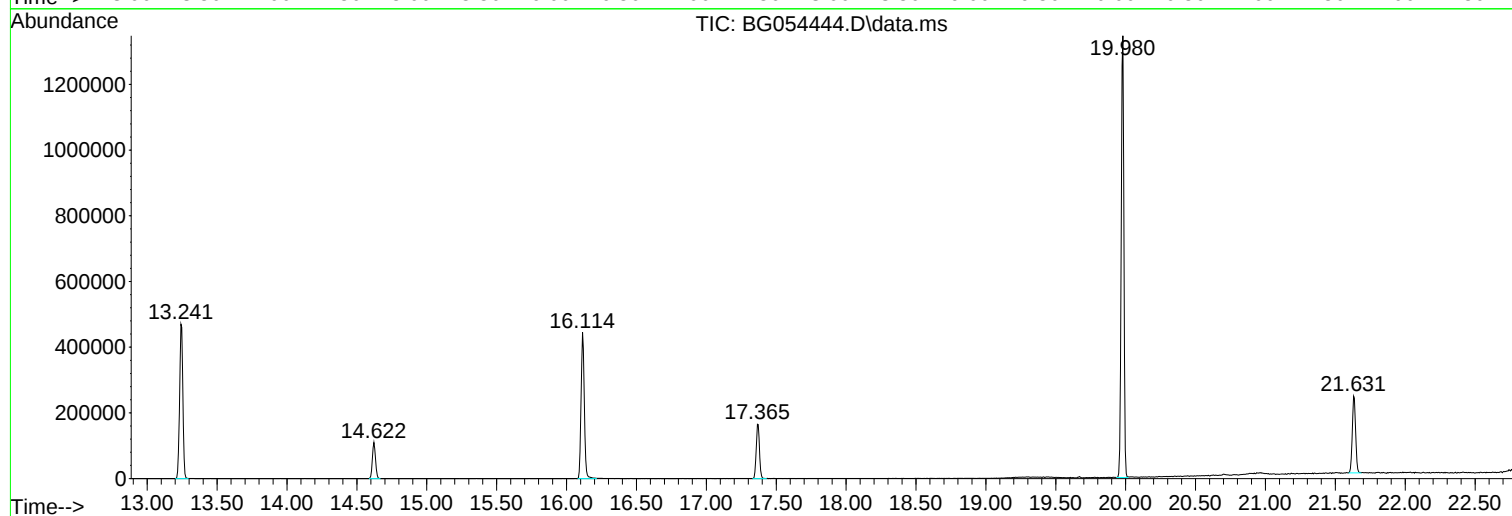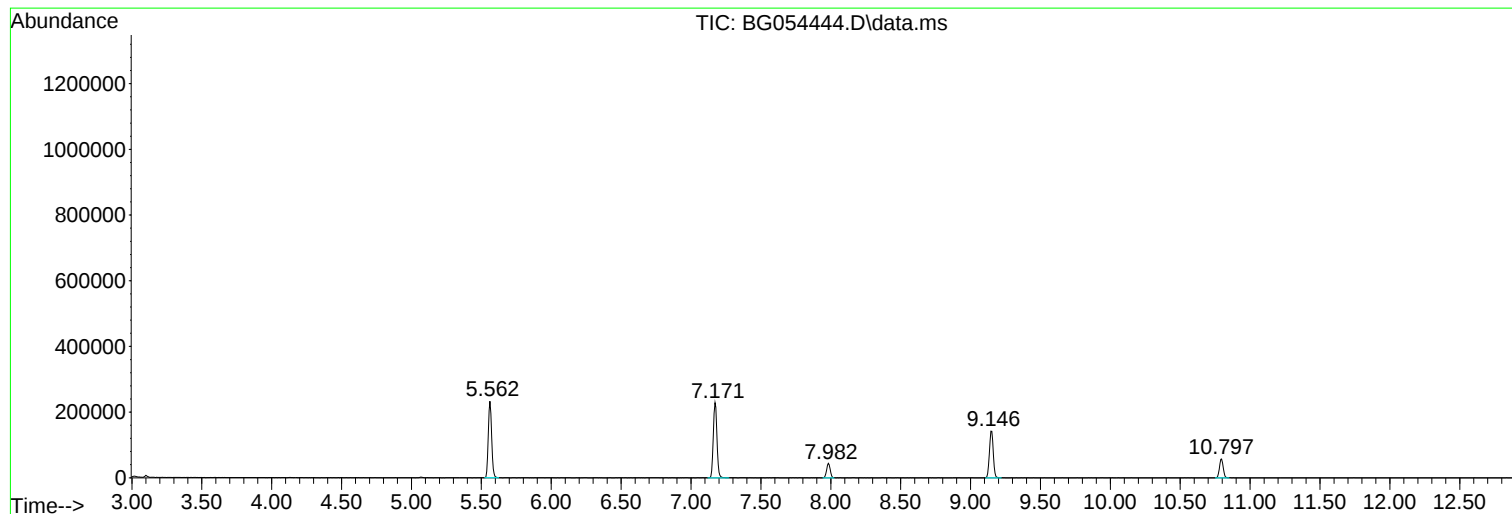

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054444.D
Acq On : 29 Jul 2022 11:15
Operator : CG/JU
Sample : PB146540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146540BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054444.D
Acq On : 29 Jul 2022 11:15
Operator : CG/JU
Sample : PB146540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146540BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------