
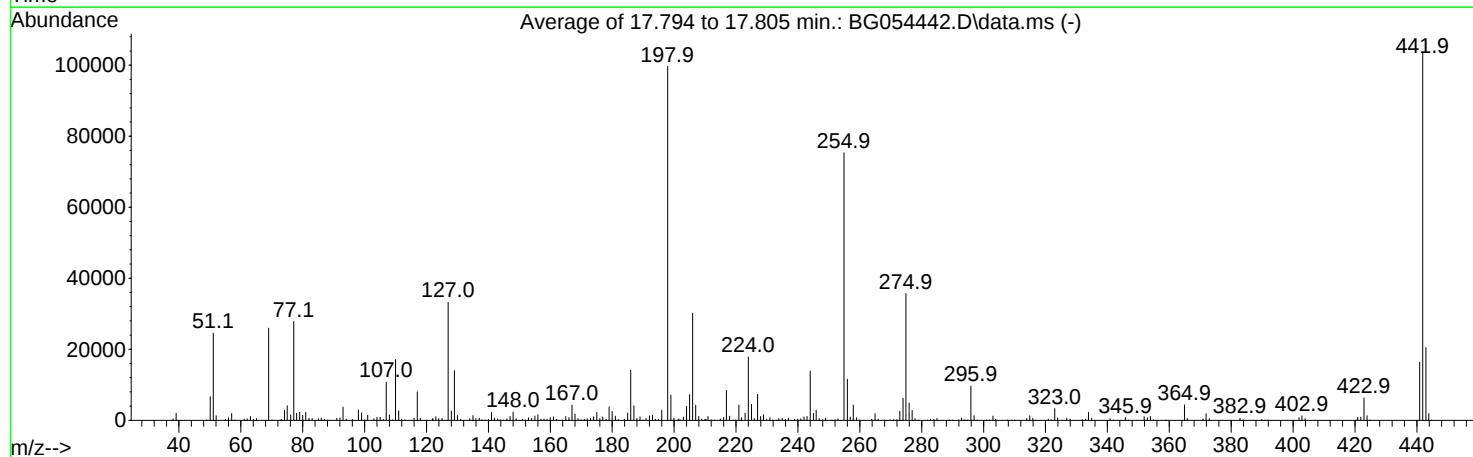


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054442.D
Acq On : 29 Jul 2022 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 28 04:30:50 2022

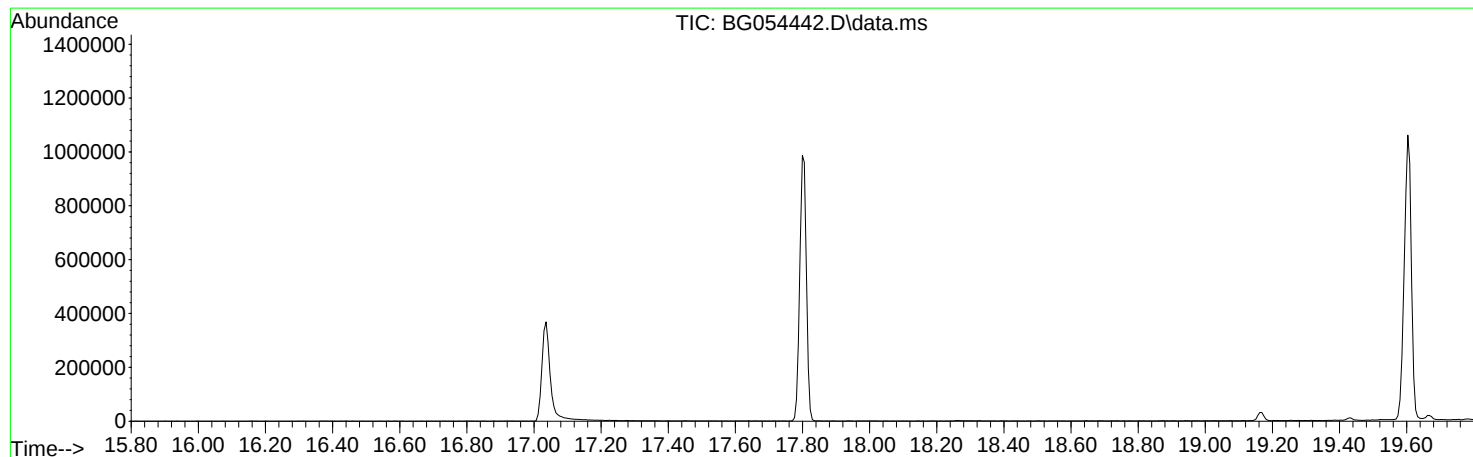




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	24520	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.0	25957	PASS
70	69	0.00	2	0.5	120	PASS
127	198	10	80	33.3	33229	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99661	PASS
199	198	5	9	7.1	7114	PASS
275	198	10	60	35.8	35648	PASS
365	198	1	100	4.3	4332	PASS
441	198	0.01	100	16.4	16340	PASS
442	442	50	100	100.0	103600	PASS
443	442	15	24	19.8	20500	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054442.D
Acq On : 29 Jul 2022 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 29 09:44:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

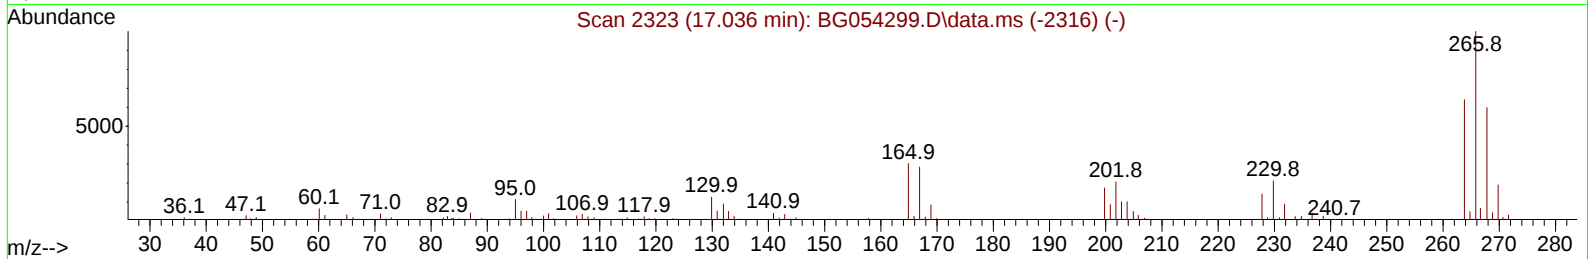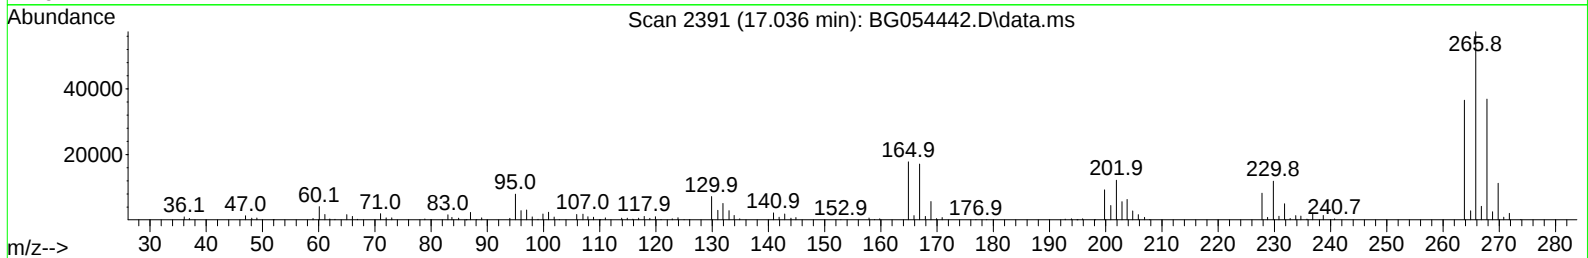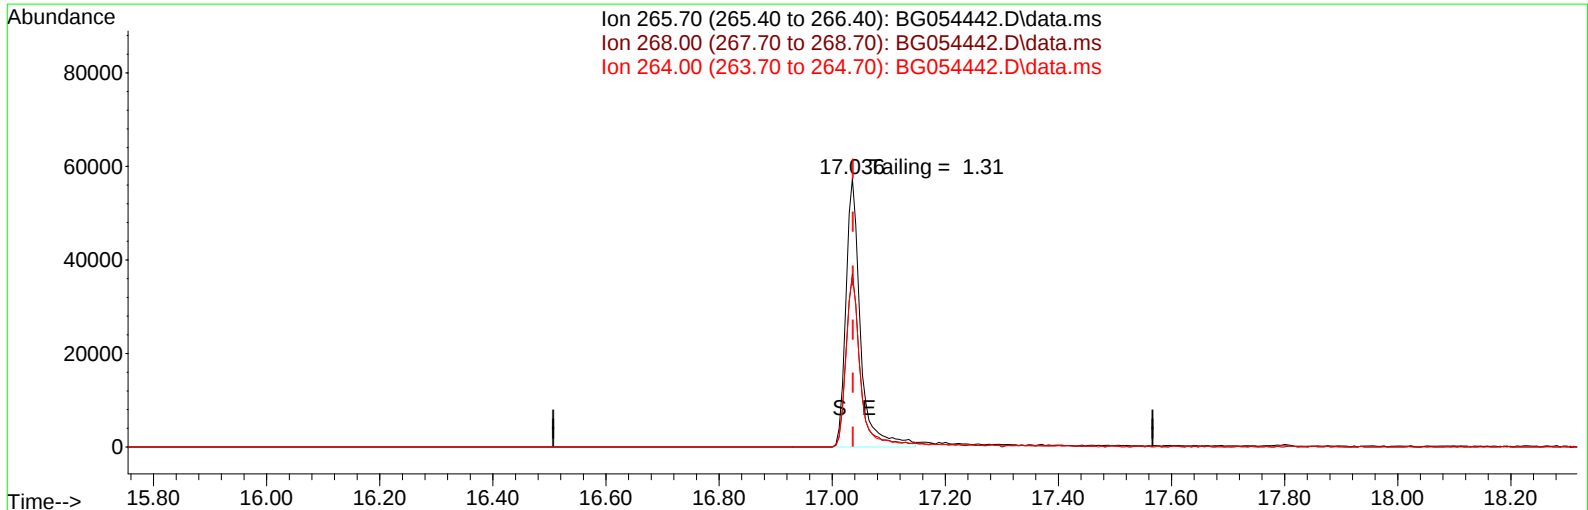

TIC: BG054442.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.001) 19757.93 ng




response 103564

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.28
264.00	66.20	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072922\
Data File : BG054442.D
Acq On : 29 Jul 2022 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 29 09:44:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

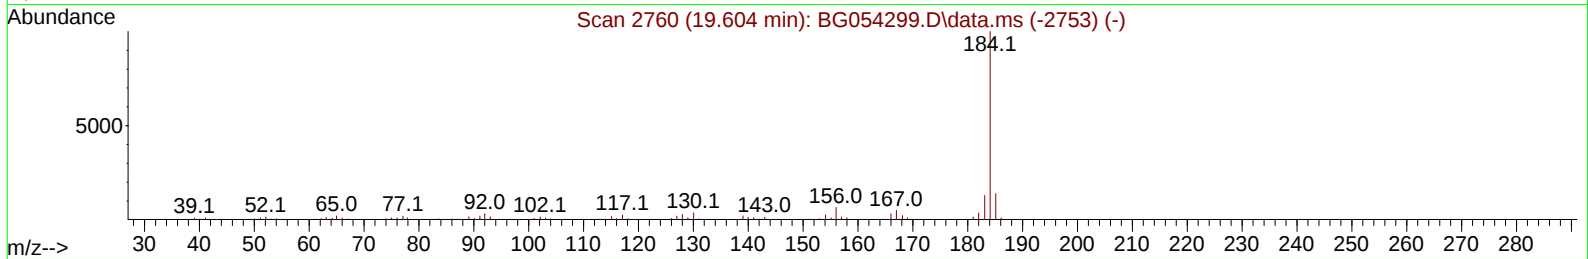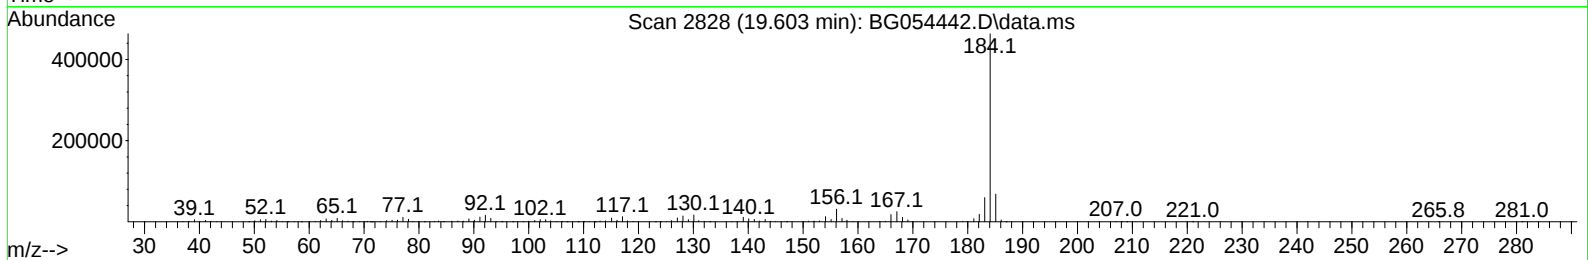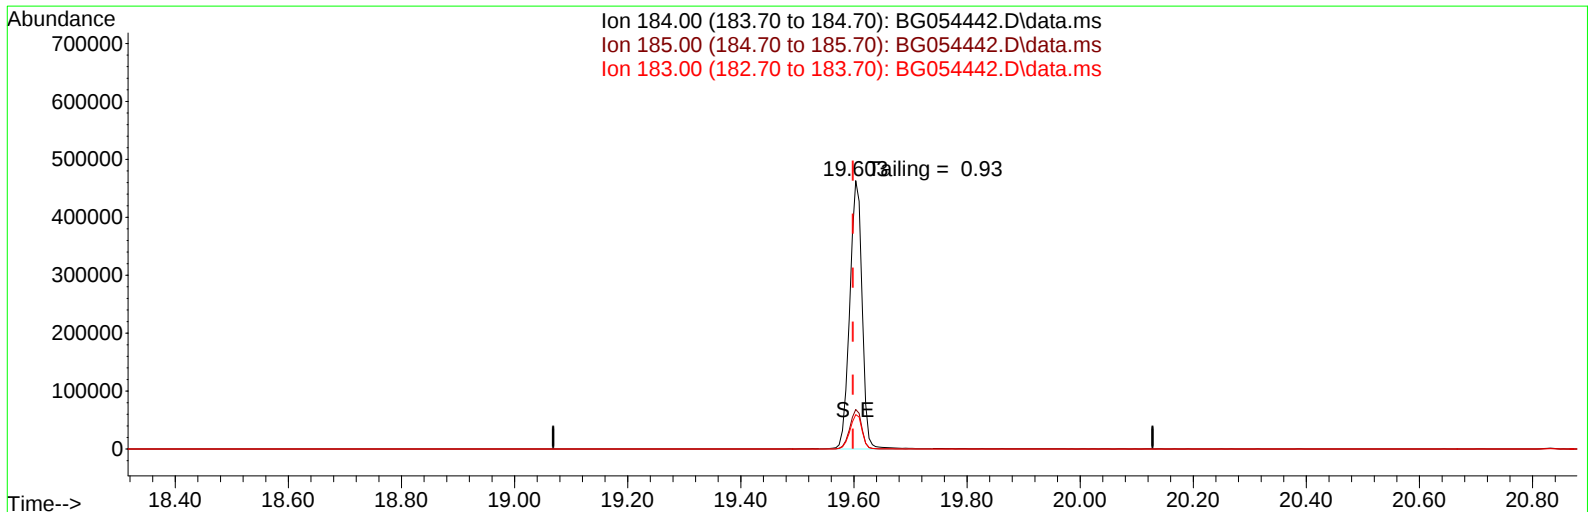

TIC: BG054442.D\data.ms

(77) Benzidine

19.603min (+ 0.005) 549844.35 ng

response 707025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.77
183.00	11.10	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/29/2022	BNA_G	<u>BG054442.D</u>
Compound Name	Response	Retention Time
DDT	408645	20.831
DDD	16171	20.391
DDE	858	19.885
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17029	425674	4.00

Instrument :
BNA_G
ClientSampleId :
DFTPP