


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073015\
Data File : BG018172.D
Acq On : 30 Jul 2015 12:26
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 08 17:26:43 2015

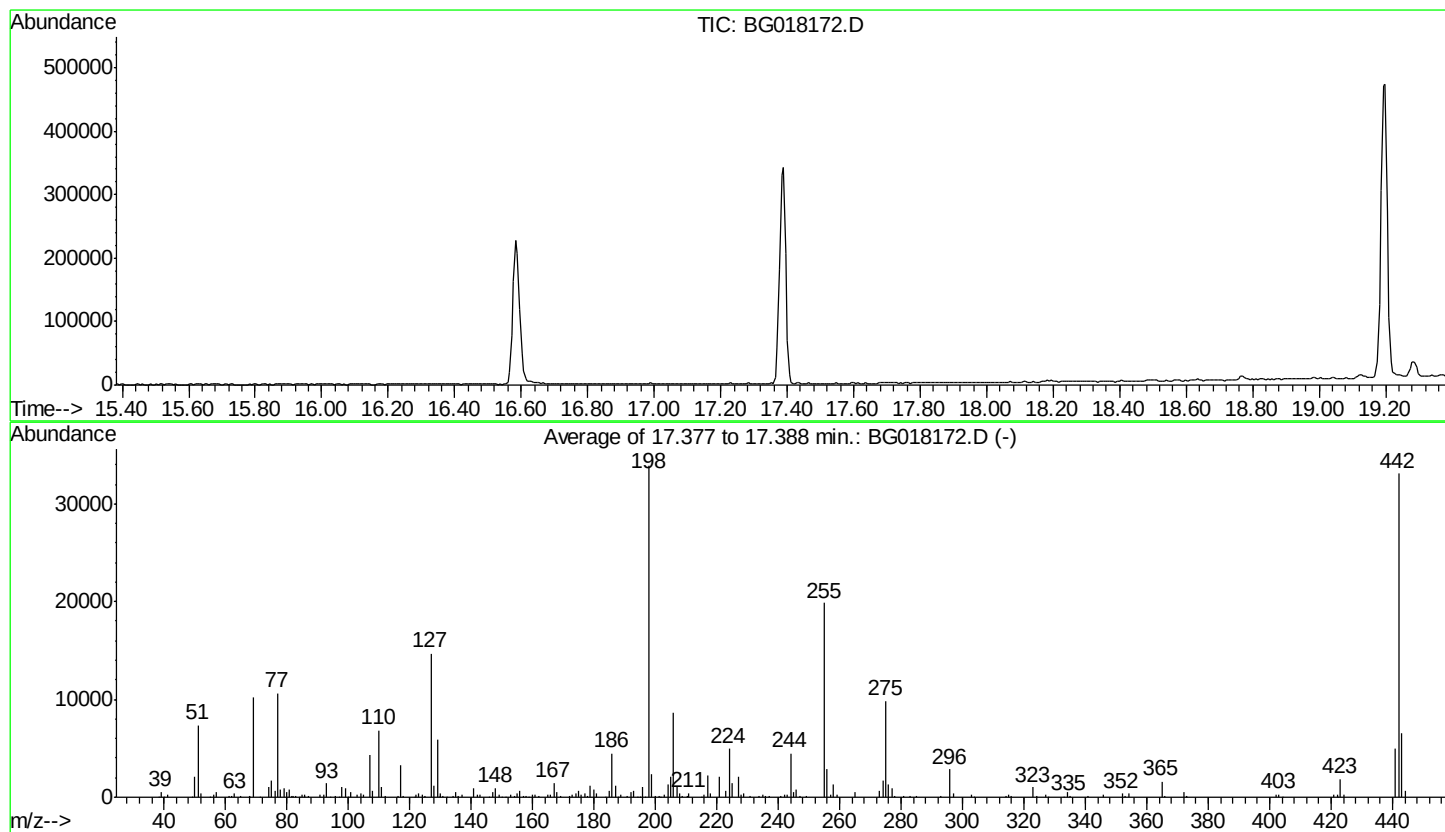

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	7382	PASS
68	69	0.00	2	1.1	115	PASS
69	198	0.00	100	29.9	10152	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.3	14675	PASS
197	198	0.00	2	0.2	69	PASS
198	198	100	100	100.0	33901	PASS
199	198	5	9	7.1	2408	PASS
275	198	10	60	29.0	9829	PASS
365	198	1	100	4.8	1611	PASS
441	442	0.01	24	14.9	4941	PASS
442	198	50	100	97.5	33061	PASS
443	442	15	24	20.0	6613	PASS