

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073016\
 Data File : BG023345.D
 Acq On : 29 Jul 2016 22:32
 Operator : UM/SJ
 Sample : H4176-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-29-5.9-15.0

Quant Time: Jul 30 01:29:25 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 27 17:30:33 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	137534	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	649209	20.00	ng	0.00
38) Acenaphthene-d10	14.80	164	454637	20.00	ng	0.00
63) Phenanthrene-d10	17.57	188	1036972	20.00	ng	0.00
75) Chrysene-d12	21.89	240	1095091	20.00	ng	0.00
86) Perylene-d12	25.29	264	1113668	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	34671	4.30	ng	0.00
7) Phenol-d6	7.29	99	325140	26.29	ng	0.00
23) Nitrobenzene-d5	9.31	82	977926	73.66	ng	0.00
41) 2,4,6-Tribromophenol	16.31	330	9478	2.01	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	2236395	92.07	ng	0.00
78) Terphenyl-d14	20.18	244	3014603	89.49	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.25	163	118974	3.55	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073016\
Data File : BG023345.D
Acq On : 29 Jul 2016 22:32
Operator : UM/SJ
Sample : H4176-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-29-5.9-15.0

Quant Time: Jul 30 01:29:25 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

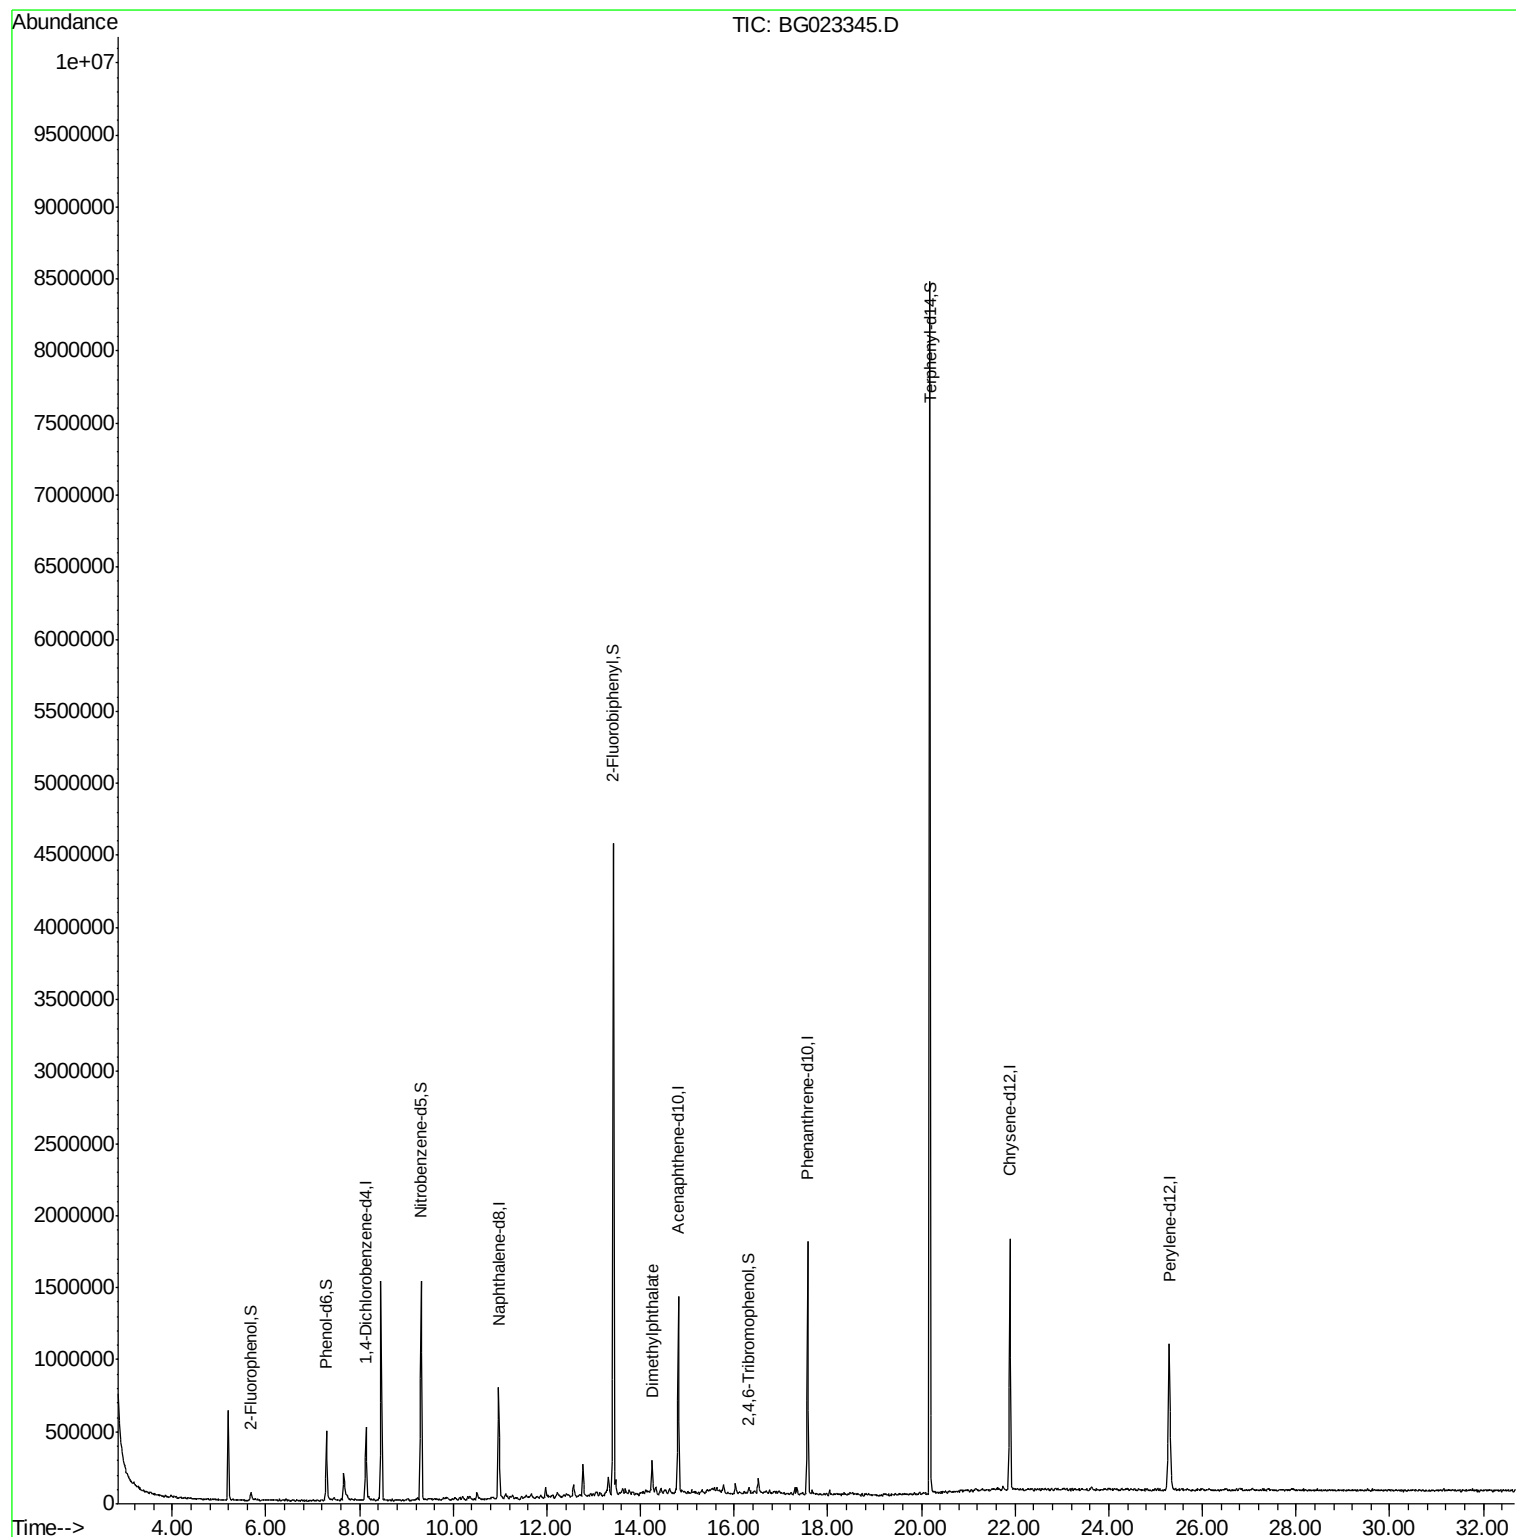



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.14 min Scan# 902

Delta R.T. -0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32

Instrument :

BNA_G

ClientSampleId :

GW-29-5.9-15.0


Tgt Ion:152 Resp: 137534

Ion Ratio Lower Upper

152 100

150 156.8 144.7 217.1




115 62.2 64.0 96.0#

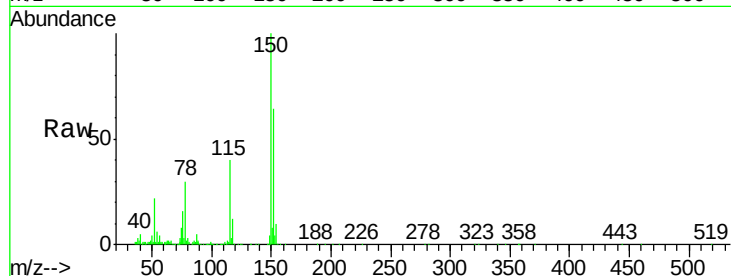

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

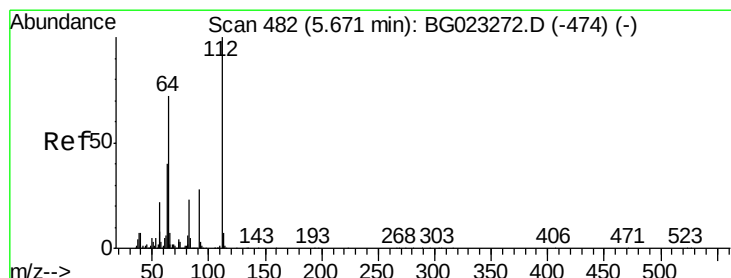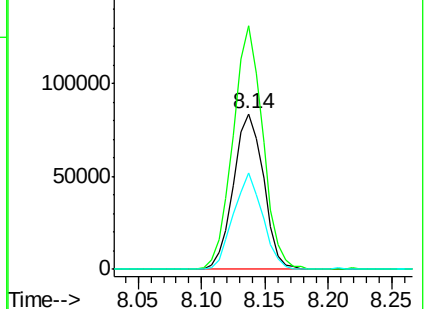

#5

2-Fluorophenol

Concen: 4.30 ng

RT: 5.68 min Scan# 484

Delta R.T. 0.01 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32


Tgt Ion:112 Resp: 34671

Ion Ratio Lower Upper

112 100

64 52.2 59.0 88.4#



63 30.0 37.8 56.8#

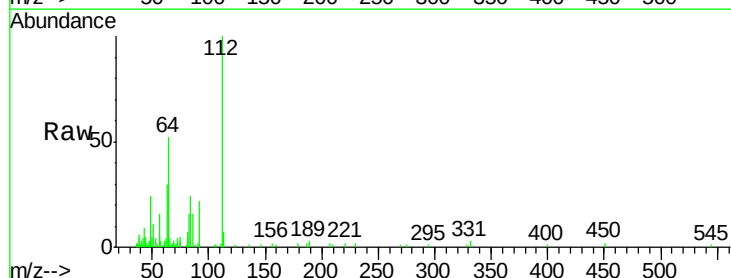


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

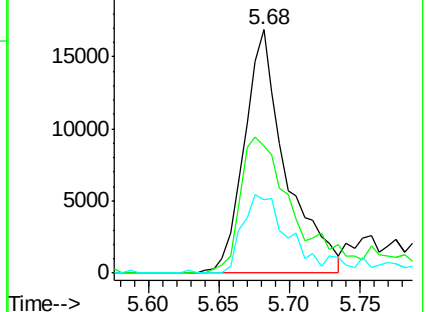



#7

Phenol-d6

Concen: 26.29 ng

RT: 7.29 min Scan# 758

Delta R.T. 0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32

Instrument :

BNA_G

ClientSampleId :

GW-29-5.9-15.0


Tgt Ion: 99 Resp: 325140

Ion Ratio Lower Upper




99 100

42 17.2 17.8 26.6#

71 35.8 41.5 62.3#

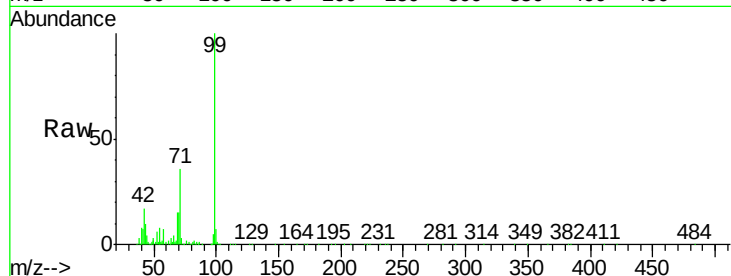

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

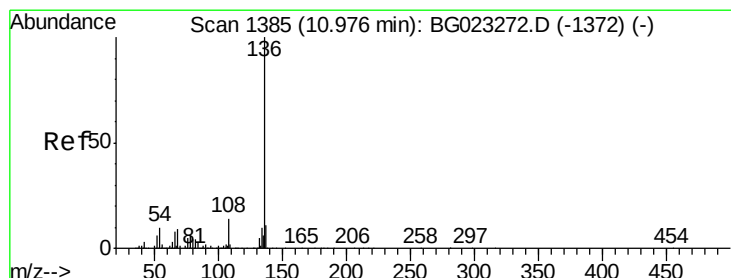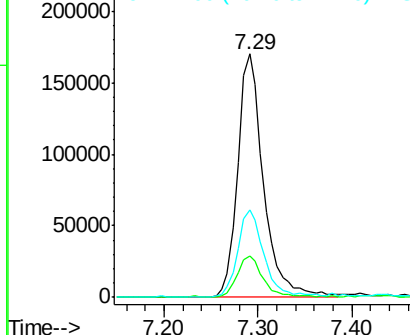

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.97 min Scan# 1385

Delta R.T. -0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32

Tgt Ion: 136 Resp: 649209


Ion Ratio Lower Upper

136 100



137 11.0 9.6 14.4


54 8.1 7.3 10.9

68 7.4 5.3 7.9

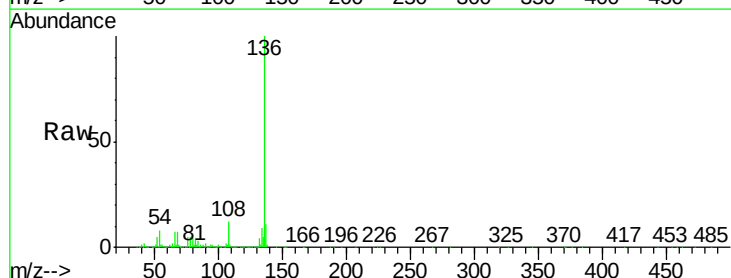

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



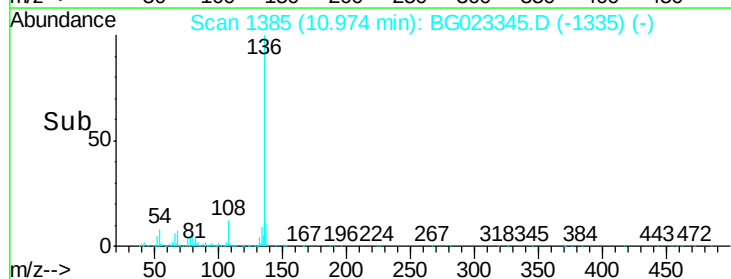
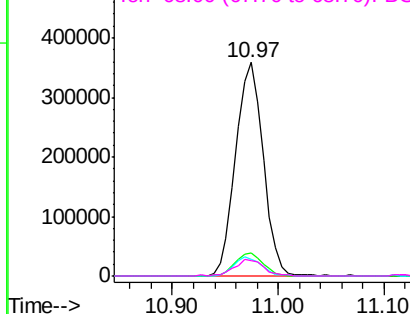


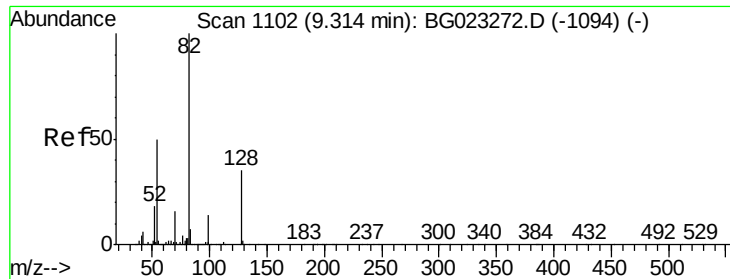

#23
 Nitrobenzene-d5
 Concen: 73.66 ng
 RT: 9.31 min Scan# 1102
 Delta R.T. 0.00 min
 Lab File: BG023345.D
 Acq: 29 Jul 2016 22:32




Instrument :
 BNA_G
 ClientSampleId :
 GW-29-5.9-15.0


Tgt Ion: 82 Resp: 977926
 Ion Ratio Lower Upper
 82 100
 128 38.8 24.4 36.6#
 54 47.8 41.4 62.0

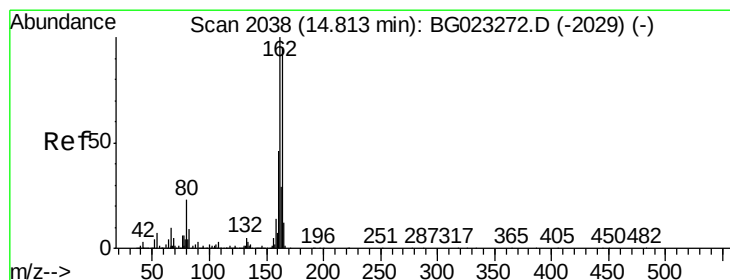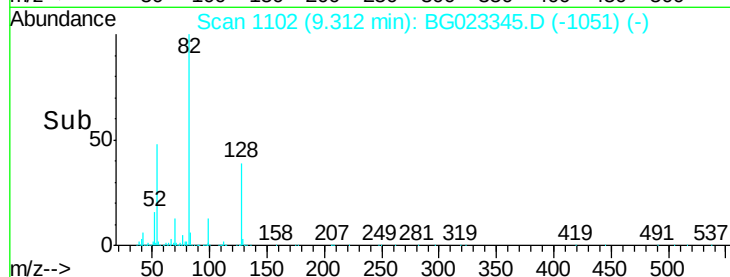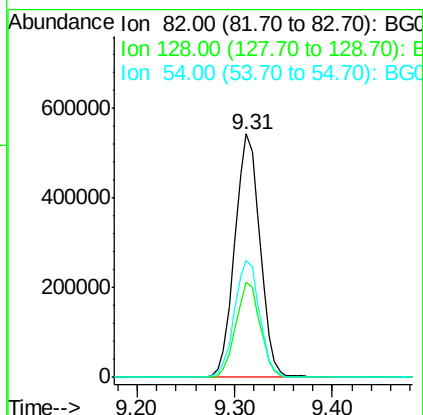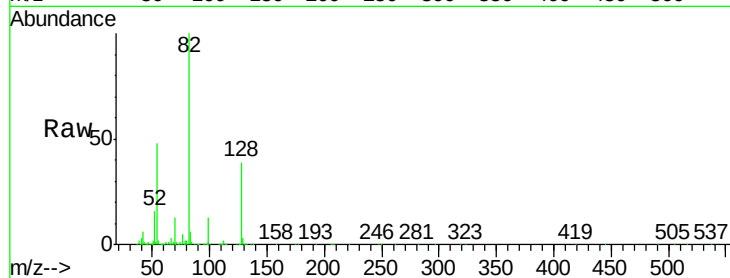

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.80 min Scan# 2037
 Delta R.T. -0.00 min
 Lab File: BG023345.D
 Acq: 29 Jul 2016 22:32

Tgt Ion: 164 Resp: 454637
 Ion Ratio Lower Upper
 164 100
 162 101.0 87.7 131.5
 160 46.7 37.2 55.8

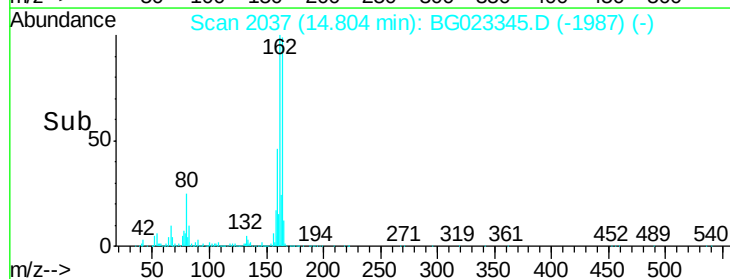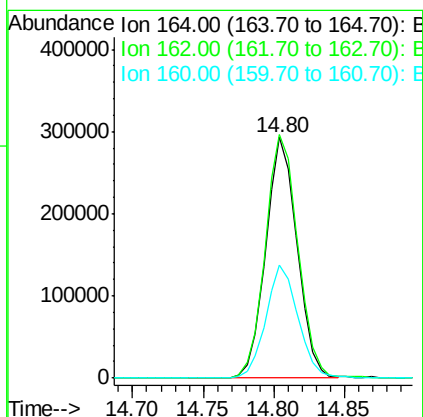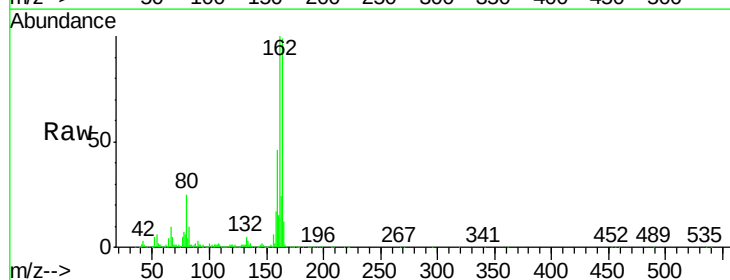


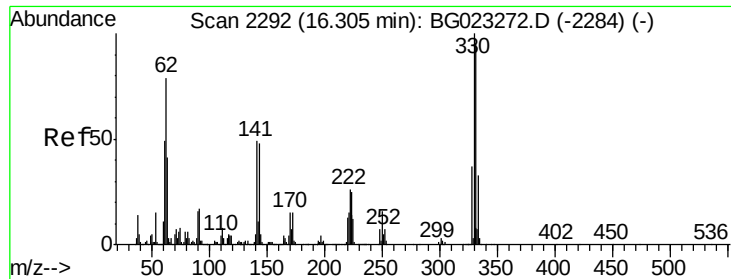




#41
2,4,6-Tribromophenol
Concen: 2.01 ng
RT: 16.31 min Scan# 2294
Delta R.T. 0.01 min
Lab File: BG023345.D
Acq: 29 Jul 2016 22:32

Instrument :
BNA_G
ClientSampleId :
GW-29-5.9-15.0

Tgt Ion:330 Resp: 9478
Ion Ratio Lower Upper
330 100
332 118.7 77.4 116.2#
141 32.7 31.7 47.5

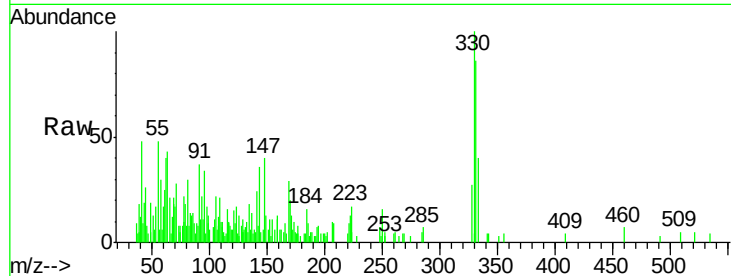


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

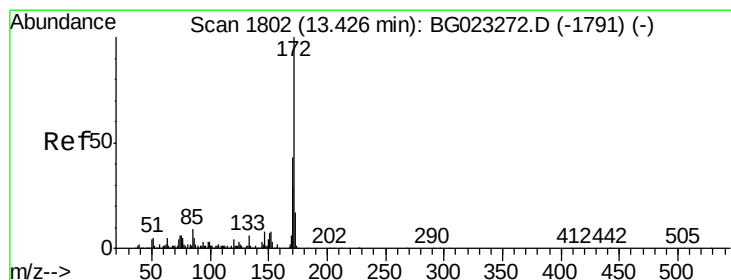
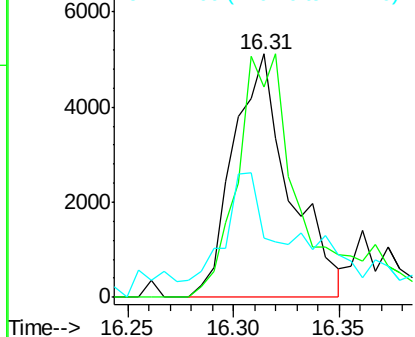



#44
2-Fluorobiphenyl
Concen: 92.07 ng
RT: 13.42 min Scan# 1801
Delta R.T. -0.00 min
Lab File: BG023345.D
Acq: 29 Jul 2016 22:32

Tgt Ion:172 Resp: 2236395
Ion Ratio Lower Upper
172 100
171 42.0 31.6 47.4
170 28.3 21.3 31.9

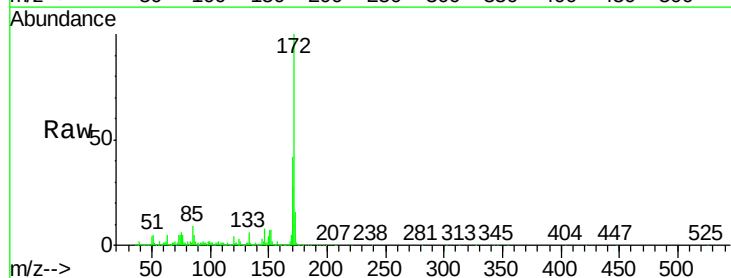

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

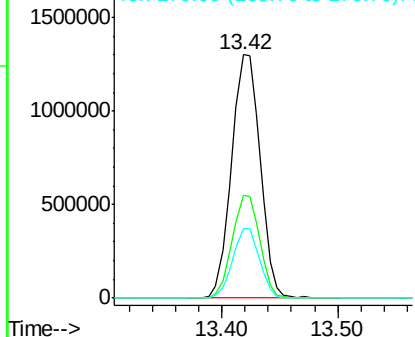



#49

Dimethylphthalate

Concen: 3.55 ng

RT: 14.25 min Scan# 1942

Delta R.T. -0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32

Instrument :

BNA_G

ClientSampleId :

GW-29-5.9-15.0


Tgt Ion:163 Resp: 118974

Ion Ratio Lower Upper

163 100

194 4.8 3.6 5.4




164 9.6 8.1 12.1

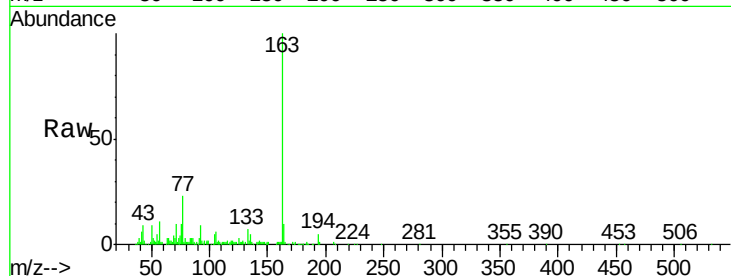

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

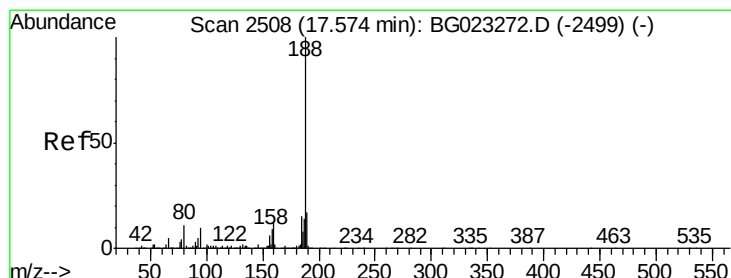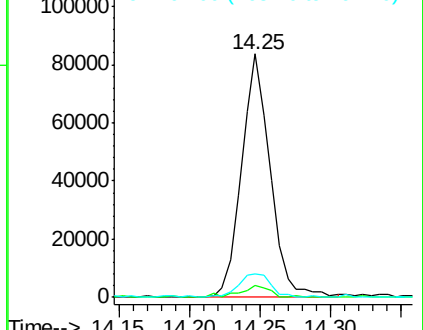

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.57 min Scan# 2507

Delta R.T. -0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32


Tgt Ion:188 Resp: 1036972

Ion Ratio Lower Upper

188 100

94 11.2 5.2 7.8#



80 12.9 7.2 10.8#

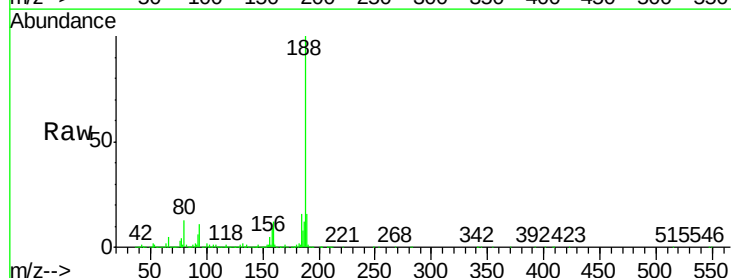


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

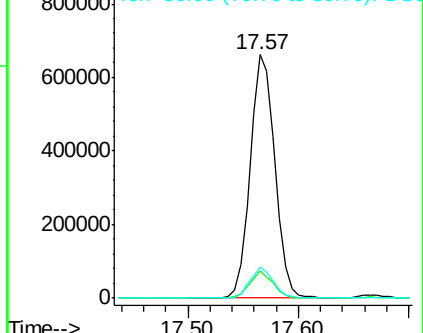



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.89 min Scan# 3243

Delta R.T. 0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32

Instrument :

BNA_G

ClientSampleId :

GW-29-5.9-15.0


Tgt Ion:240 Resp: 1095091

Ion Ratio Lower Upper

240 100

120 10.4 4.1 6.1#




236 29.3 21.1 31.7

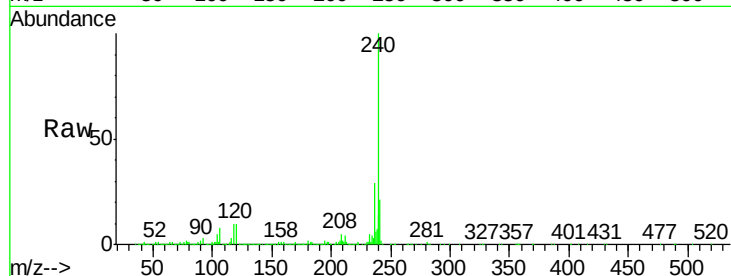

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

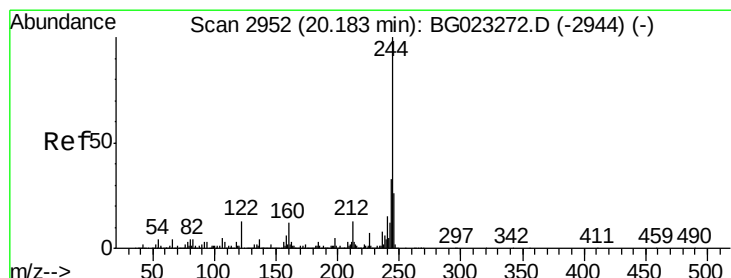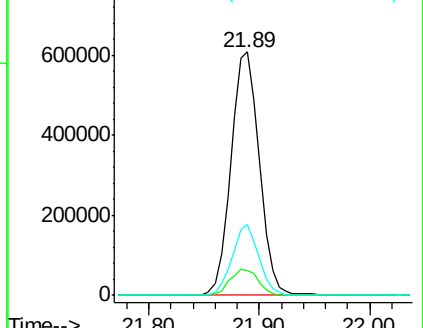

#78

Terphenyl-d14

Concen: 89.49 ng

RT: 20.18 min Scan# 2952

Delta R.T. 0.00 min

Lab File: BG023345.D

Acq: 29 Jul 2016 22:32


Tgt Ion:244 Resp: 3014603

Ion Ratio Lower Upper

244 100

212 14.0 10.8 16.2



122 14.6 8.0 12.0#

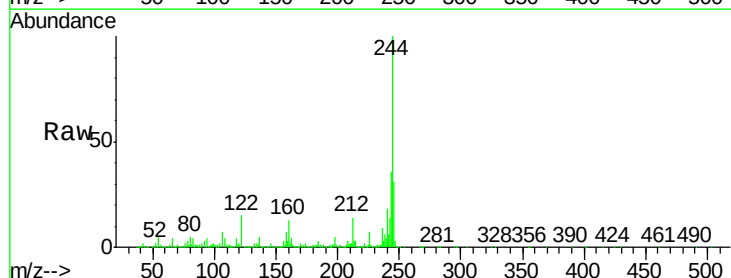


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

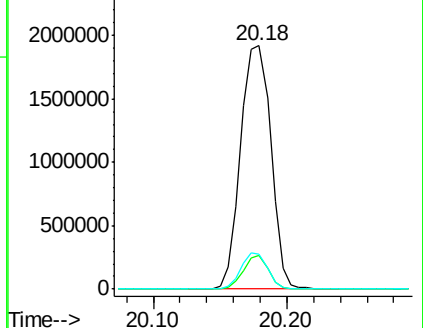

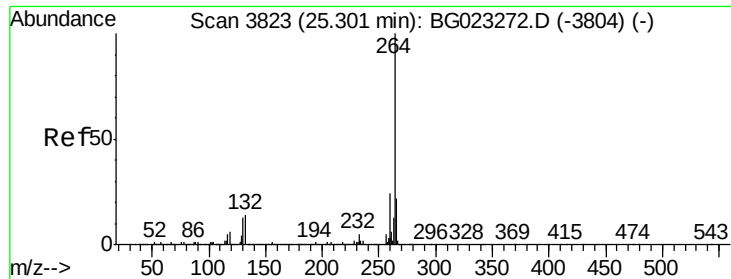

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.29 min Scan# 3822
Delta R.T. -0.01 min
Lab File: BG023345.D
Acq: 29 Jul 2016 22:32

Instrument :
BNA_G
ClientSampleId :
GW-29-5.9-15.0

Tgt Ion:264 Resp: 1113668

Ion	Ratio	Lower	Upper
264	100		
260	24.7	18.4	27.6
265	23.0	18.9	28.3

