


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073016\
 Data File : BG023338.D
 Acq On : 29 Jul 2016 15:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

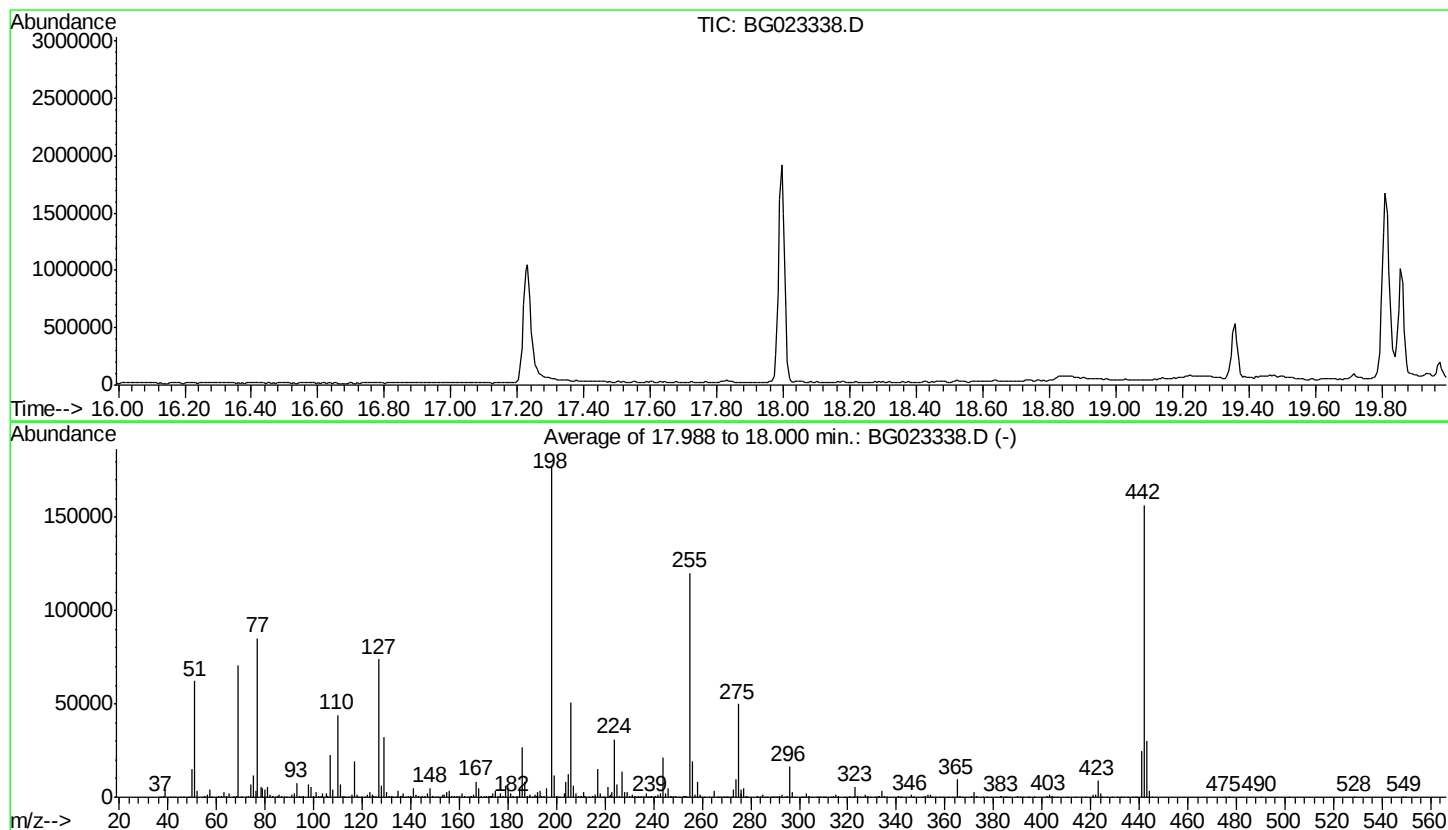

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	62285	PASS
68	69	0.00	2	0.9	611	PASS
69	198	0.00	100	39.9	70916	PASS
70	69	0.00	2	0.4	269	PASS
127	198	10	80	41.7	74002	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177642	PASS
199	198	5	9	6.7	11962	PASS
275	198	10	60	28.1	49941	PASS
365	198	1	100	5.2	9300	PASS
441	442	0.01	24	15.7	24650	PASS
442	198	50	100	88.2	156680	PASS
443	442	15	24	19.4	30365	PASS