
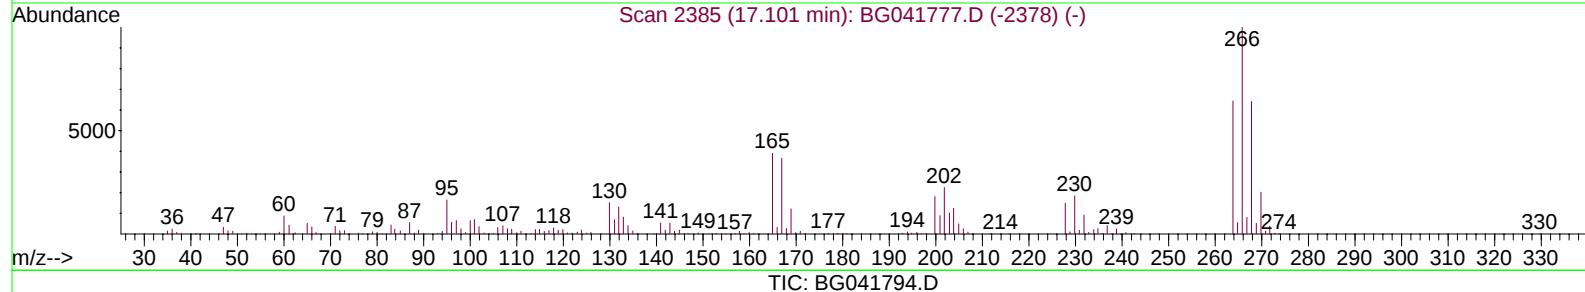
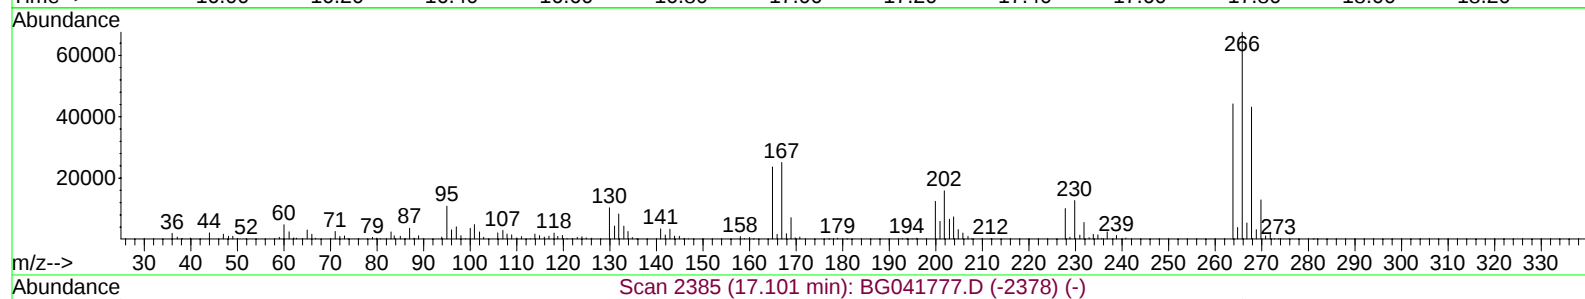


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041794.D
Acq On : 30 Jul 2019 8:13
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:05:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

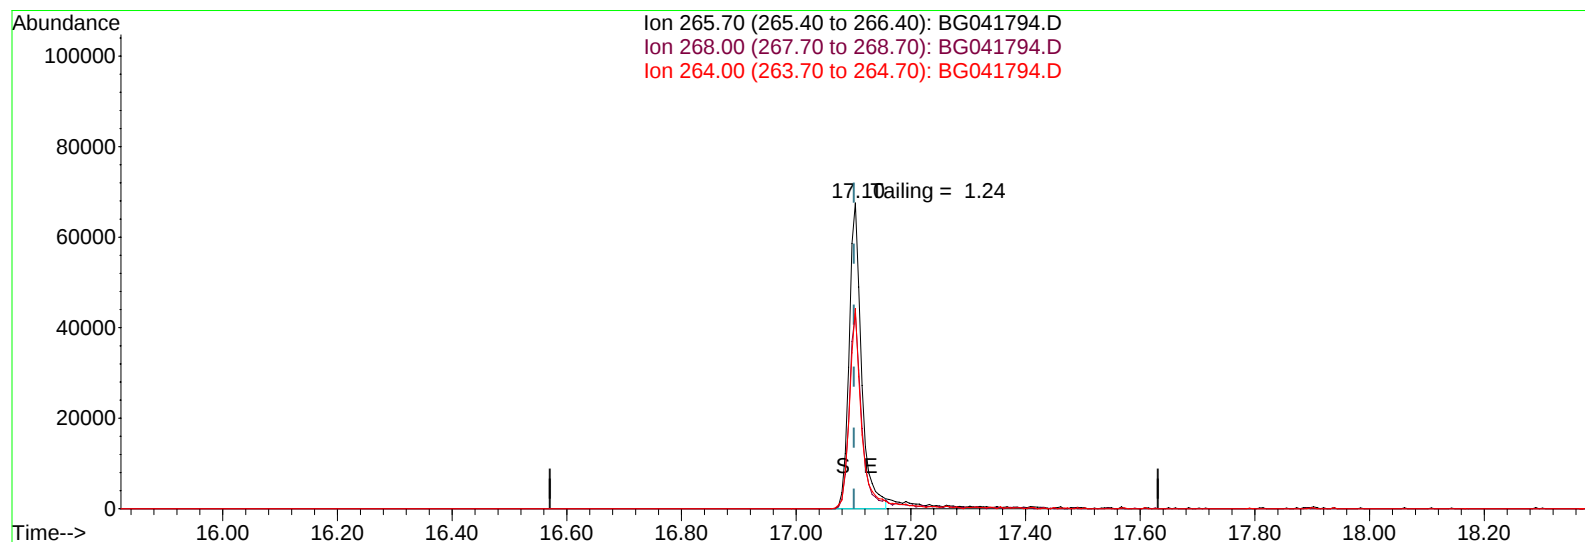

(70) Pentachlorophenol (C)




17.103min (+0.003) 22416.31ng

response 104699

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.89
264.00	64.30	65.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041794.D
Acq On : 30 Jul 2019 8:13
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:05:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

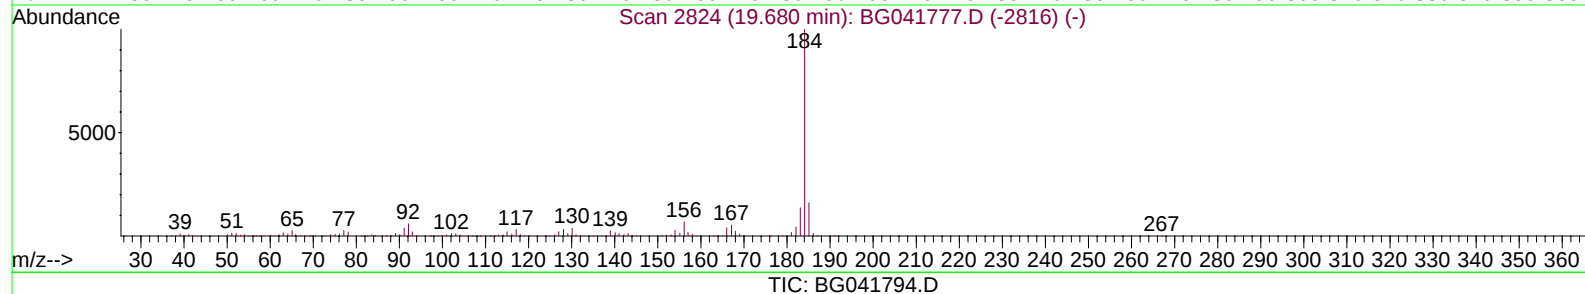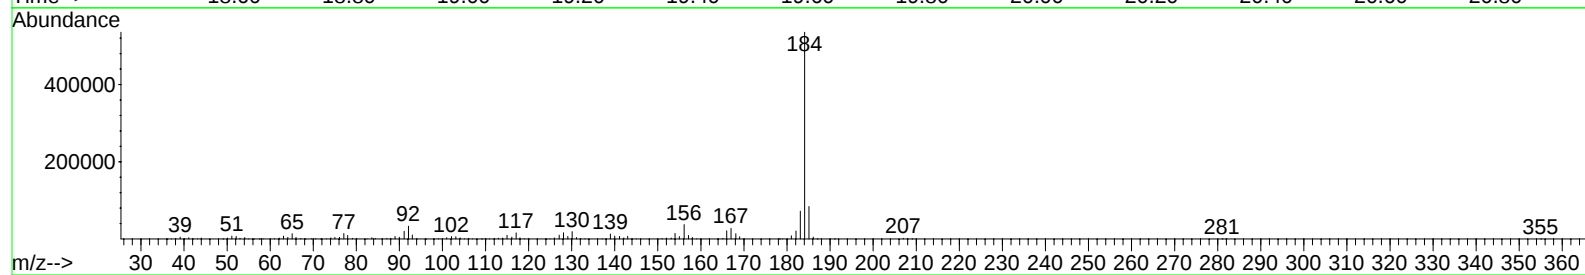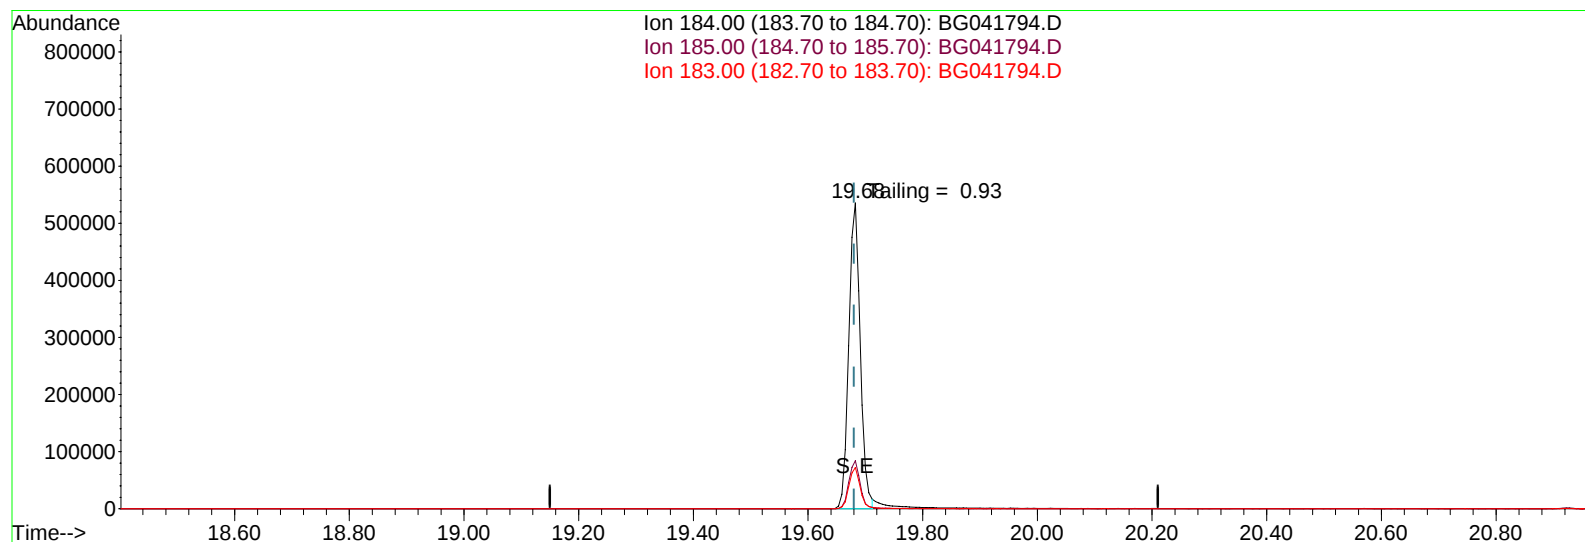

(77) Benzidine

19.683min (+0.003) 431075.66ng

response 773870

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.72
183.00	14.70	13.51
0.00	0.00	0.00