
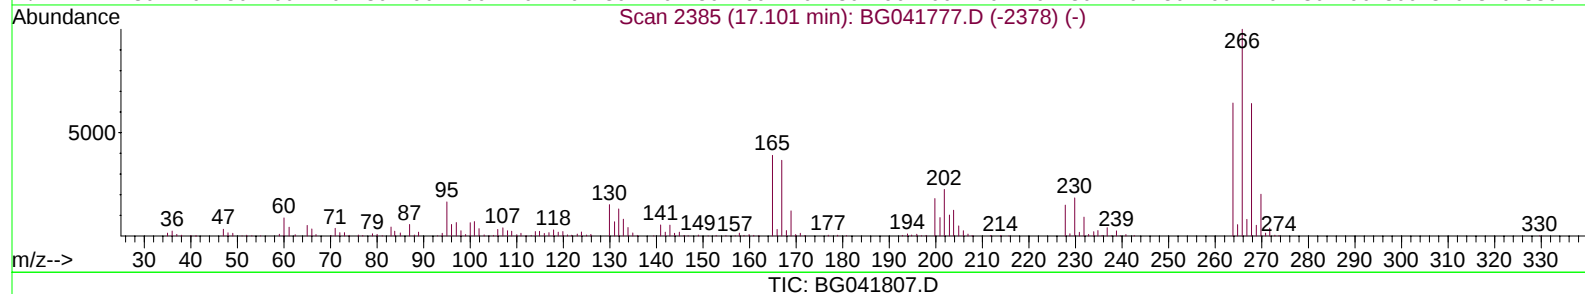
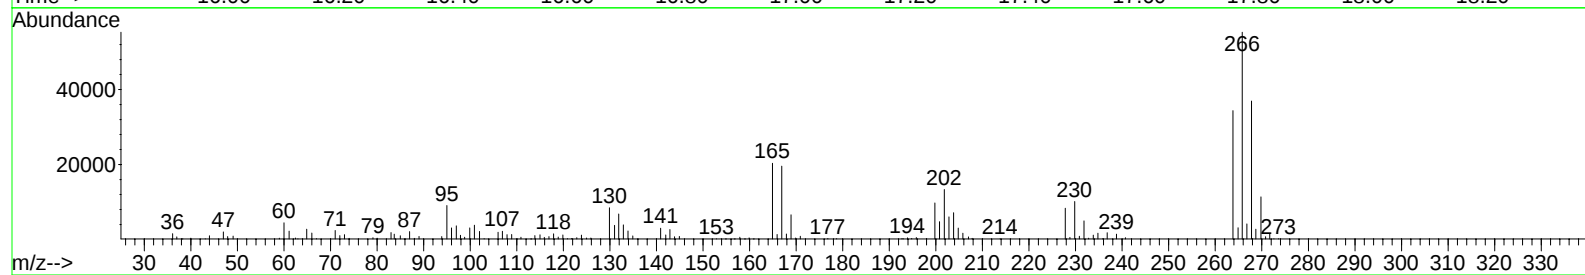


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041807.D
Acq On : 30 Jul 2019 18:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:03:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

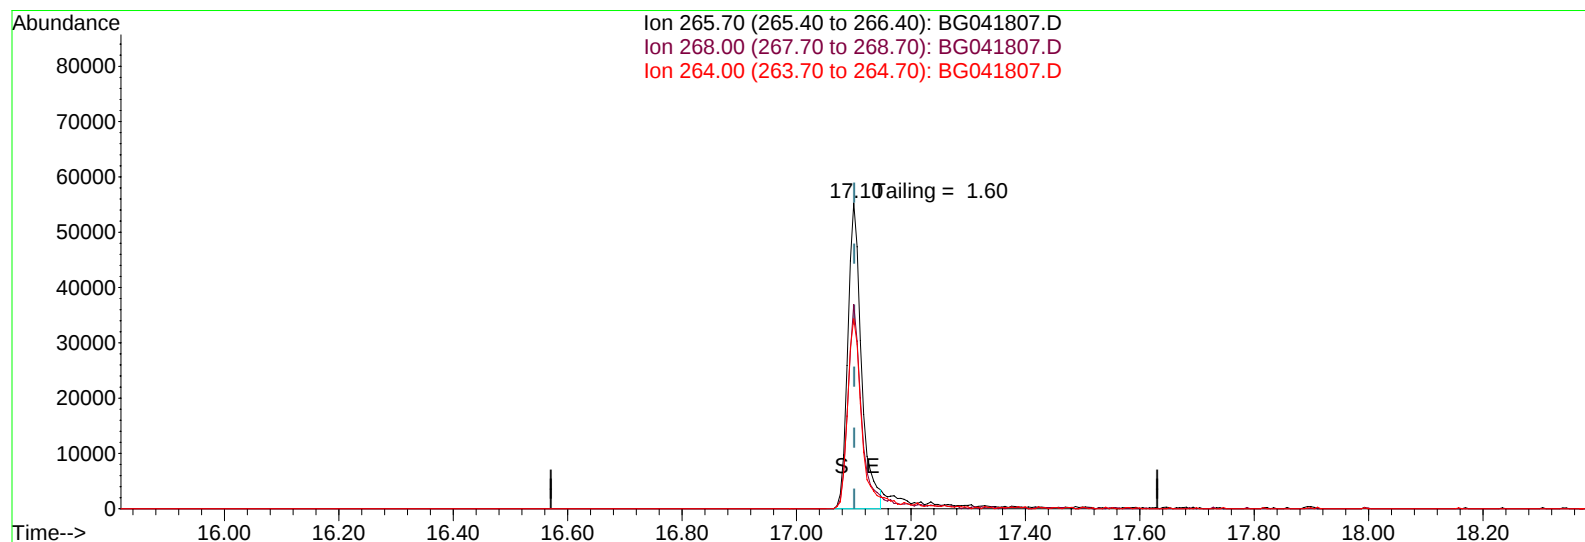

(70) Pentachlorophenol (C)




17.100min (-0.001) 169421.73ng

response 99224

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	71.73
264.00	64.30	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041807.D
Acq On : 30 Jul 2019 18:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:03:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

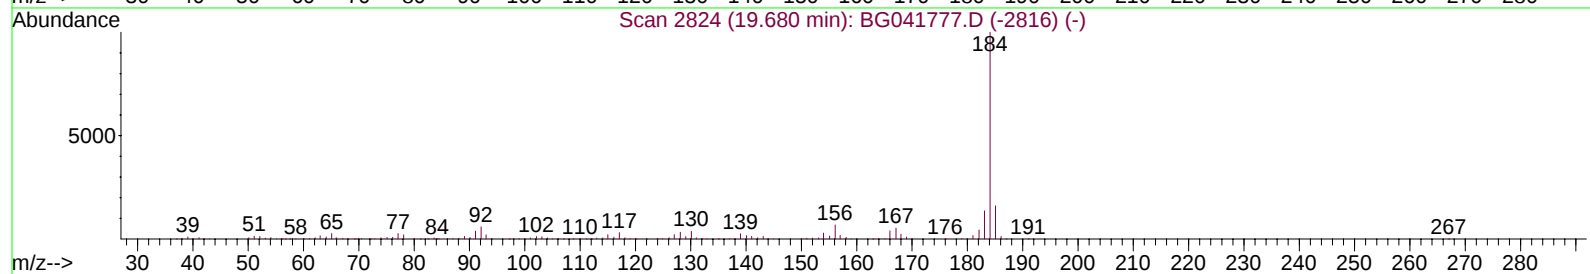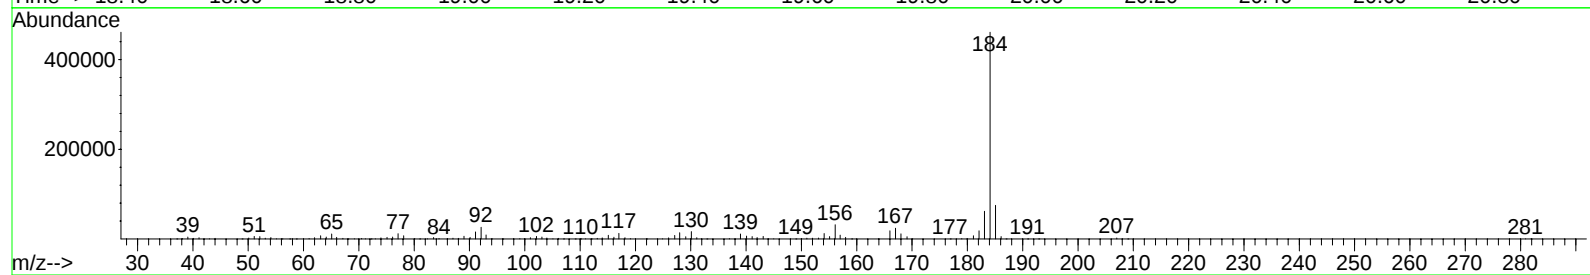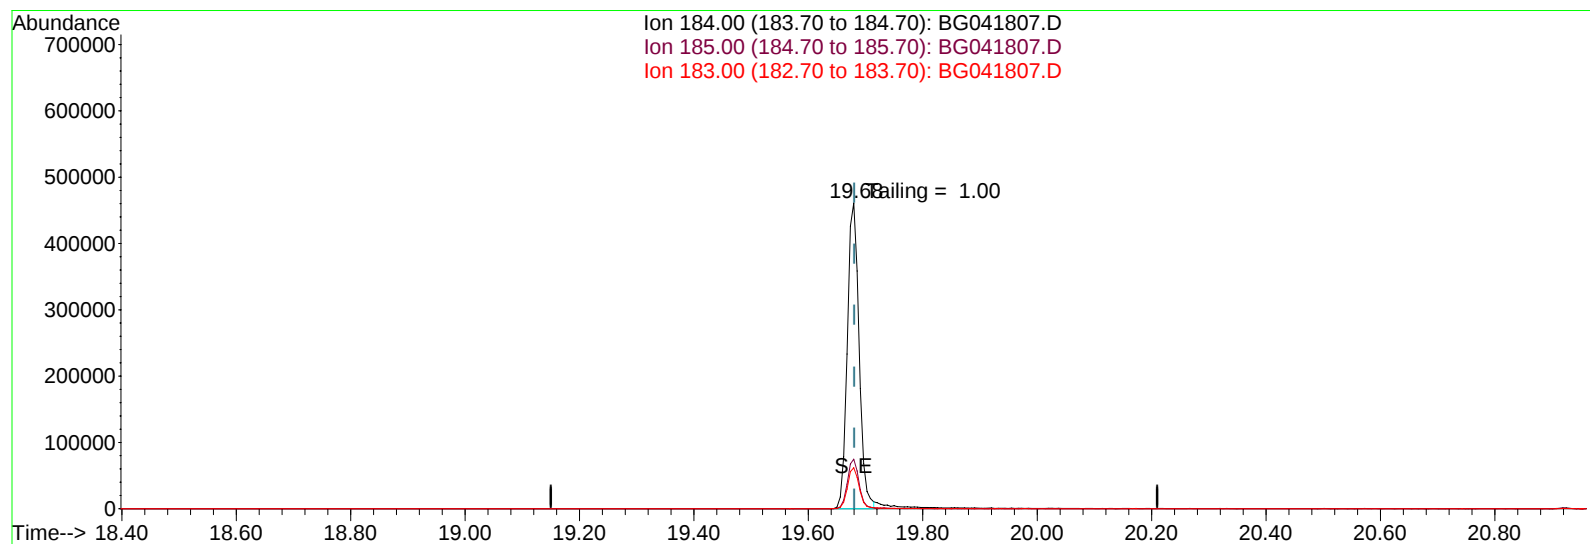

TIC: BG041807.D

(77) Benzidine

19.679min (-0.001) 350678.29ng

response 686771

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	16.25
183.00	14.70	13.40
0.00	0.00	0.00