
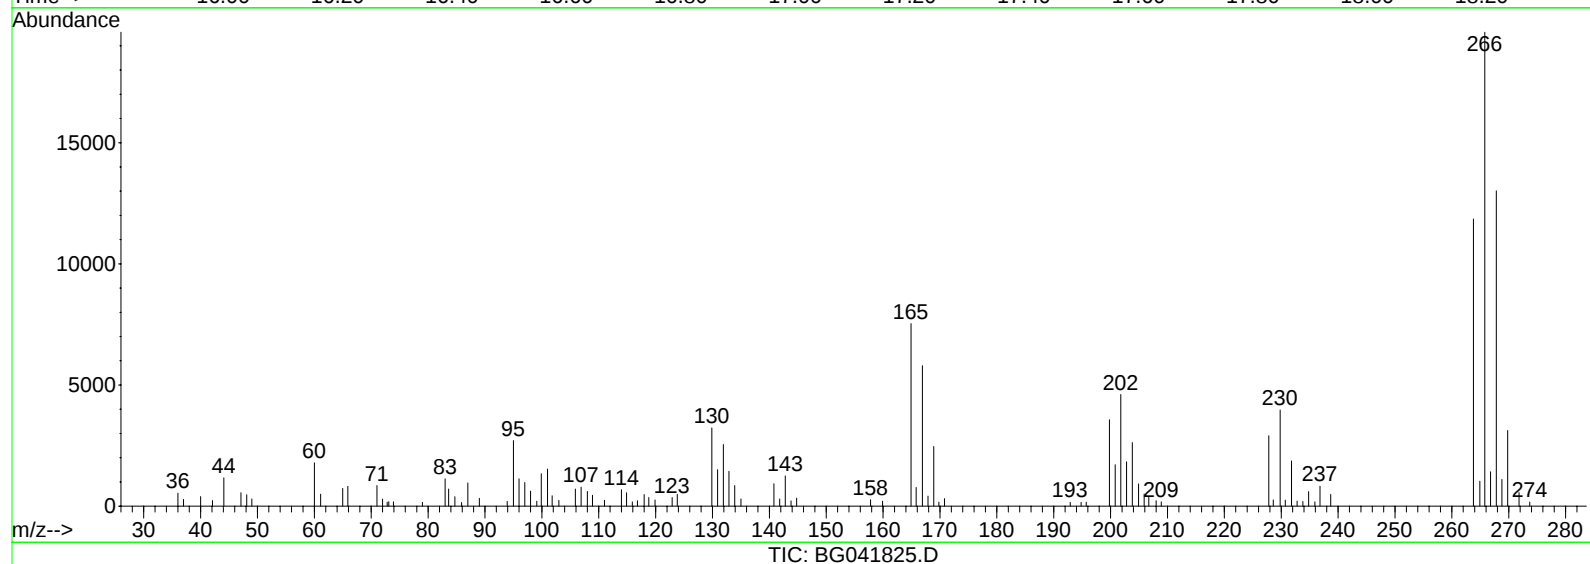


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041825.D
Acq On : 31 Jul 2019 6:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:00:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

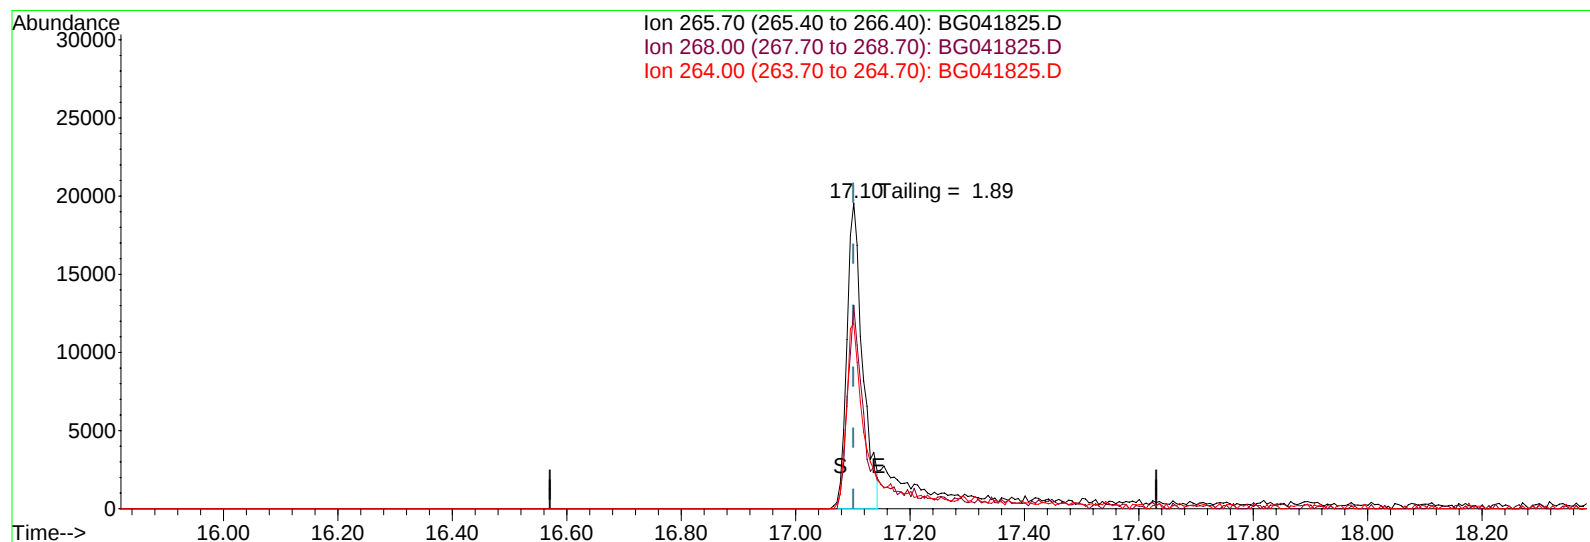

(70) Pentachlorophenol (C)



17.101min (+0.001) 13437.20ng

response 44562

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	66.53
264.00	64.30	60.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073019\
Data File : BG041825.D
Acq On : 31 Jul 2019 6:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 14:00:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

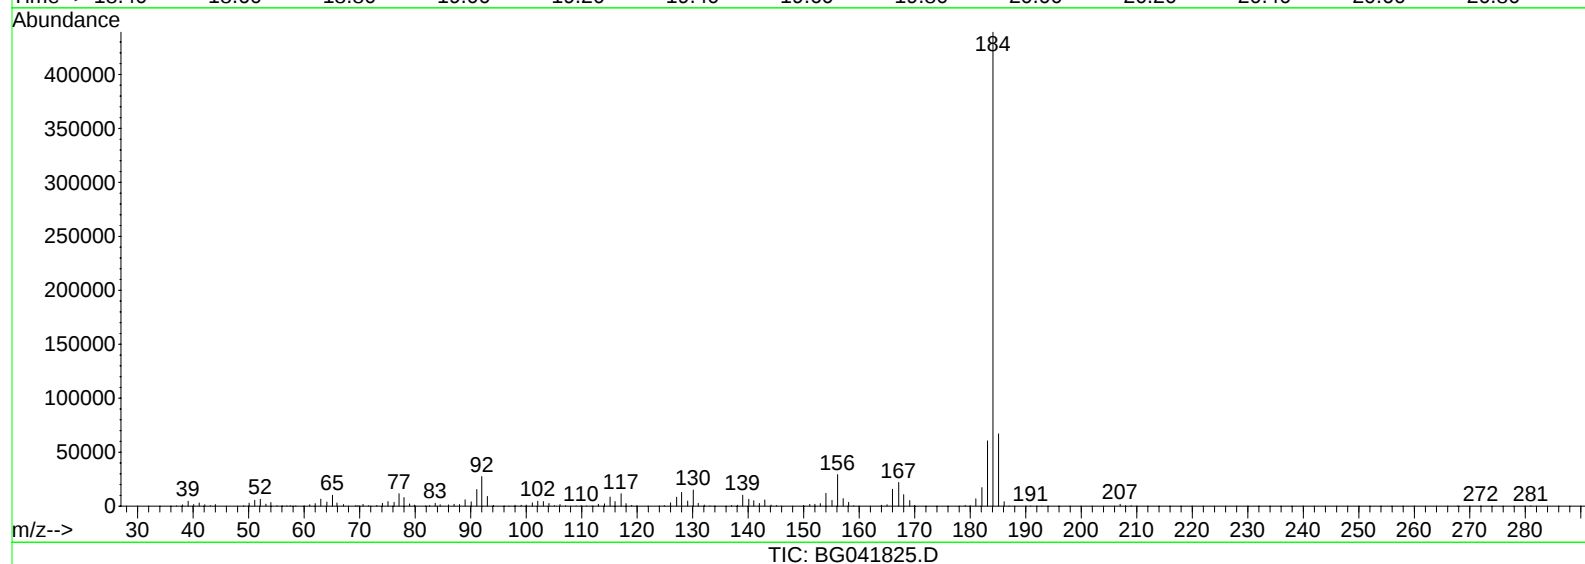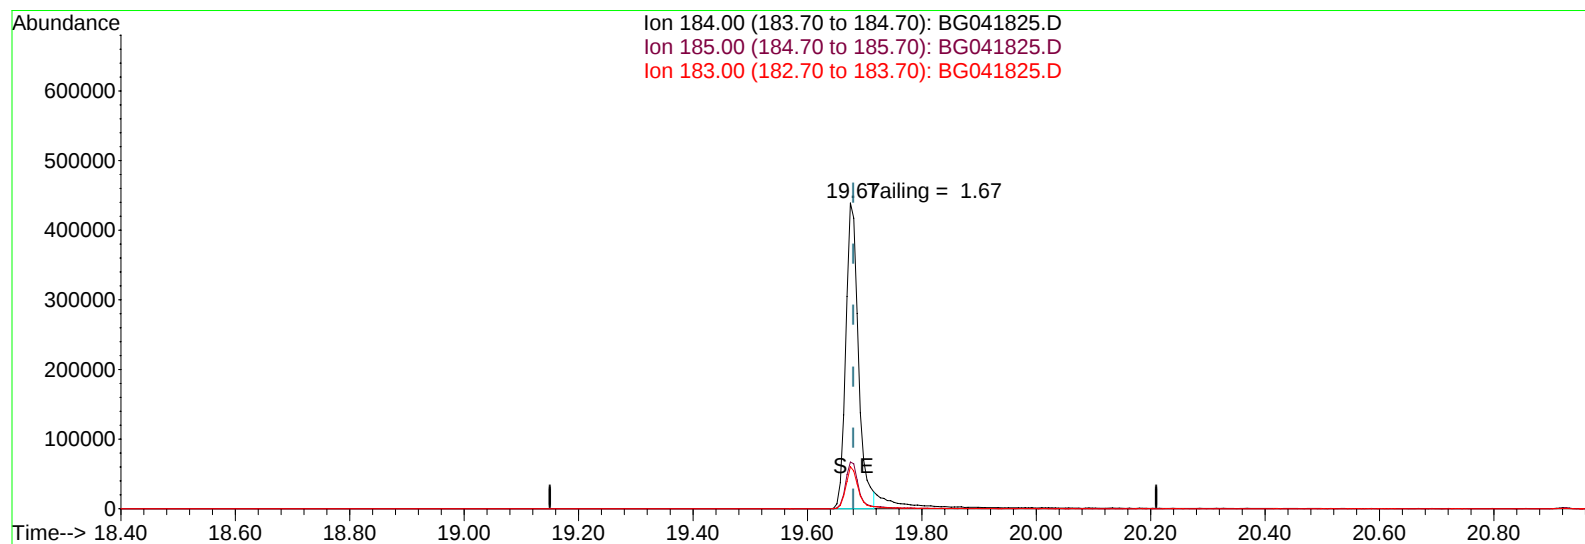

(77) Benzidine

19.675min (-0.005) 0.00ng

response 736391

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.26
183.00	14.70	13.78
0.00	0.00	0.00