


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG073019\
 Data File : BG041807.D
 Acq On : 30 Jul 2019 18:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 08:57:26 2019

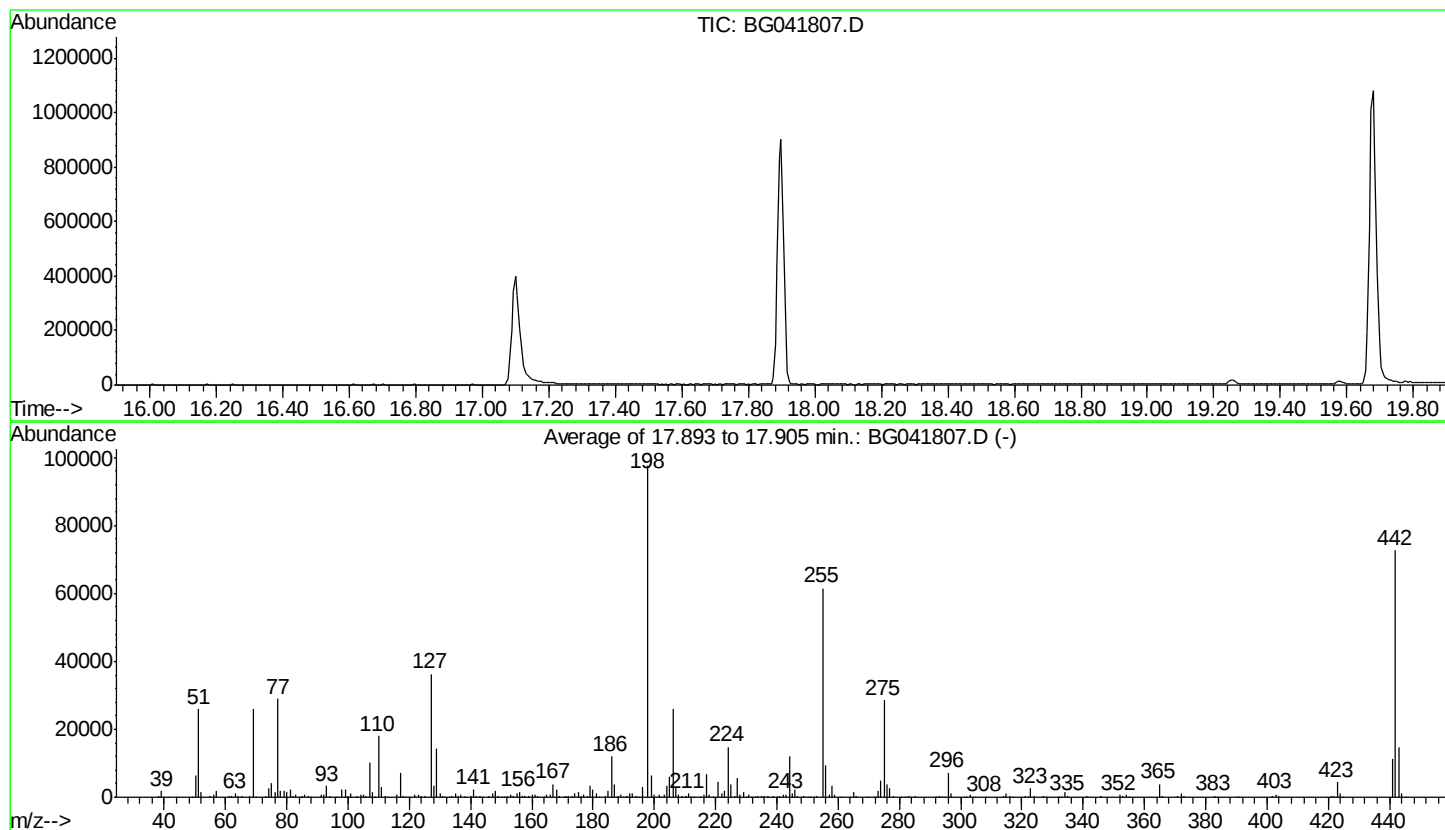

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	25959	PASS
68	69	0.00	2	1.0	266	PASS
69	198	0.00	100	26.5	25848	PASS
70	69	0.00	2	0.6	161	PASS
127	198	10	80	37.1	36261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97666	PASS
199	198	5	9	6.8	6598	PASS
275	198	10	60	29.3	28645	PASS
365	198	1	100	4.0	3924	PASS
441	198	0.01	100	11.6	11299	PASS
442	198	50	100	74.3	72605	PASS
443	442	15	24	20.1	14606	PASS