


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG073019\
 Data File : BG041825.D
 Acq On : 31 Jul 2019 6:47
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 08:57:26 2019

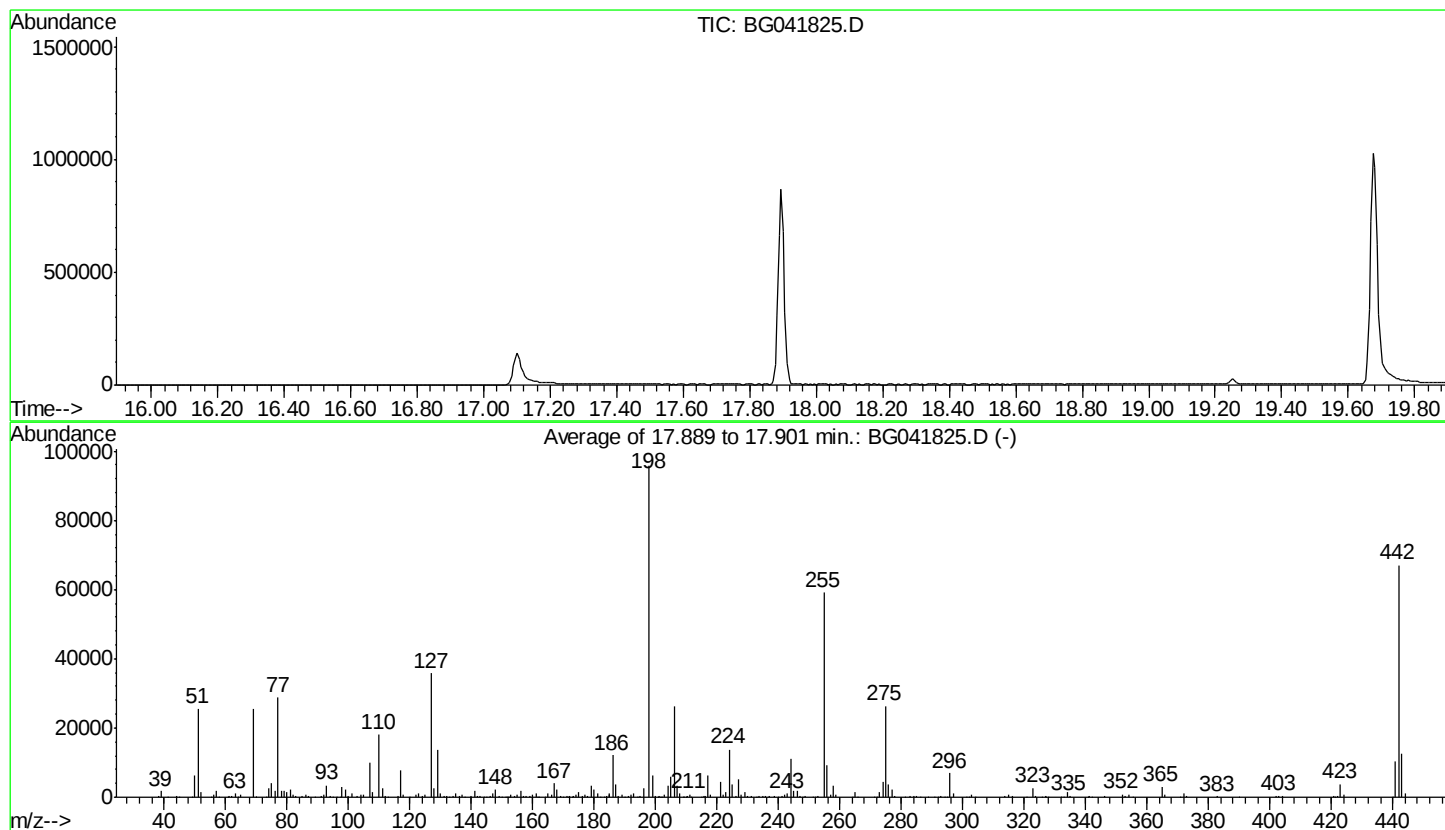

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	25563	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.8	25674	PASS
70	69	0.00	2	0.4	92	PASS
127	198	10	80	37.4	35816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95794	PASS
199	198	5	9	6.7	6389	PASS
275	198	10	60	27.5	26317	PASS
365	198	1	100	3.2	3101	PASS
441	198	0.01	100	10.8	10355	PASS
442	198	50	100	69.9	66989	PASS
443	442	15	24	19.0	12695	PASS