
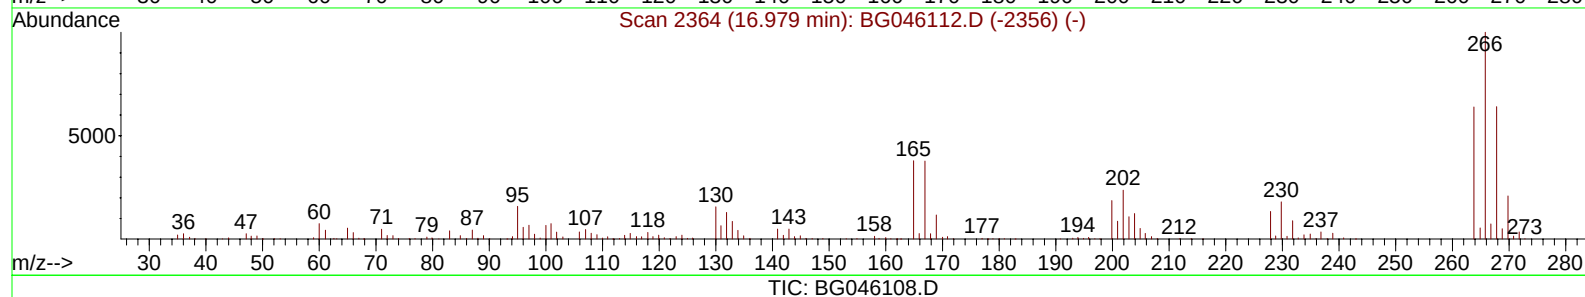
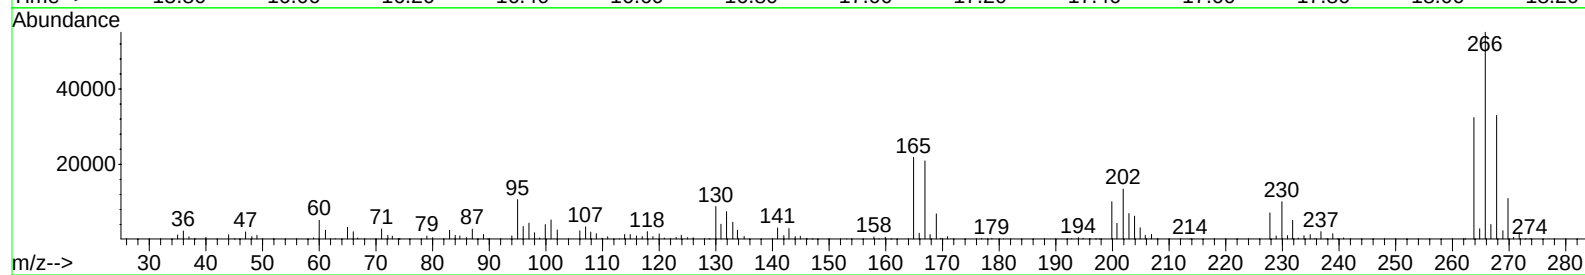


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073020\
Data File : BG046108.D
Acq On : 30 Jul 2020 13:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 18:55:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

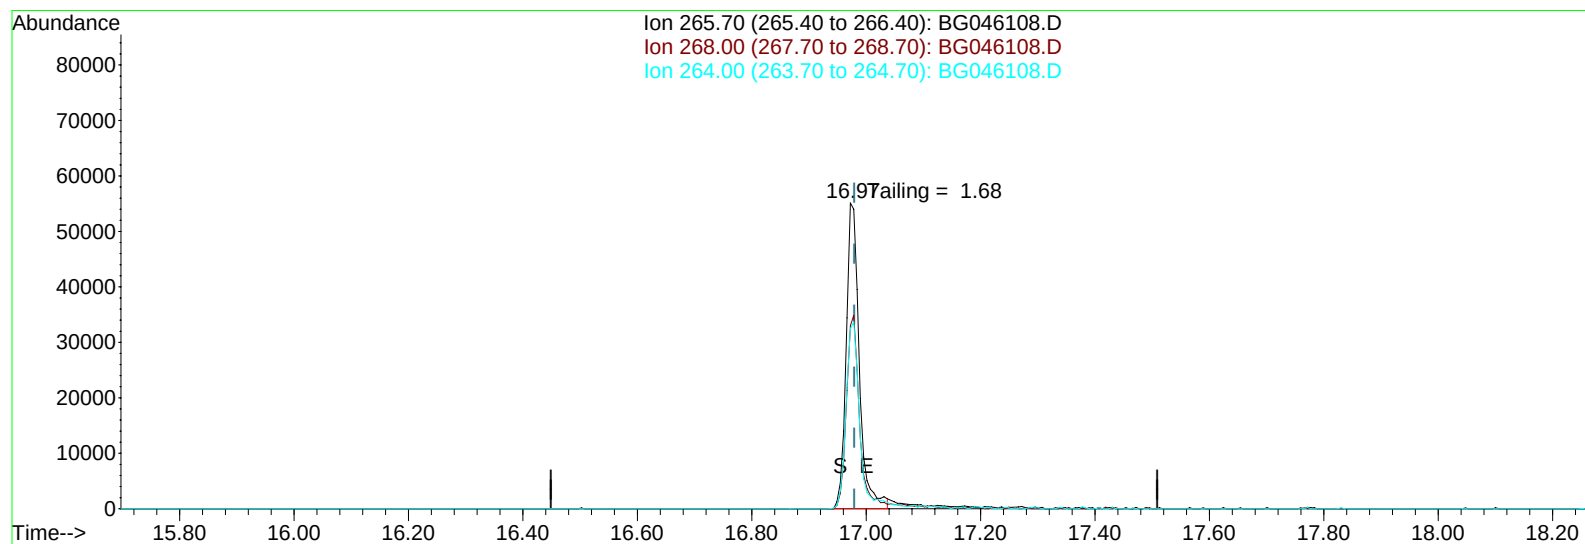

(70) Pentachlorophenol (C)




16.972min (-0.007) 112959.17ng

response 92394

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	59.85
264.00	63.90	58.90
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073020\
Data File : BG046108.D
Acq On : 30 Jul 2020 13:11
Operator : CG/JU
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 18:55:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

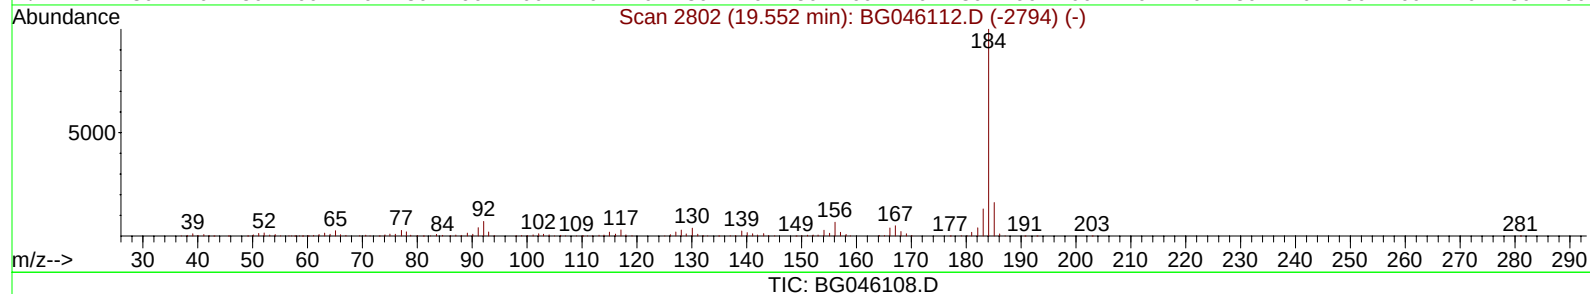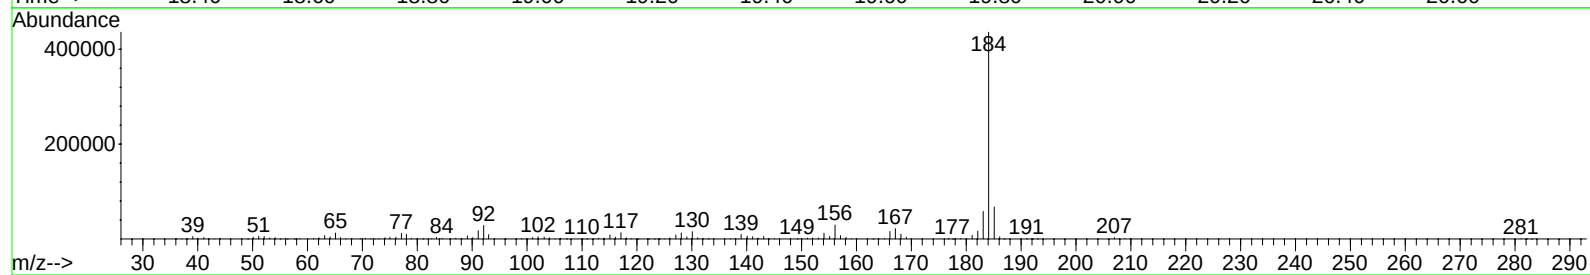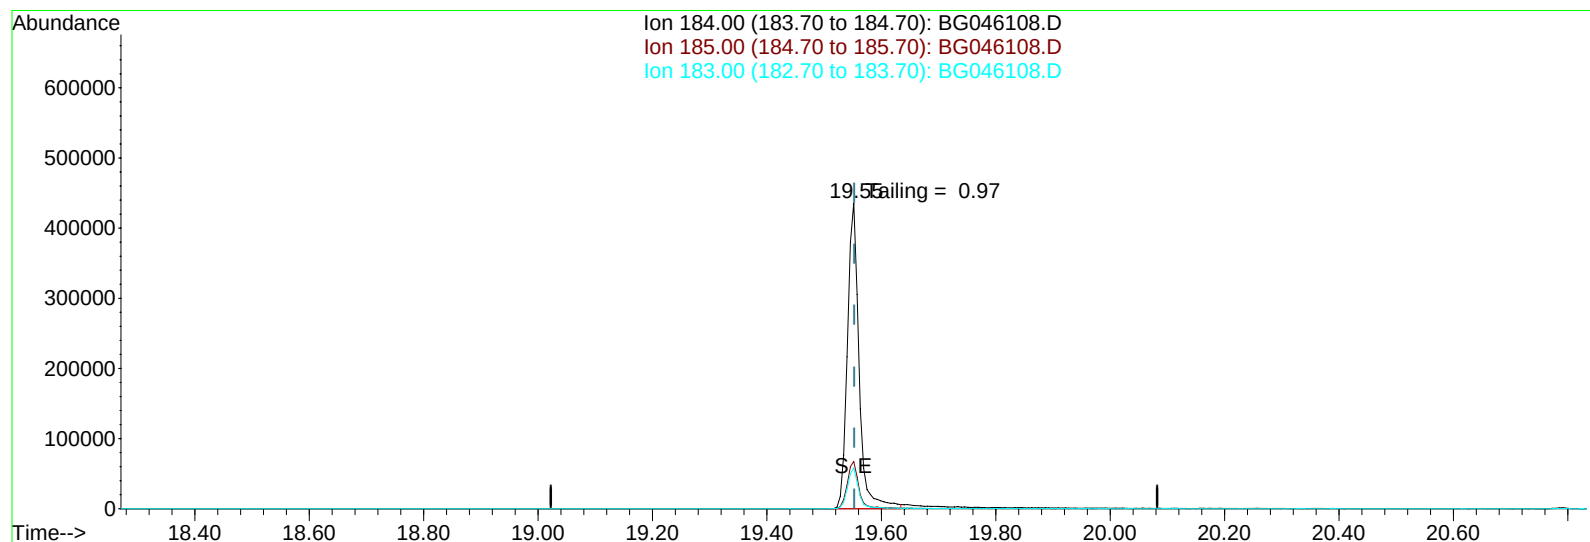

(77) Benzidine

19.552min (-0.001) 8403.70ng

response 643899

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.48
183.00	13.10	13.36
0.00	0.00	0.00