


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073020\
 Data File : BG046108.D
 Acq On : 30 Jul 2020 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 18:43:49 2020

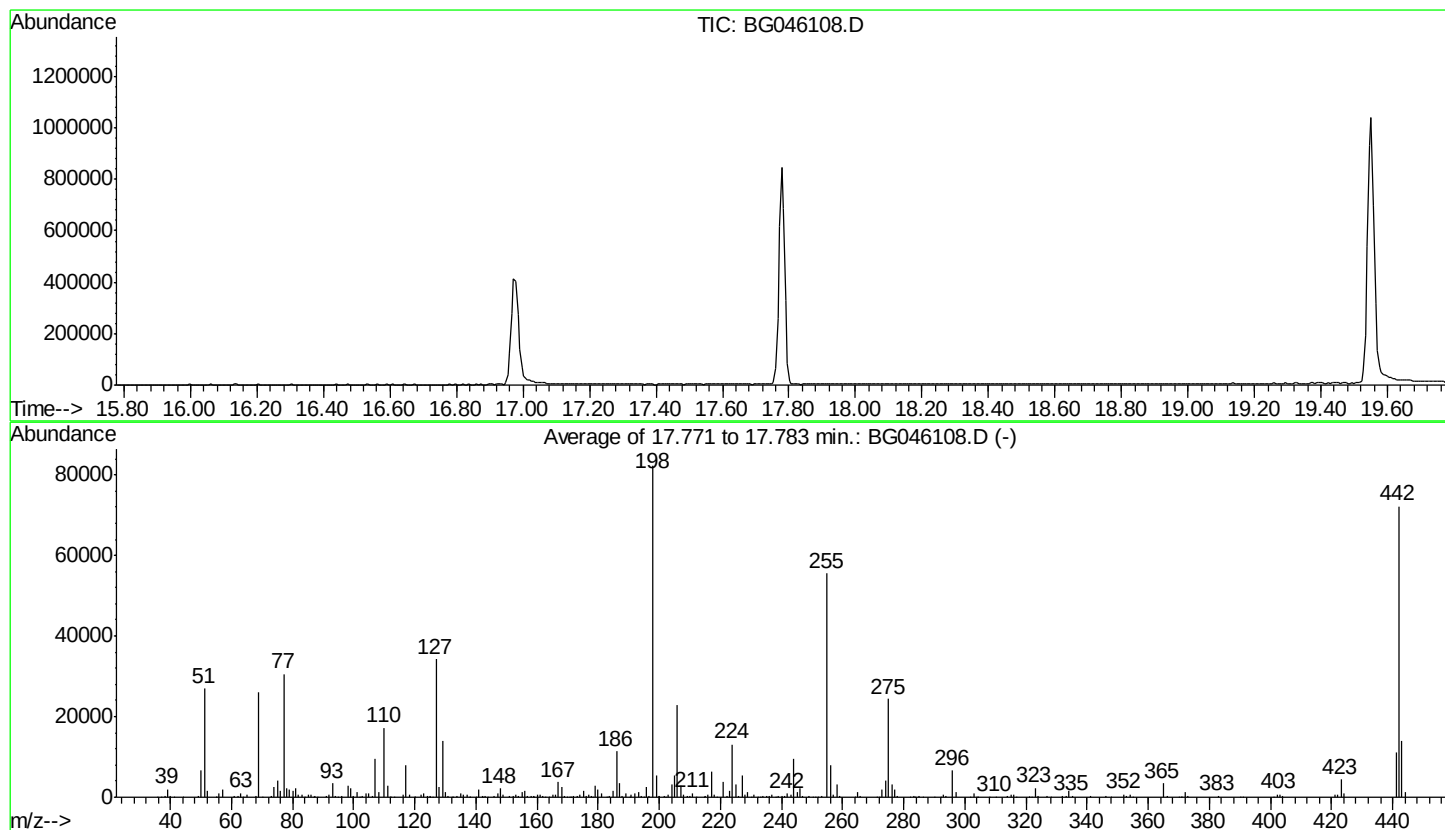

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	26978	PASS
68	69	0.00	2	1.3	335	PASS
69	198	0.00	100	31.5	25909	PASS
70	69	0.00	2	0.2	61	PASS
127	198	10	80	41.6	34218	PASS
197	198	0.00	2	0.4	315	PASS
198	198	100	100	100.0	82274	PASS
199	198	5	9	6.7	5477	PASS
275	198	10	60	29.6	24357	PASS
365	198	1	100	4.1	3363	PASS
441	198	0.01	100	13.5	11100	PASS
442	198	50	100	87.7	72146	PASS
443	442	15	24	19.2	13879	PASS