

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073115\
 Data File : BG018189.D
 Acq On : 31 Jul 2015 20:25
 Operator : TP/UM
 Sample : PB84669BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 01 00:53:53 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG073115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 00:52:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	28815	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	137698	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	100298	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.91	188	257869	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	285008	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	249970	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.97	96	3659	9.59	ng/uL	0.00
5) Phenol-d5	6.67	99	92468	35.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	54034	40.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	73502	37.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	75553	35.81	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	42014	38.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	48866	39.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	78285	35.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	118234	43.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	318720	41.12	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	360283	40.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	56264	39.22	ng/ul	0.00
58) Fluorene-d10	15.15	176	279540	39.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.28	200	58587	32.54	ng/ul	0.00
71) Anthracene-d10	17.01	188	451769	40.29	ng/ul	0.00
79) Pyrene-d10	19.32	212	522597	37.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	534935	42.32	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.20	70	1937	1.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073115\
Data File : BG018189.D
Acq On : 31 Jul 2015 20:25
Operator : TP/UM
Sample : PB84669BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 01 00:53:53 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 00:52:12 2015
Response via : Initial Calibration

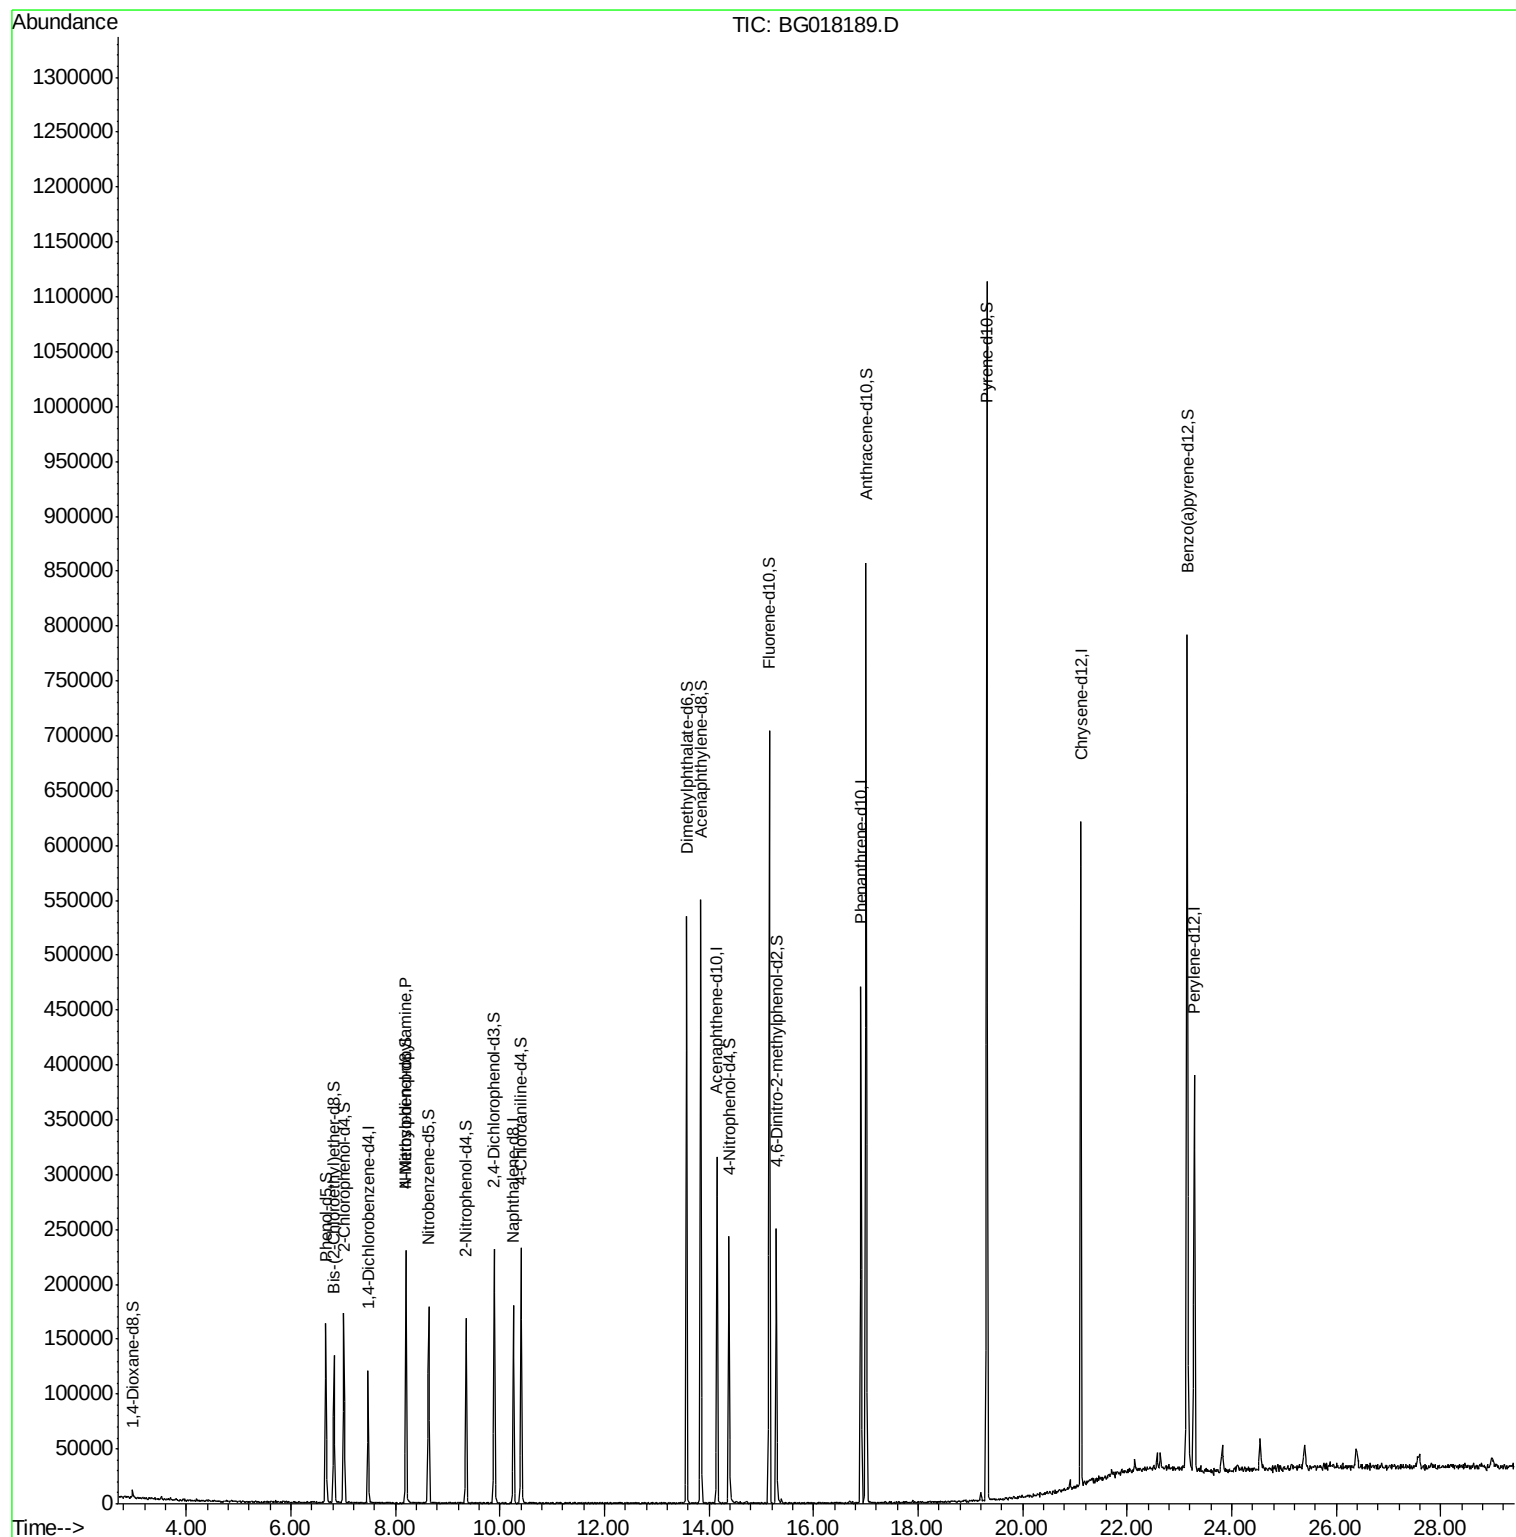

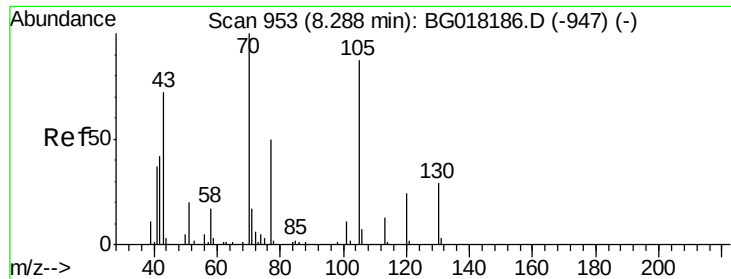

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.04 ng/ul
 RT: 8.20 min Scan# 938
 Delta R.T. -0.09 min
 Lab File: BG018189.D
 Acq: 31 Jul 2015 20:25

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 70 Resp: 1937
 Ion Ratio Lower Upper
 70 100
 42 357.5 36.5 54.7#
 101 0.0 10.2 15.4#
 130 0.0 30.7 46.1#

