

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073115\
 Data File : BG018192.D
 Acq On : 31 Jul 2015 22:10
 Operator : TP/UM
 Sample : G3073-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 01 00:54:11 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG073115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 00:52:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	27878	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	135191	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	97602	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.91	188	241708	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	275113	20.00	ng/ul	0.00
86) Perylene-d12	23.28	264	255373	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.97	96	2806	7.60	ng/uL	0.00
5) Phenol-d5	6.67	99	76610	30.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	42834	33.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	60505	31.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	65550	32.11	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	34410	32.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	40723	33.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	64909	30.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	96121	35.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	272040	36.07	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	288647	33.01	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	49084	35.16	ng/ul	0.00
58) Fluorene-d10	15.15	176	222004	32.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	48343	28.65	ng/ul	0.00
71) Anthracene-d10	17.00	188	348535	33.16	ng/ul	0.00
79) Pyrene-d10	19.32	212	383395	28.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	389662	30.17	ng/ul	0.00

Target Compounds


						Ovalue
15) N-Nitroso-di-n-propylamine	8.20	70	1833	1.02	ng/ul#	1
45) Dimethylphthalate	13.61	163	99341	13.24	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073115\
Data File : BG018192.D
Acq On : 31 Jul 2015 22:10
Operator : TP/UM
Sample : G3073-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 01 00:54:11 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 00:52:12 2015
Response via : Initial Calibration




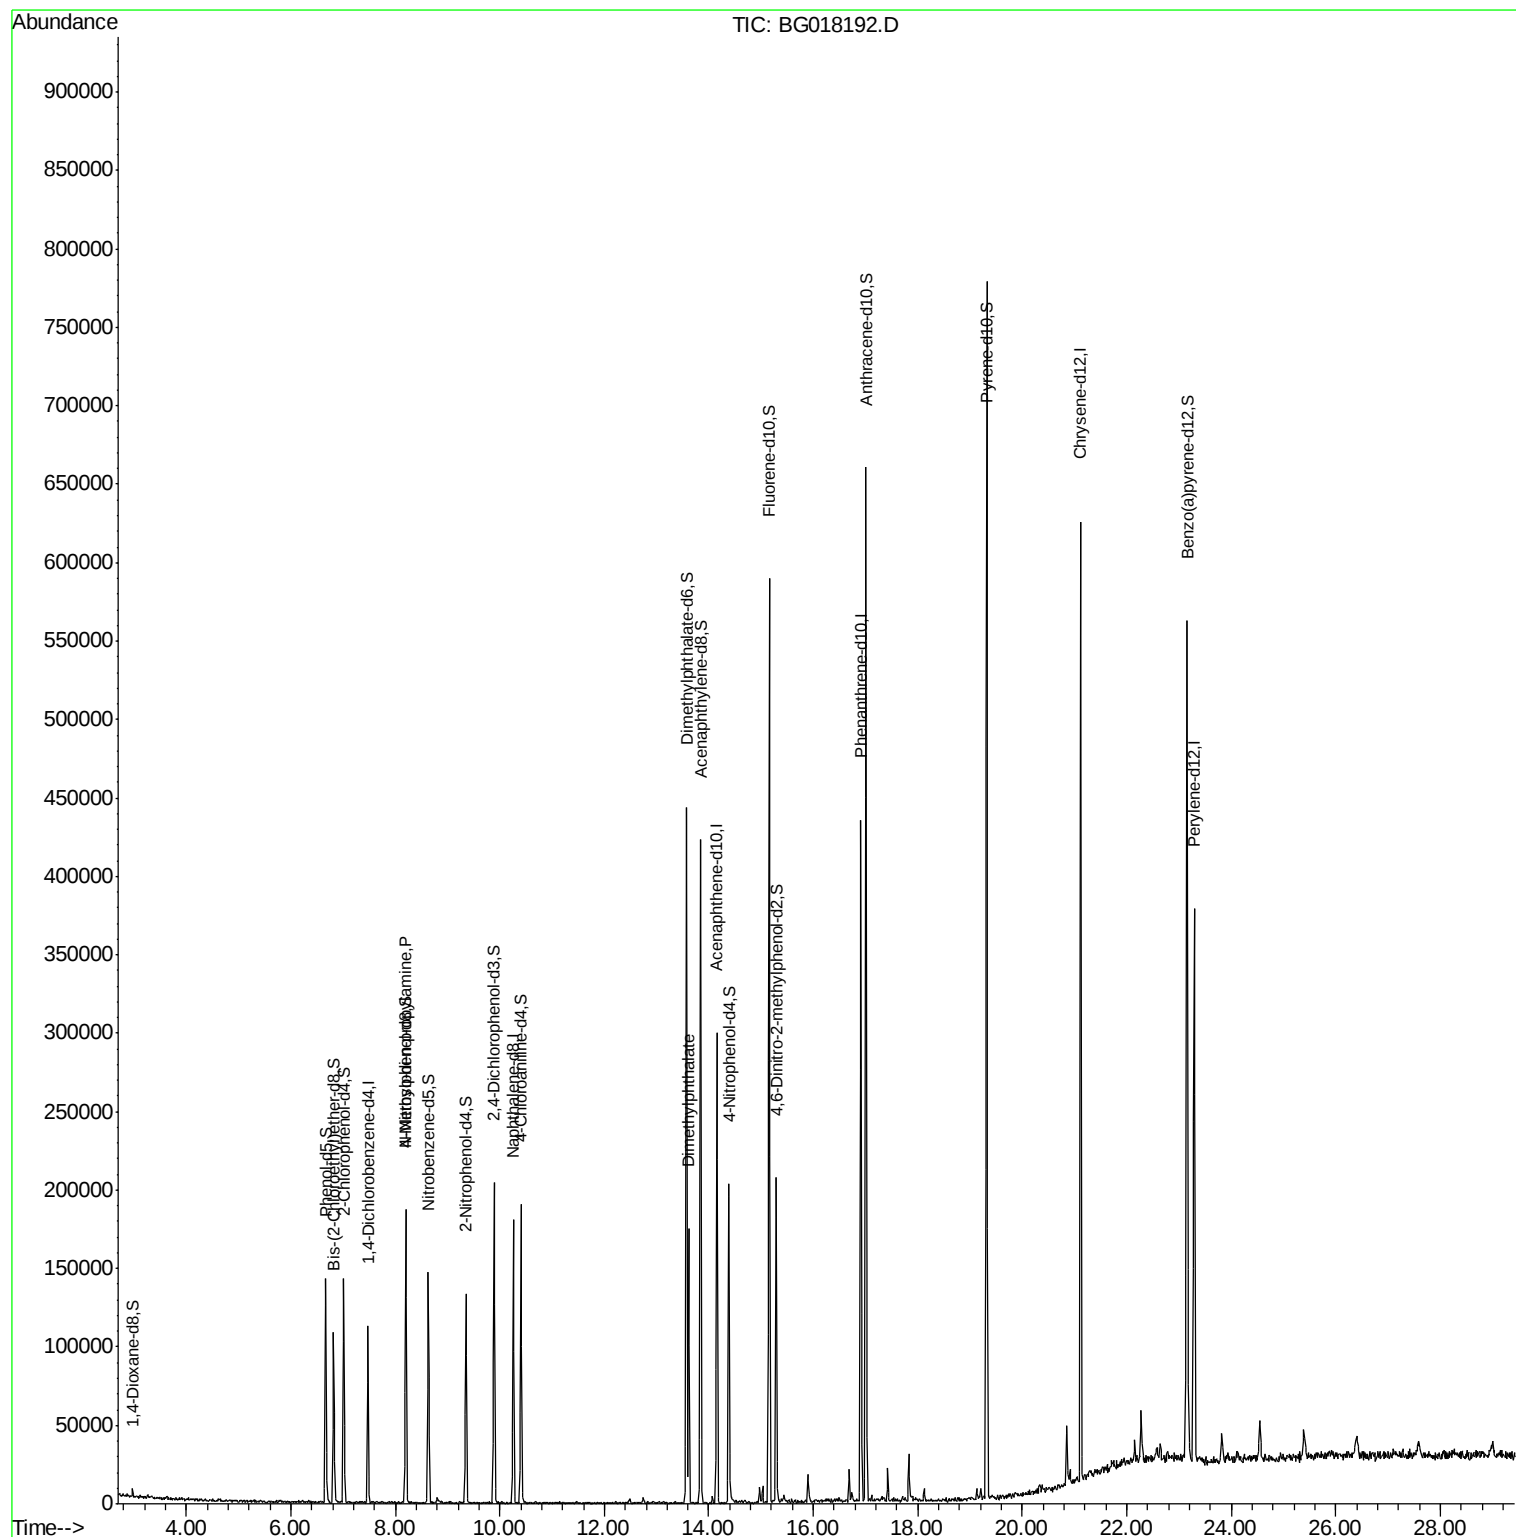


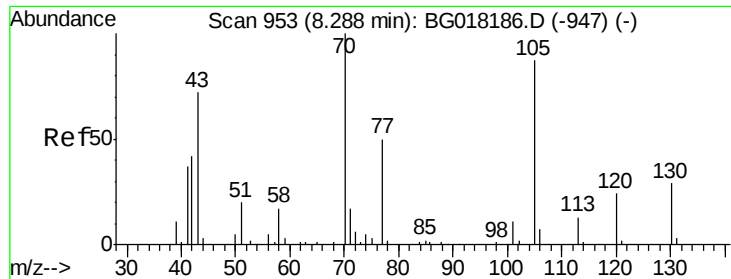

#15
N-Nitroso-di-n-propylamine
Concen: 1.02 ng/ul
RT: 8.20 min Scan# 938
Delta R.T. -0.09 min
Lab File: BG018192.D
Acq: 31 Jul 2015 22:10

Instrument :
BNA_G
ClientSampled :

Tot Ion: 70 Resp: 1833
Ion Ratio Lower Upper
70 100
42 281.4 36.5 54.7#
101 0.0 10.2 15.4#
130 0.0 30.7 46.1#

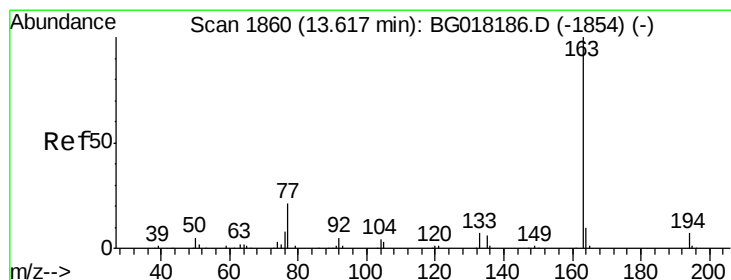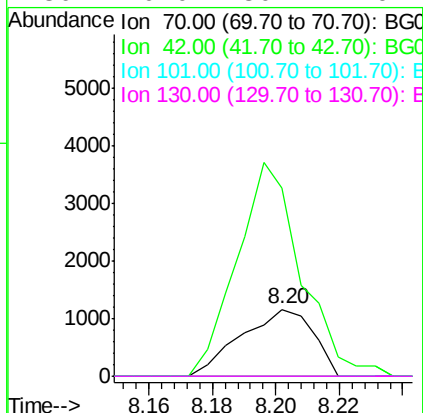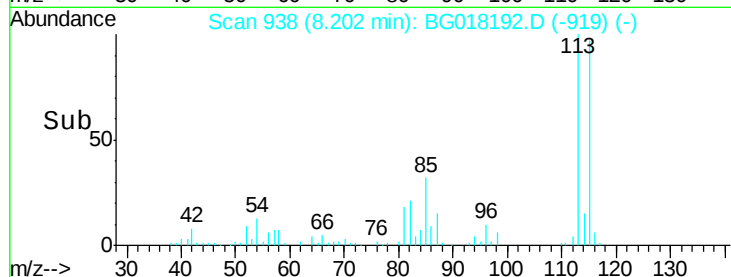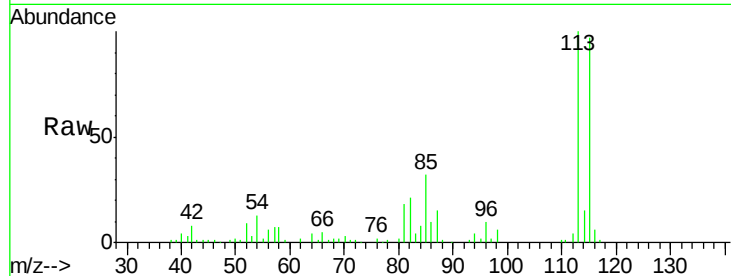

#45
Dimethylphthalate
Concen: 13.24 ng/ul
RT: 13.61 min Scan# 1859
Delta R.T. -0.00 min
Lab File: BG018192.D
Acq: 31 Jul 2015 22:10

Tgt Ion: 163 Resp: 99341
Ion Ratio Lower Upper
163 100
194 6.3 5.2 7.8
164 9.4 8.4 12.6

