

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
 Data File : BG018193.D
 Acq On : 31 Jul 2015 22:45
 Operator : TP/UM
 Sample : G3073-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01R2

Quant Time: Aug 01 01:15:37 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 00:52:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	30034	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	141430	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	104401	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.91	188	253081	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	288112	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	273642	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.97	96	2503	6.29	ng/uL	0.00
5) Phenol-d5	6.66	99	76107	28.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	44923	32.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	61887	30.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	66129	30.07	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	35824	32.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	40704	31.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	69275	30.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	94311	33.49	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	272265	33.75	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	300300	32.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	48859	32.72	ng/ul	0.00
58) Fluorene-d10	15.15	176	233633	32.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.28	200	52203	29.54	ng/ul	0.00
71) Anthracene-d10	17.01	188	367252	33.37	ng/ul	0.00
79) Pyrene-d10	19.31	212	412509	29.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	429784	31.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.62	163	98844	12.31	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018193.D
Acq On : 31 Jul 2015 22:45
Operator : TP/UM
Sample : G3073-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01R2

Quant Time: Aug 01 01:15:37 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 00:52:12 2015
Response via : Initial Calibration

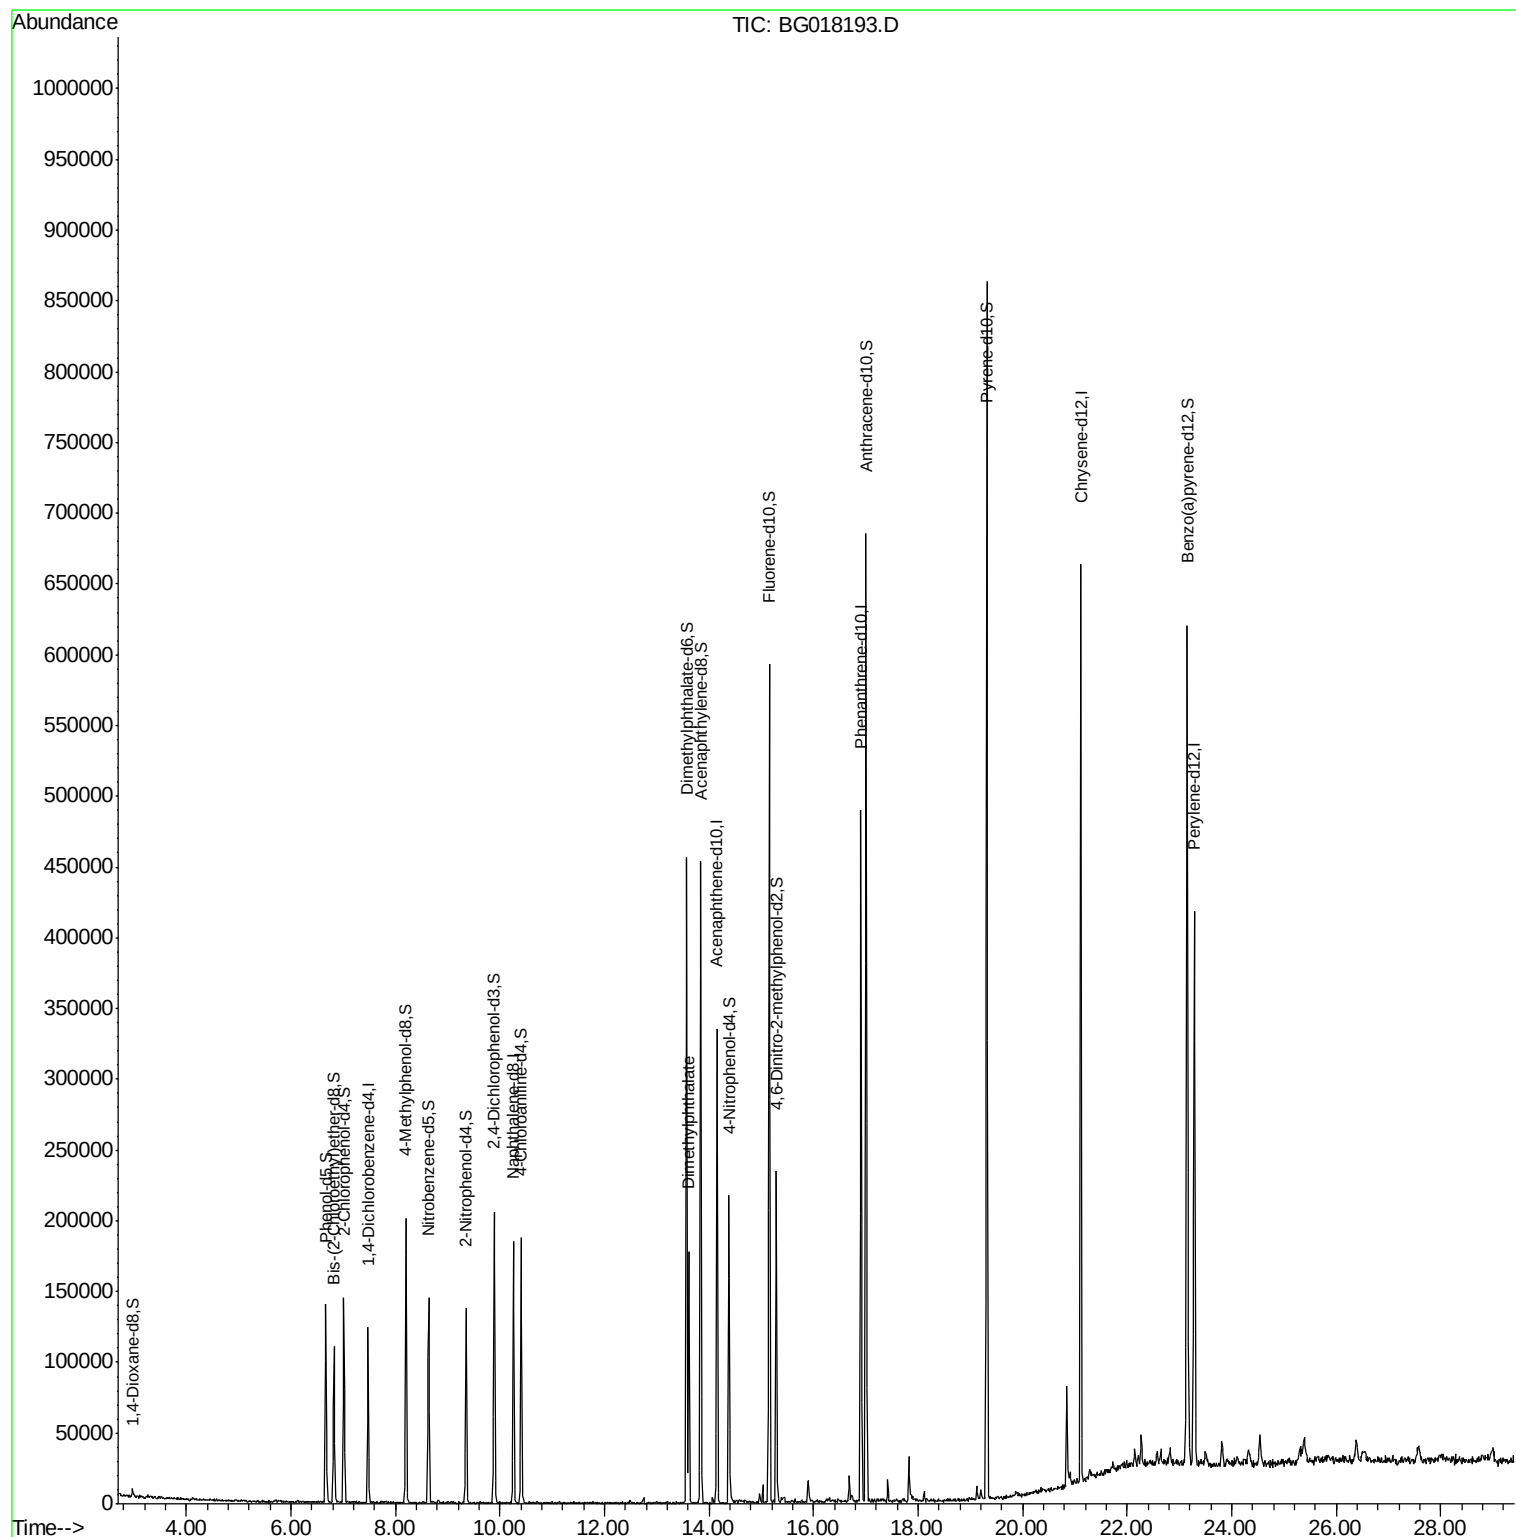

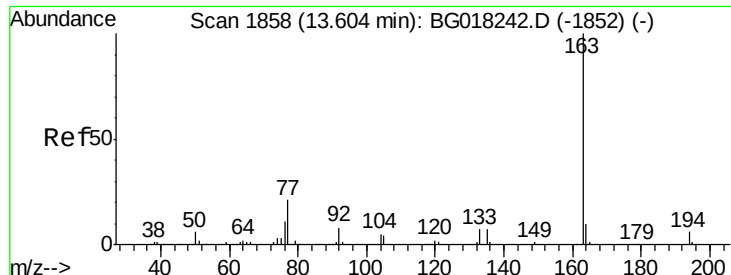

#45

Dimethylphthalate

Concen: 12.31 ng/ul

RT: 13.62 min Scan# 1860

Delta R.T. -0.00 min

Lab File: BG018193.D


Acq: 31 Jul 2015 22:45

Instrument :

BNA_G

ClientSampleId :

C01R2

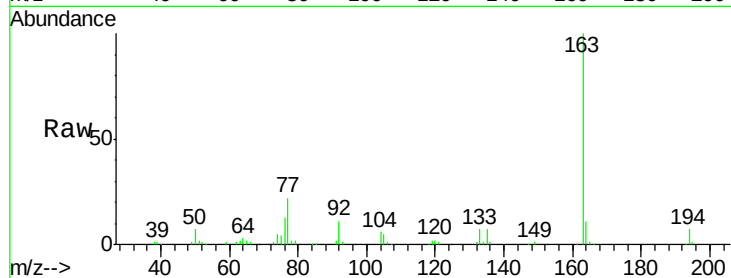

Tgt Ion:163 Resp: 98844

Ion Ratio Lower Upper

163 100

194 6.8 5.2 7.8

164 10.6 8.4 12.6

