

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
 Data File : BG018194.D
 Acq On : 31 Jul 2015 23:21
 Operator : TP/UM
 Sample : G3073-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01L8

Manual Integrations
 APPROVED

MMDadoda
 8/4/2015 12:22:13 PM

Quant Time: Aug 01 01:19:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 00:52:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	29480	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	133023	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	97776	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	243353m	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	283080	20.00	ng/ul	0.00
86) Perylene-d12	23.28	264	265647	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.97	96	2093	5.36	ng/uL	0.00
5) Phenol-d5	6.67	99	62285	23.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	34151	25.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	48319	24.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	52505	24.32	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	27606	26.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	31593	26.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	54840	25.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	76582	28.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	213389	28.24	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	227533	25.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.38	143	37018	26.47	ng/ul	0.00
58) Fluorene-d10	15.15	176	176471	25.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.29	200	38407m	22.60	ng/ul	0.00
71) Anthracene-d10	17.00	188	287795	27.20	ng/ul	0.00
79) Pyrene-d10	19.31	212	318069	23.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	347400	25.86	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.61	163	59366	7.90	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018194.D
Acq On : 31 Jul 2015 23:21
Operator : TP/UM
Sample : G3073-05
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C01L8

Manual Integrations
APPROVED

MMDadoda
8/4/2015 12:22:13 PM

Quant Time: Aug 01 01:19:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 00:52:12 2015
Response via : Initial Calibration

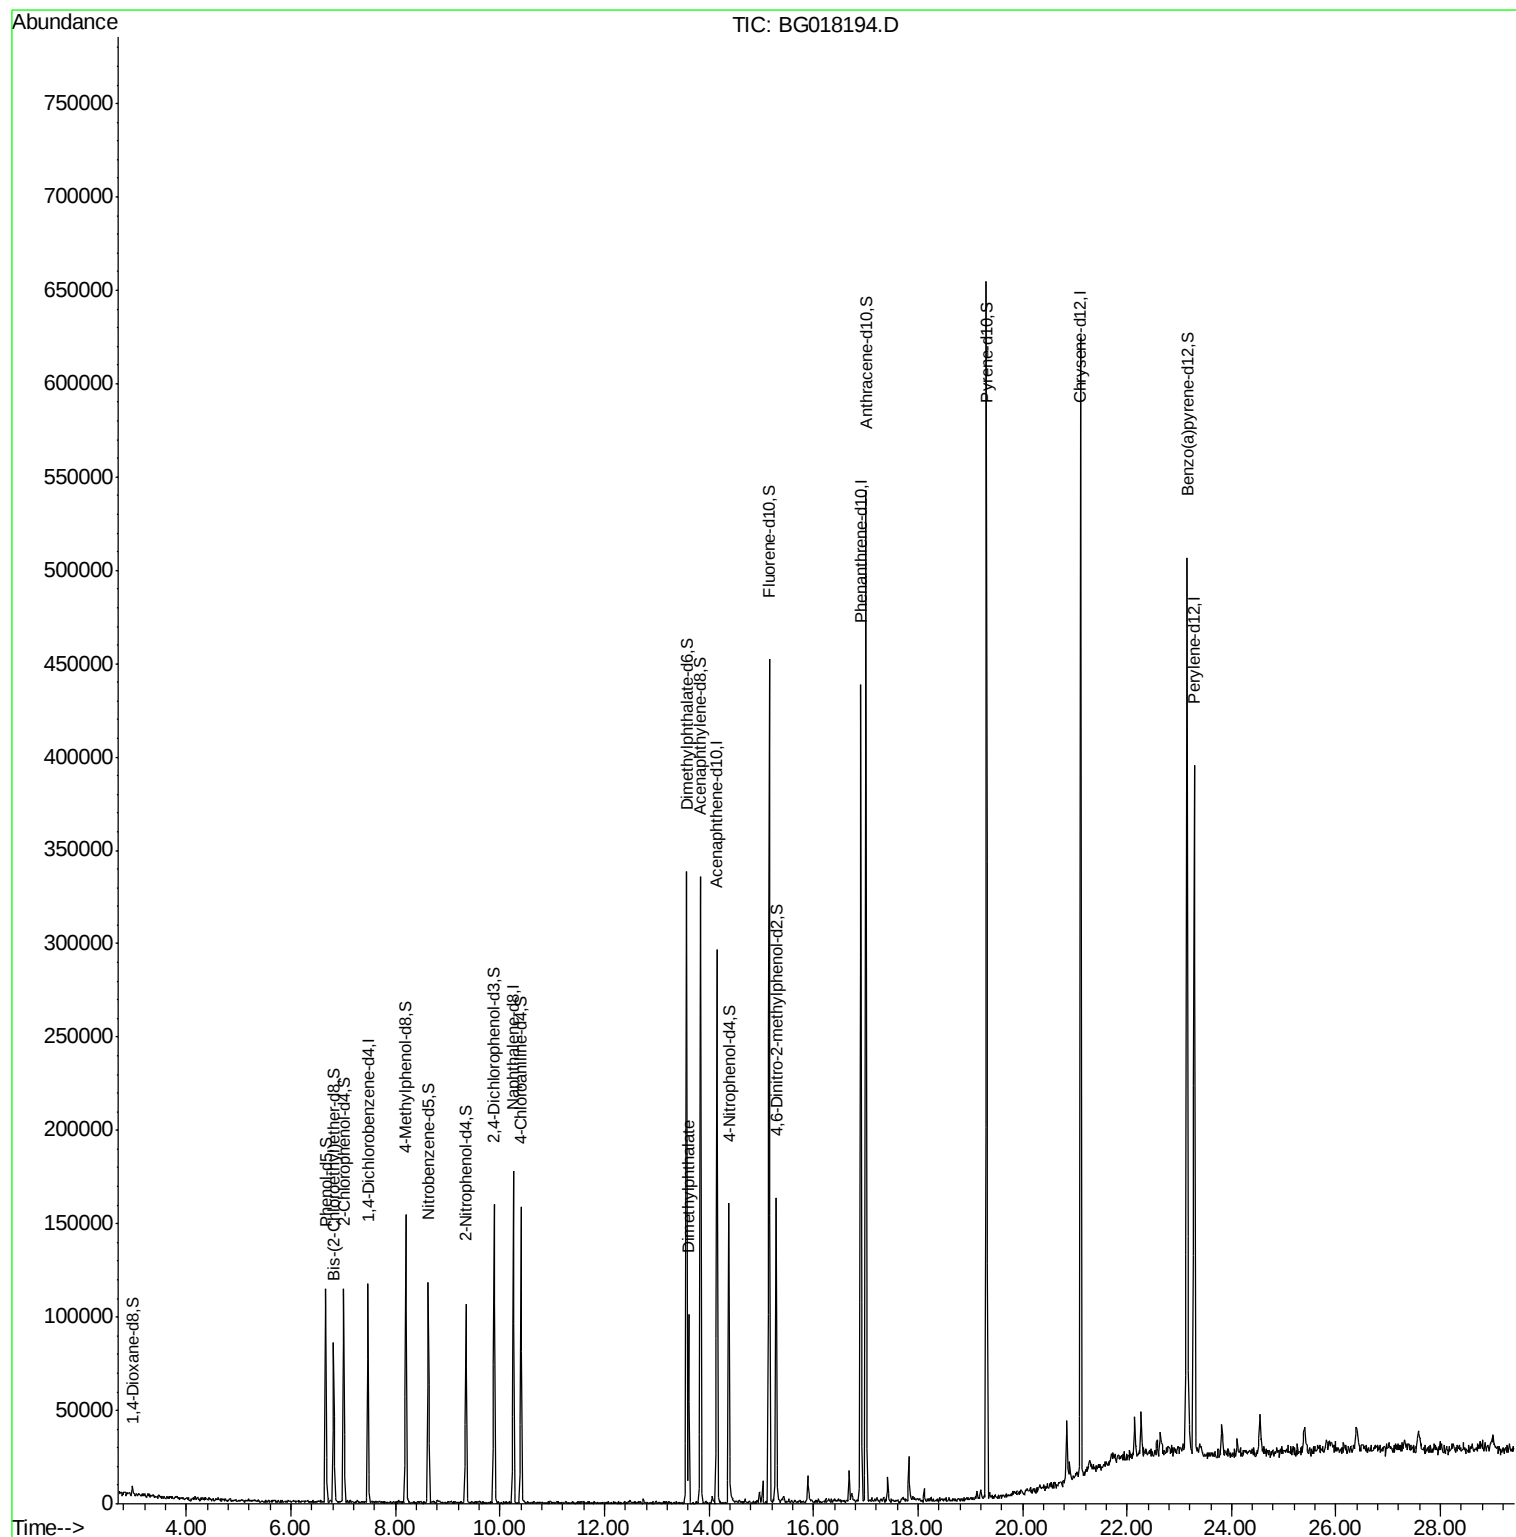

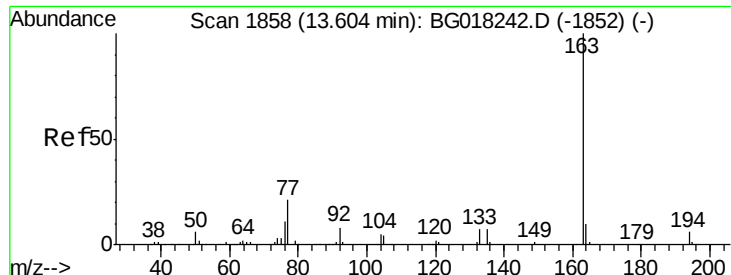


#45
 Dimethylphthalate
 Concen: 7.90 ng/ul
 RT: 13.61 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BG018194.D
 Acq: 31 Jul 2015 23:21

Instrument :
 BNA_G
 ClientSampleId :
 C01L8

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	6.5	5.2	7.8
164	10.5	8.4	12.6

Manual Integrations
 APPROVED

MMDadoda
 8/4/2015 12:22:13 PM

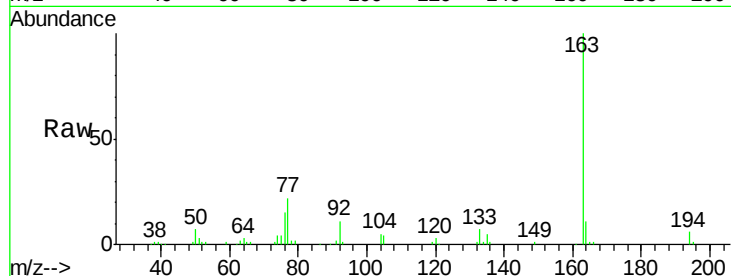

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

