

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
 Data File : BG018187.D
 Acq On : 31 Jul 2015 17:58
 Operator : TP/UM
 Sample : PB84763BL
 Misc : SBLK63
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.741	7	9	12	rVB3	1671	1704	0.12%	0.013%
2	2.823	21	23	24	rVB2	2779	1695	0.12%	0.013%
3	2.970	45	48	53	rBV3	6928	9765	0.67%	0.075%
4	3.522	138	142	144	rVB3	2926	2722	0.19%	0.021%
5	3.698	170	172	176	rBV3	2315	2955	0.20%	0.023%
6	3.986	219	221	224	rBV2	1498	1621	0.11%	0.012%
7	4.433	296	297	301	rVB	1500	1561	0.11%	0.012%
8	4.462	301	302	307	rBV2	1102	1663	0.11%	0.013%
9	4.686	336	340	343	rBV2	1326	2075	0.14%	0.016%
10	5.878	537	543	546	rBV2	1173	1701	0.12%	0.013%
11	6.143	585	588	591	rBV	952	1569	0.11%	0.012%
12	6.671	670	678	686	rBV	176062	274543	18.90%	2.102%
13	6.824	698	704	712	rBV	143641	210697	14.50%	1.613%
14	6.918	718	720	723	rVB2	1670	1961	0.13%	0.015%
15	7.012	729	736	744	rBV	185059	282121	19.42%	2.160%
16	7.476	809	815	823	rVV	132093	202252	13.92%	1.548%
17	7.565	825	830	834	rVB3	1205	1702	0.12%	0.013%
18	8.199	932	938	945	rBV	237999	369704	25.45%	2.830%
19	8.634	1005	1012	1019	rVB	187686	302052	20.79%	2.312%
20	9.351	1127	1134	1142	rBV	177261	285382	19.64%	2.185%
21	9.891	1219	1226	1239	rVB	244456	395761	27.24%	3.029%
22	10.261	1283	1289	1297	rVB	193935	316127	21.76%	2.420%
23	10.408	1306	1314	1325	rBV	243433	404637	27.85%	3.097%
24	12.600	1682	1687	1690	rBV2	1324	1918	0.13%	0.015%
25	13.569	1846	1852	1859	rVB	554980	730387	50.27%	5.591%
26	13.840	1892	1898	1905	rVB	532832	784668	54.01%	6.006%
27	14.151	1943	1951	1958	rBV2	317903	477573	32.87%	3.656%
28	14.386	1985	1991	1999	rVV	243245	359214	24.73%	2.750%
29	14.439	1999	2000	2003	rVB2	2710	2264	0.16%	0.017%
30	15.156	2115	2122	2130	rVB	721013	1011726	69.64%	7.744%
31	15.291	2139	2145	2156	rBV	245250	353041	24.30%	2.702%
32	15.397	2158	2163	2166	rBV3	3954	6709	0.46%	0.051%
33	15.784	2228	2229	2234	rBV	1359	1472	0.10%	0.011%
34	16.107	2280	2284	2287	rBV2	2326	1882	0.13%	0.014%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
 Data File : BG018187.D
 Acq On : 31 Jul 2015 17:58
 Operator : TP/UM
 Sample : PB84763BL
 Misc : SBLK63
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Title : SVOA CALIBRATION

35	16.695	2380	2384	2388	rBV	2018	2957	0.20%	0.023%
36	16.907	2414	2420	2426	rBV2	483146	651425	44.84%	4.986%
37	17.006	2431	2437	2443	rVV	893783	1206304	83.03%	9.234%
38	17.065	2445	2447	2450	rVB	1513	1624	0.11%	0.012%
39	17.424	2504	2508	2510	rVB2	1299	1697	0.12%	0.013%
40	17.758	2562	2565	2568	rBV2	1182	1522	0.10%	0.012%
41	18.475	2686	2687	2690	rBV2	2058	1725	0.12%	0.013%
42	18.552	2696	2700	2701	rBV3	1090	1692	0.12%	0.013%
43	19.075	2788	2789	2793	rBV2	1544	1657	0.11%	0.013%
44	19.204	2806	2811	2817	rVB3	9345	12962	0.89%	0.099%
45	19.315	2824	2830	2837	rVV	1111724	1452809	100.00%	11.121%
46	19.439	2850	2851	2854	rVB3	1891	1800	0.12%	0.014%
47	19.468	2854	2856	2859	rBV3	2318	2714	0.19%	0.021%
48	19.509	2861	2863	2866	rBV2	2461	2929	0.20%	0.022%
49	19.650	2885	2887	2889	rVB	3199	1801	0.12%	0.014%
50	19.686	2889	2893	2895	rBV3	2180	3447	0.24%	0.026%
51	19.727	2899	2900	2903	rVB3	3197	2815	0.19%	0.022%
52	19.756	2903	2905	2908	rBV2	2500	3075	0.21%	0.024%
53	19.821	2913	2916	2919	rVB4	1807	2073	0.14%	0.016%
54	19.874	2923	2925	2927	rBV2	2523	2344	0.16%	0.018%
55	19.897	2927	2929	2931	rBV3	2554	2302	0.16%	0.018%
56	19.932	2931	2935	2936	rBV2	1860	1979	0.14%	0.015%
57	19.979	2940	2943	2946	rBV3	1759	2459	0.17%	0.019%
58	20.091	2960	2962	2964	rBV2	2084	1752	0.12%	0.013%
59	20.173	2973	2976	2977	rBV3	1638	1919	0.13%	0.015%
60	20.214	2981	2983	2984	rVB2	2961	1713	0.12%	0.013%
61	20.297	2993	2997	2998	rBV4	3333	4377	0.30%	0.034%
62	20.391	3012	3013	3015	rBV2	3041	2225	0.15%	0.017%
63	20.532	3035	3037	3038	rVB2	2786	1488	0.10%	0.011%
64	20.549	3038	3040	3042	rBV3	1904	1851	0.13%	0.014%
65	20.679	3059	3062	3065	rBV5	4772	6405	0.44%	0.049%
66	20.726	3068	3070	3071	rVV2	2984	2045	0.14%	0.016%
67	20.849	3088	3091	3094	rBV5	3264	5069	0.35%	0.039%
68	20.914	3098	3102	3106	rVB6	8878	13190	0.91%	0.101%
69	21.113	3131	3136	3141	rBV	658288	779050	53.62%	5.963%
70	21.272	3161	3163	3167	rBV4	3959	6433	0.44%	0.049%
71	22.788	3419	3421	3424	rBV4	6329	6310	0.43%	0.048%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018187.D
Acq On : 31 Jul 2015 17:58
Operator : TP/UM
Sample : PB84763BL
Misc : SBLK63
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Title : SVOA CALIBRATION

72	23.152	3475	3483	3496	rVV	737773	1353229	93.15%	10.359%
73	23.287	3499	3506	3514	rVB	374640	657966	45.29%	5.037%
74	23.428	3528	3530	3531	rBV2	6426	5245	0.36%	0.040%
75	23.751	3583	3585	3586	rBV2	5705	4260	0.29%	0.033%
76	23.816	3593	3596	3601	rVB6	9126	16752	1.15%	0.128%
77	24.075	3638	3640	3641	rVB2	7728	3474	0.24%	0.027%
78	24.486	3708	3710	3713	rVB3	7903	6020	0.41%	0.046%
79	25.444	3871	3873	3875	rBV3	6147	4567	0.31%	0.035%
80	28.422	4378	4380	4381	rBV	7479	5582	0.38%	0.043%


Sum of corrected areas: 13063858

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018187.D
Acq On : 31 Jul 2015 17:58
Operator : TP/UM
Sample : PB84763BL
Misc : SBLK63
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

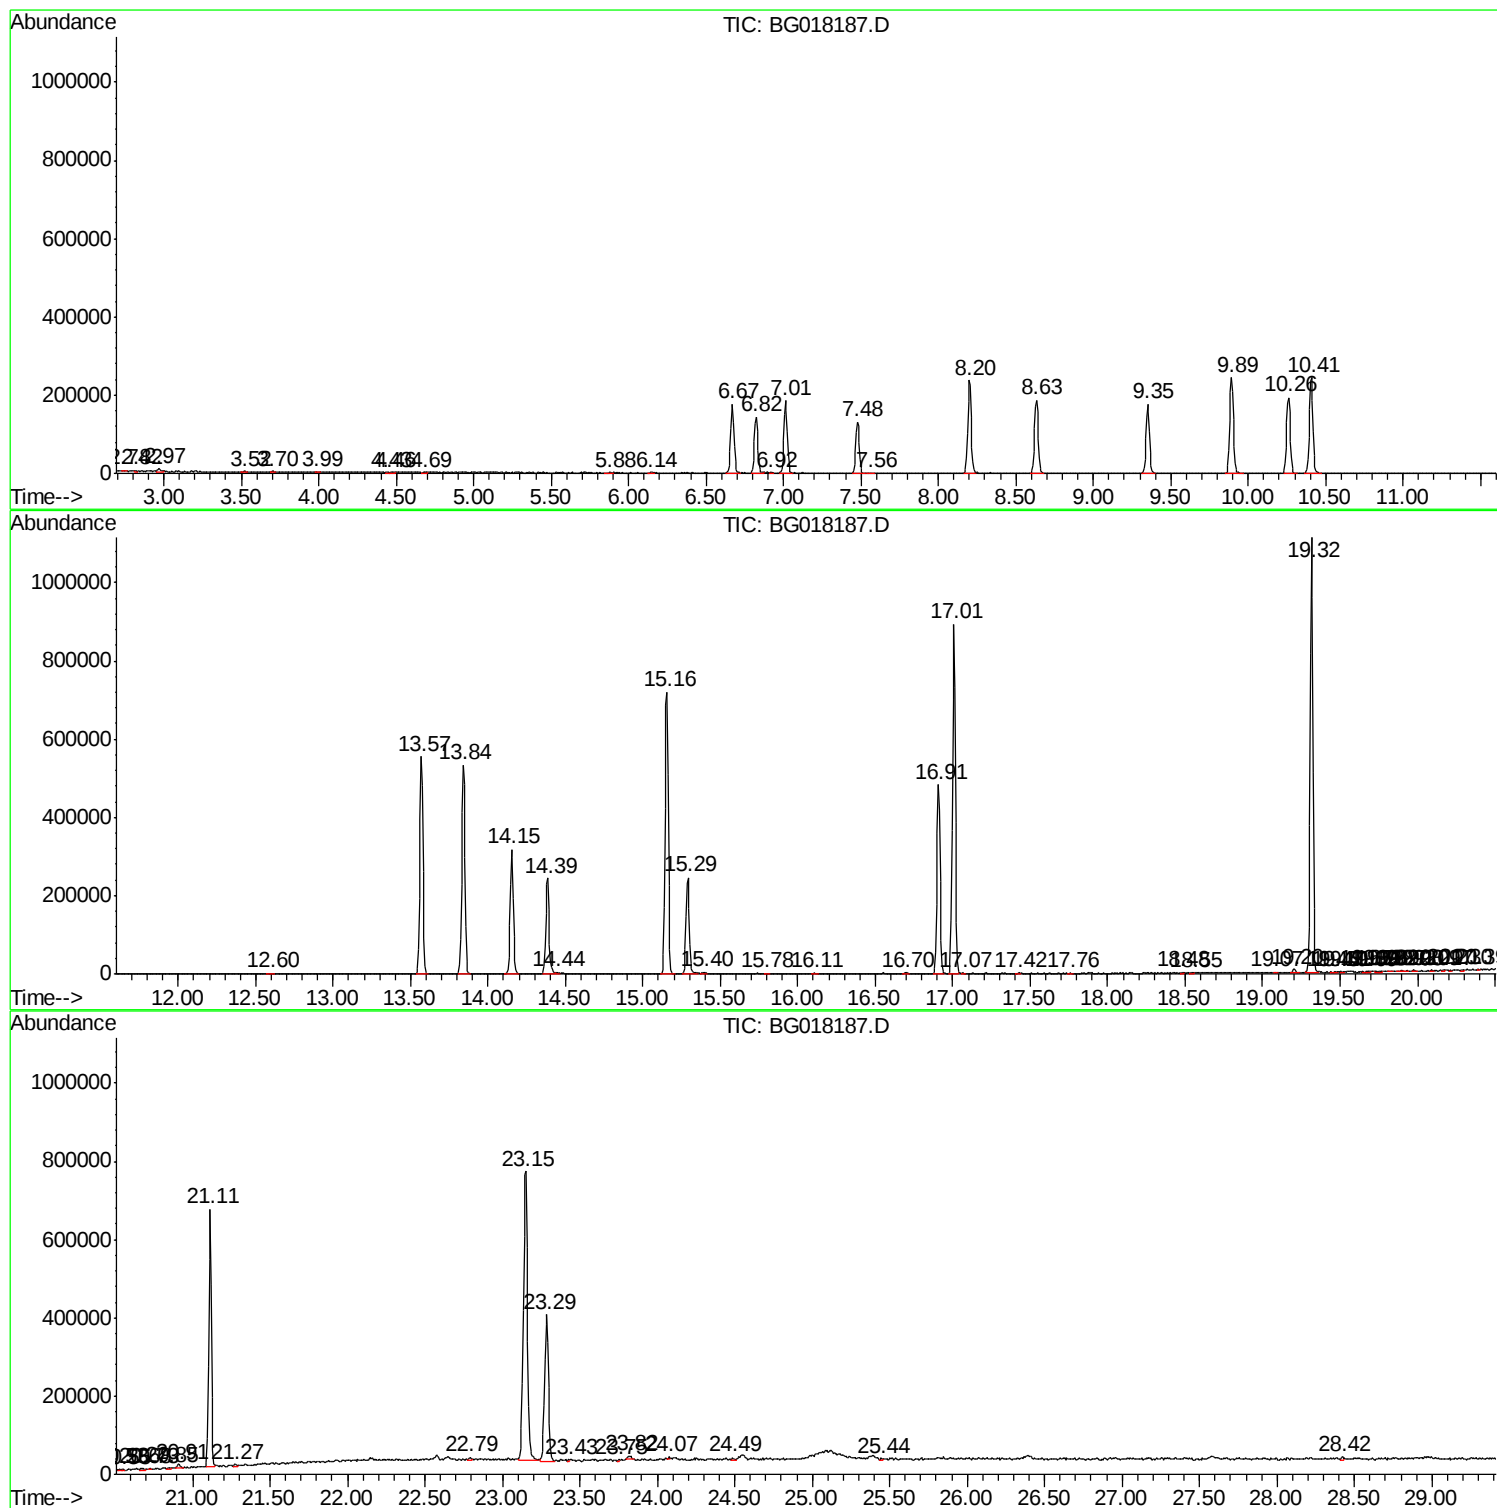

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018187.D
Acq On : 31 Jul 2015 17:58
Operator : TP/UM
Sample : PB84763BL
Misc : SBLK63
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073115\
Data File : BG018187.D
Acq On : 31 Jul 2015 17:58
Operator : TP/UM
Sample : PB84763BL
Misc : SBLK63
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK63

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc