

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073116\
 Data File : BG023364.D
 Acq On : 30 Jul 2016 19:30
 Operator : UM/SJ
 Sample : H4223-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 01 01:24:49 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 27 17:30:33 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	178005	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	883150	20.00	ng	0.00
38) Acenaphthene-d10	14.81	164	615935	20.00	ng	0.00
63) Phenanthrene-d10	17.57	188	1158953	20.00	ng	0.00
75) Chrysene-d12	21.88	240	1022438	20.00	ng	0.00
86) Perylene-d12	25.28	264	1040805	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	898036	86.13	ng	0.00
7) Phenol-d6	7.29	99	1653535	103.29	ng	0.00
23) Nitrobenzene-d5	9.31	82	1176779	65.16	ng	0.00
41) 2,4,6-Tribromophenol	16.30	330	453016	71.06	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	2466114	74.94	ng	0.00
78) Terphenyl-d14	20.17	244	2384147	75.80	ng	0.00
Target Compounds						
10) Phenol	7.32	94	40315	2.39	ng	89
32) Benzoic acid	10.27	122	55	8.11	ng	# 27
49) Dimethylphthalate	14.25	163	500198	11.00	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073116\
Data File : BG023364.D
Acq On : 30 Jul 2016 19:30
Operator : UM/SJ
Sample : H4223-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 01 01:24:49 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

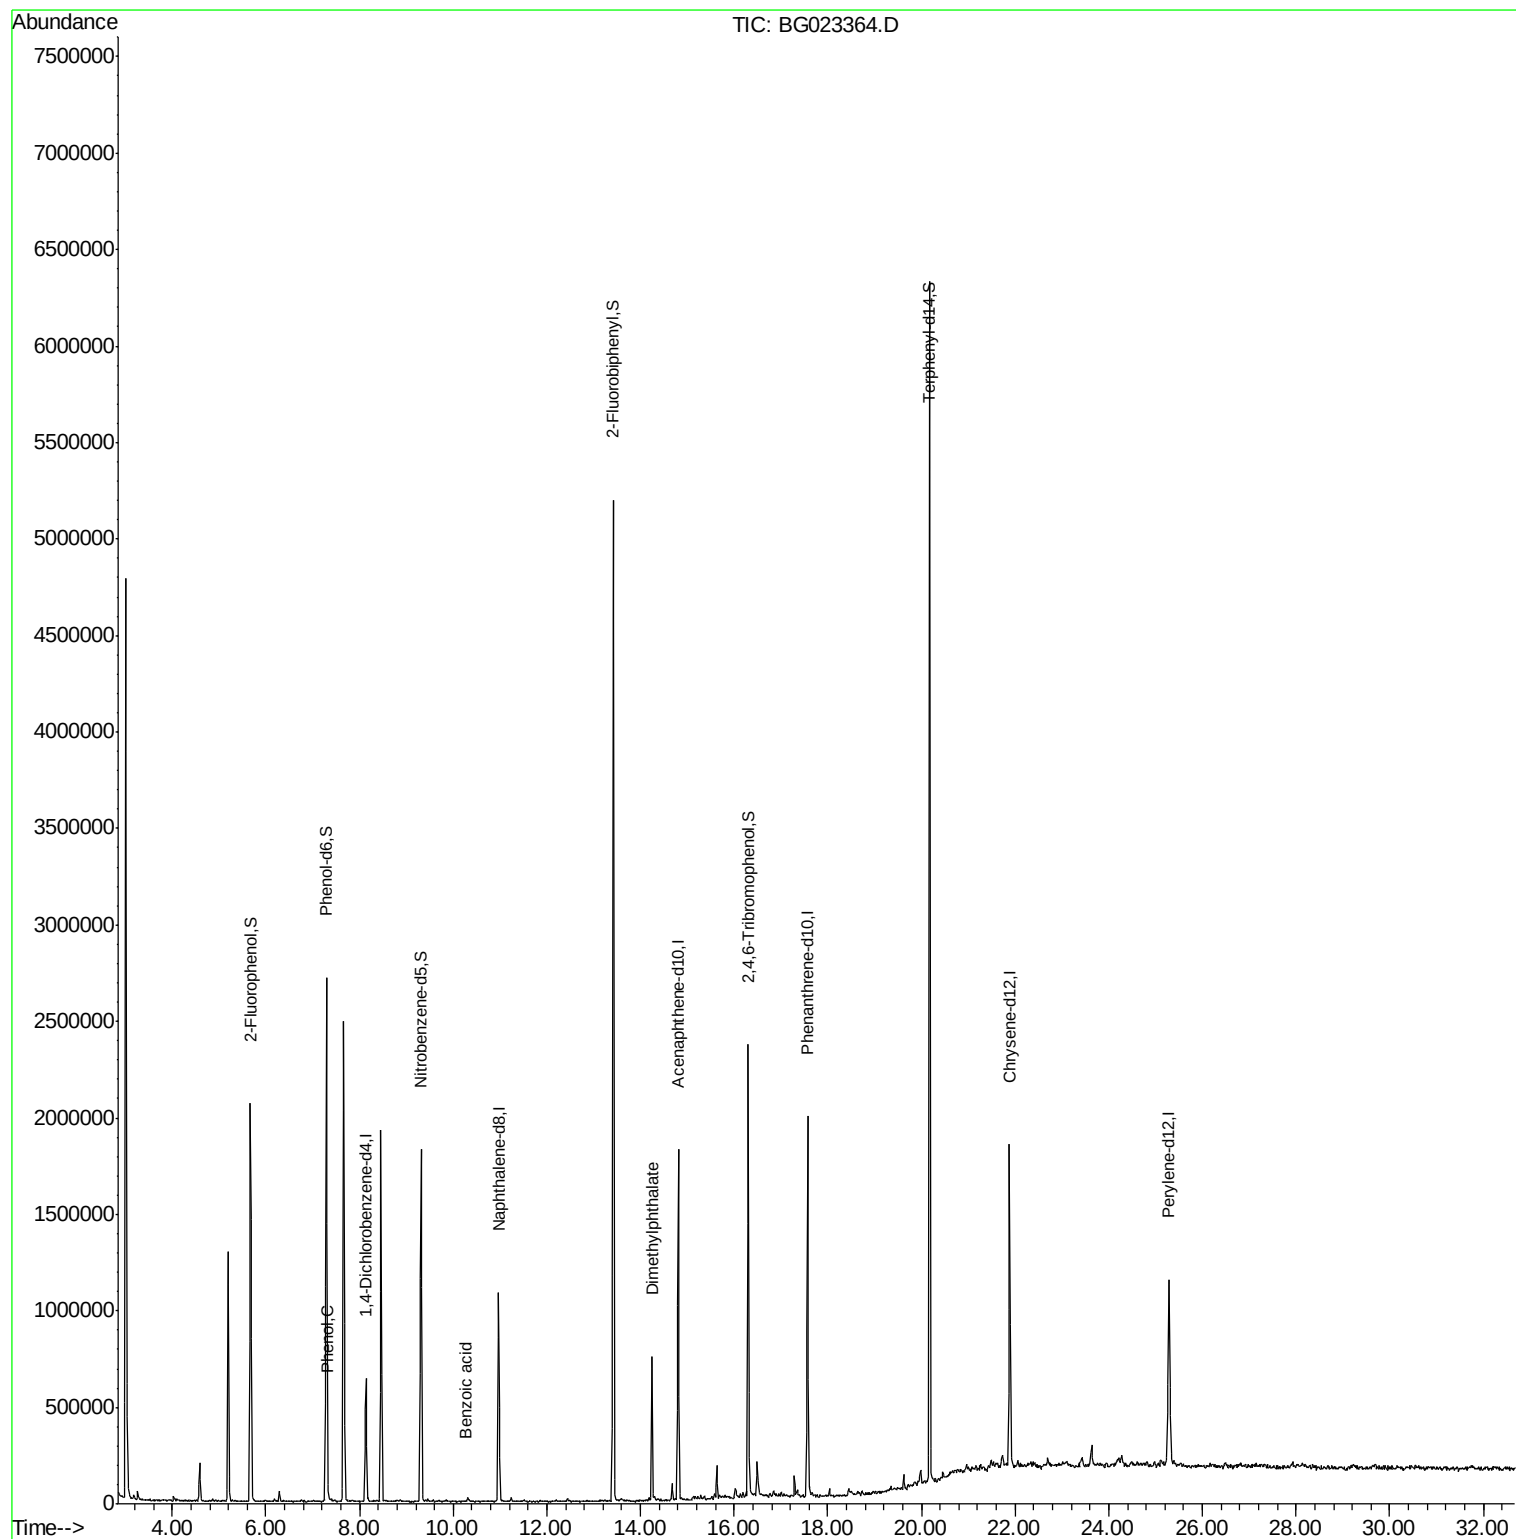







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.13 min Scan# 901
Delta R.T. -0.01 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Instrument :
BNA_G
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
152	100		
150	145.2	144.7	217.1
115	57.3	64.0	96.0#

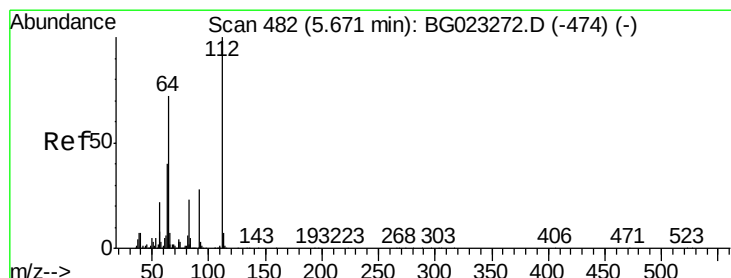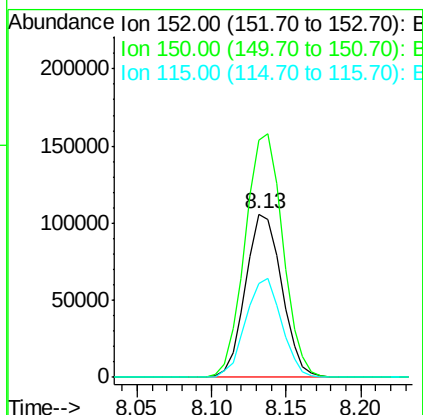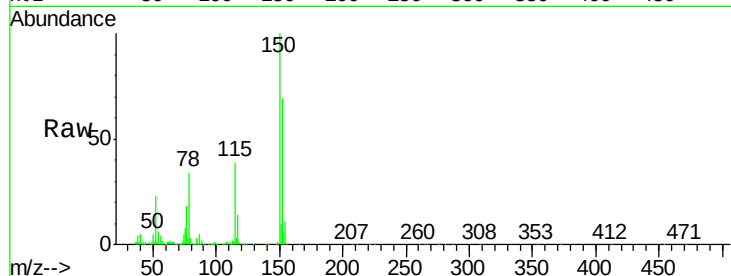


#5

2-Fluorophenol
Concen: 86.13 ng
RT: 5.67 min Scan# 482
Delta R.T. -0.00 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.7	59.0	88.4
63	37.1	37.8	56.8#

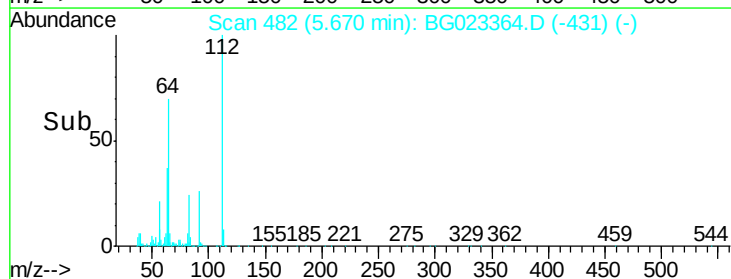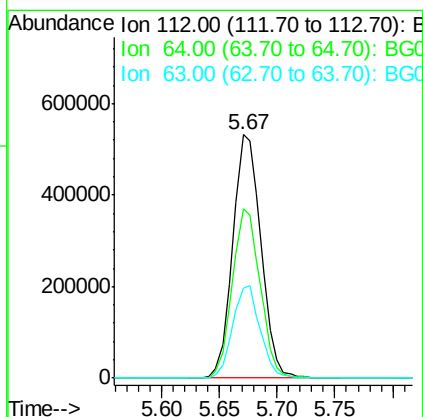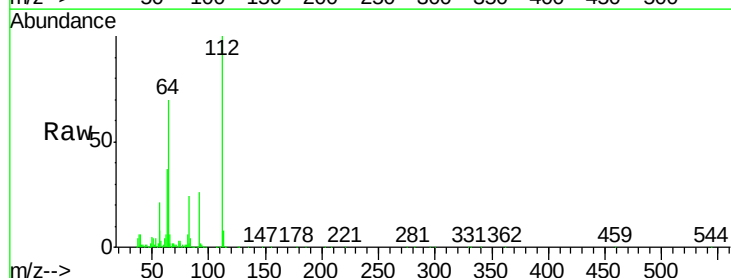

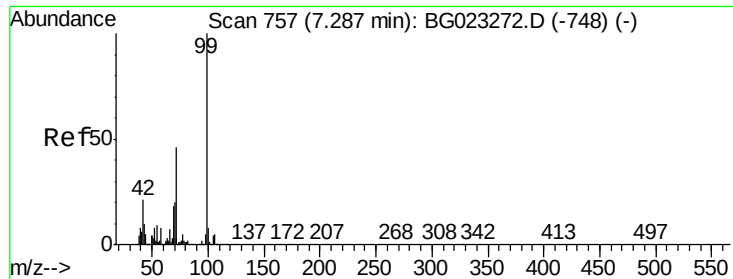

#7

Phenol-d6

Concen: 103.29 ng

RT: 7.29 min Scan# 758

Delta R.T. 0.00 min

Lab File: BG023364.D

Acq: 30 Jul 2016 19:30





Instrument :

BNA_G

ClientSampled :

Tot Ion: 99 Resp: 1653535

Ion	Ratio	Lower	Upper
99	100		
42	18.5	17.8	26.6
71	41.1	41.5	62.3#

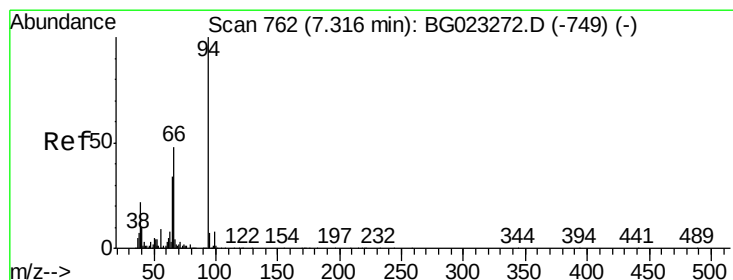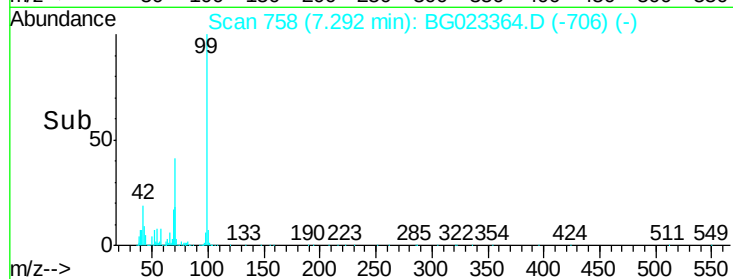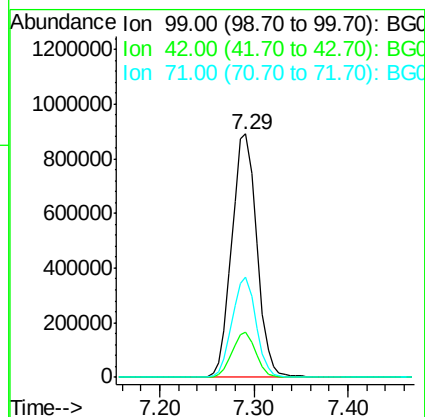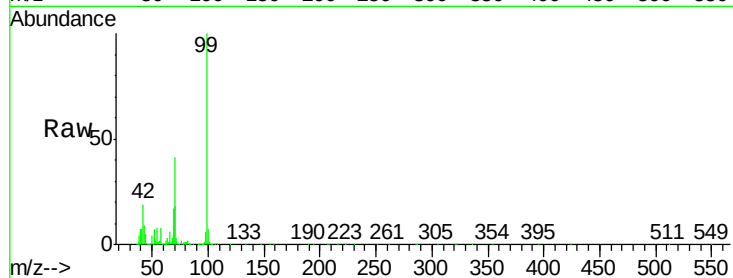

#10

Phenol

Concen: 2.39 ng

RT: 7.32 min Scan# 763




Delta R.T. 0.00 min


Lab File: BG023364.D

Acq: 30 Jul 2016 19:30

Tgt Ion: 94 Resp: 40315

Ion	Ratio	Lower	Upper
94	100		
65	33.0	18.1	58.1
66	52.2	42.1	82.1

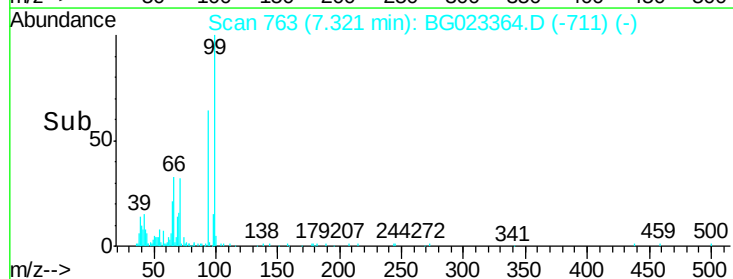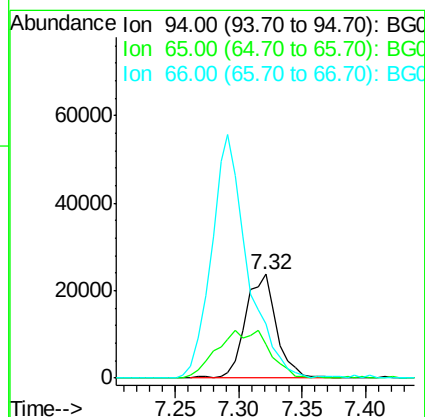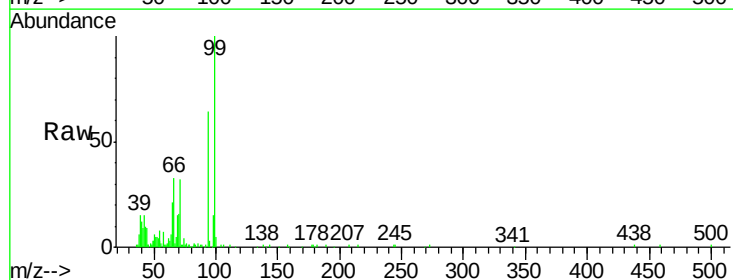







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.97 min Scan# 1384
Delta R.T. -0.01 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	883150
Ion Ratio	Lower	Upper
136 100		
137 11.9	9.6	14.4
54 9.0	7.3	10.9
68 7.8	5.3	7.9

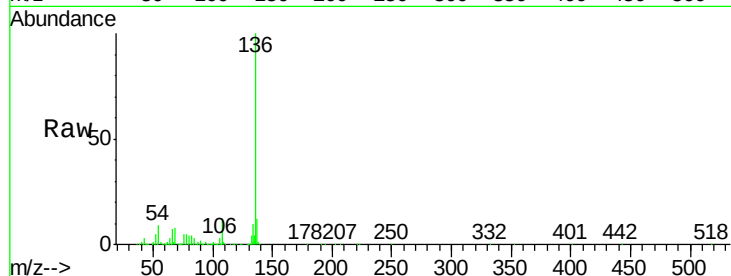


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

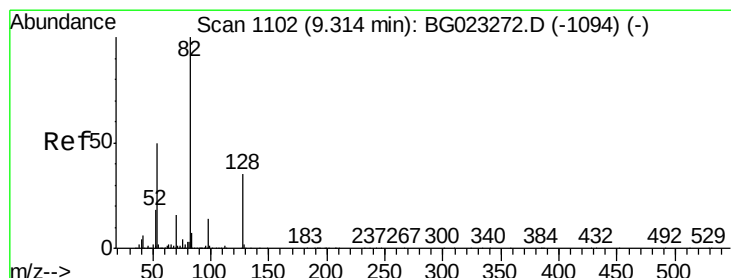
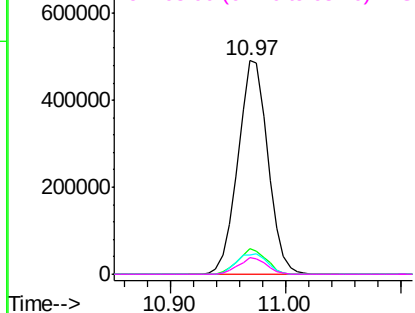



#23
Nitrobenzene-d5
Concen: 65.16 ng
RT: 9.31 min Scan# 1102
Delta R.T. 0.00 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Tgt Ion: 82	Resp: 1176779
Ion Ratio	Lower Upper
82 100	
128 38.0	24.4 36.6#
54 49.8	41.4 62.0

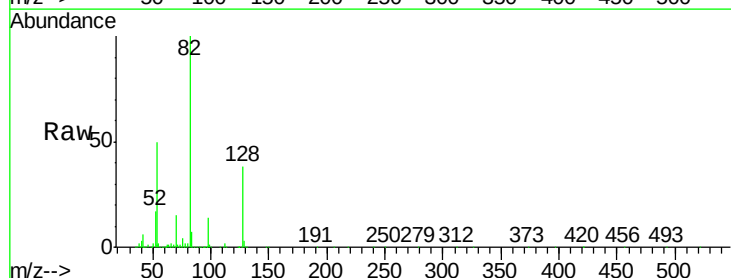

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC




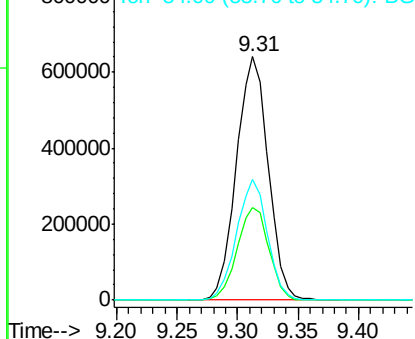




#32
Benzoic acid
Concen: 8.11 ng
RT: 10.27 min Scan# 1265
Delta R.T. -0.01 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30




Instrument :
BNA_G
ClientSampleId :


Tot Ion:122 Resp: 55
Ion Ratio Lower Upper
122 100
105 180.9 117.2 157.2#
77 0.0 109.2 149.2#

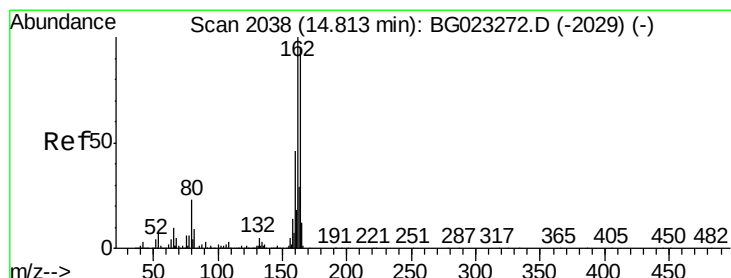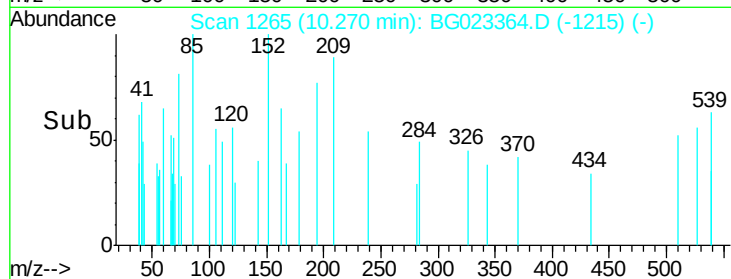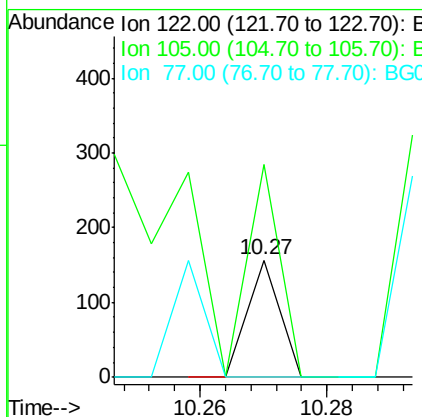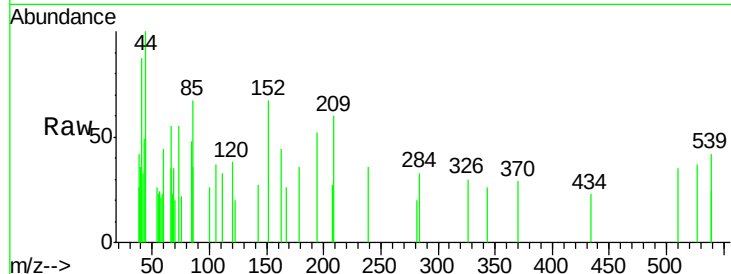

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.81 min Scan# 2037
Delta R.T. -0.00 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Tgt Ion:164 Resp: 615935
Ion Ratio Lower Upper
164 100
162 104.9 87.7 131.5
160 45.7 37.2 55.8

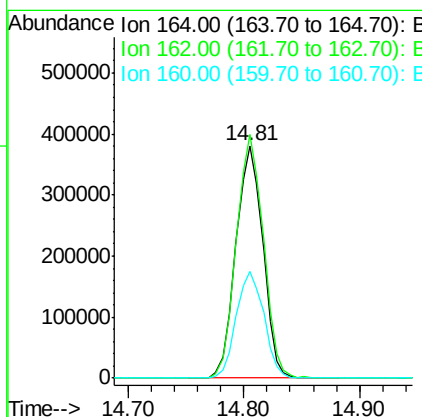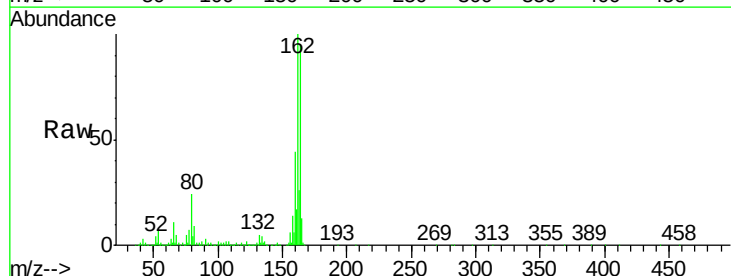


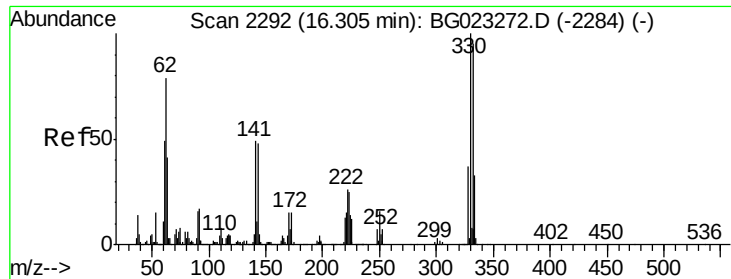




#41
 2,4,6-Tribromophenol
 Concen: 71.06 ng
 RT: 16.30 min Scan# 2292
 Delta R.T. -0.00 min
 Lab File: BG023364.D
 Acq: 30 Jul 2016 19:30

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:330 Resp: 453016
 Ion Ratio Lower Upper
 330 100
 332 102.3 77.4 116.2
 141 37.8 31.7 47.5

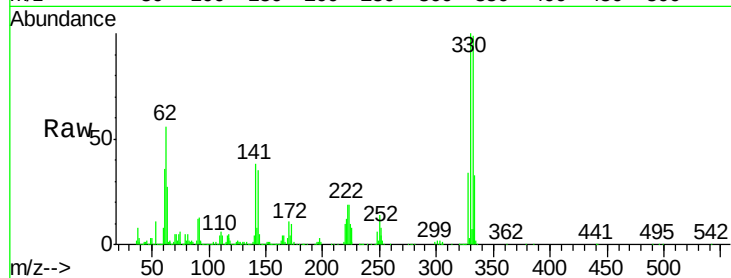


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

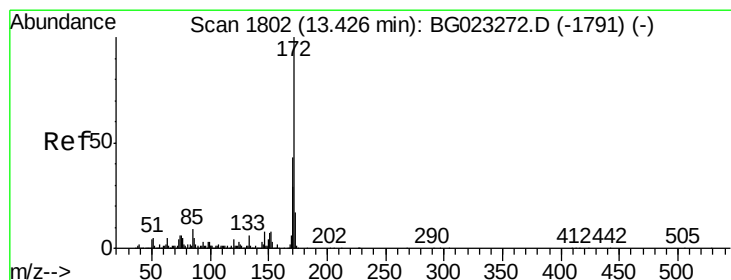
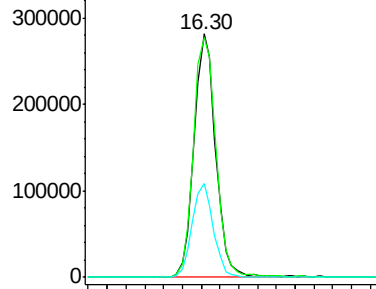



#44
 2-Fluorobiphenyl
 Concen: 74.94 ng
 RT: 13.42 min Scan# 1801
 Delta R.T. -0.00 min
 Lab File: BG023364.D
 Acq: 30 Jul 2016 19:30

Tgt Ion:172 Resp: 2466114
 Ion Ratio Lower Upper
 172 100
 171 43.8 31.6 47.4
 170 29.8 21.3 31.9

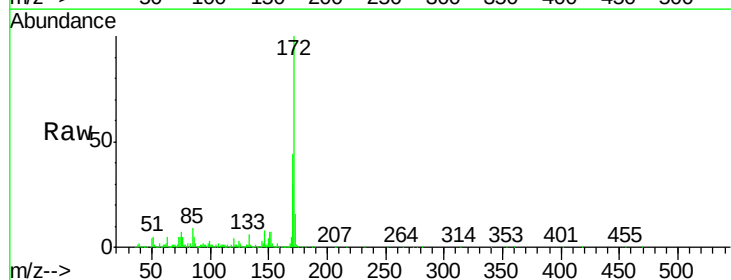

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

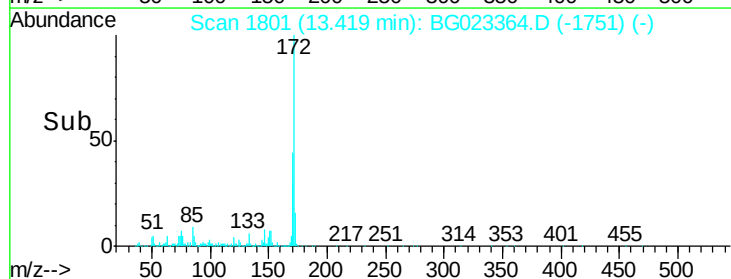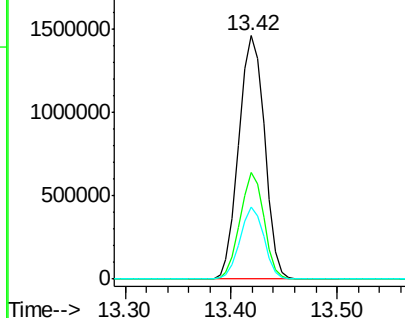



#49

Dimethylphthalate

Concen: 11.00 ng

RT: 14.25 min Scan# 1942

Delta R.T. -0.00 min

Lab File: BG023364.D

Acq: 30 Jul 2016 19:30

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 500198

Ion Ratio Lower Upper




163 100

194 3.9 3.6 5.4

164 10.4 8.1 12.1

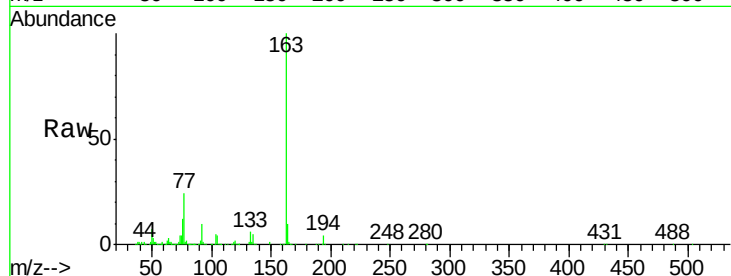

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

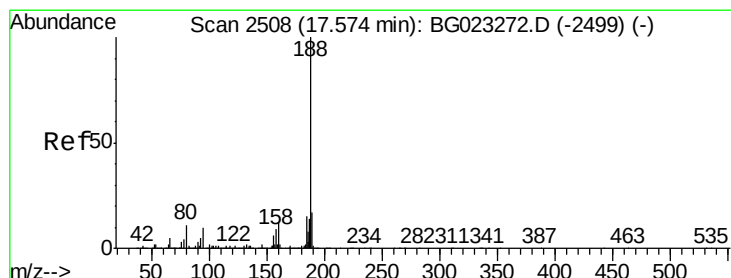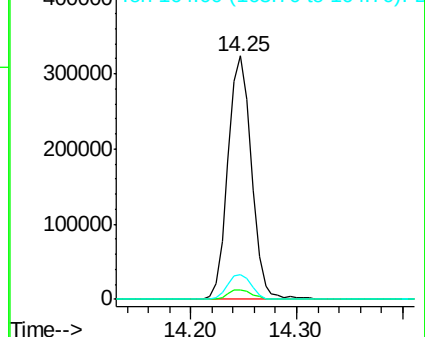

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.57 min Scan# 2507

Delta R.T. -0.00 min

Lab File: BG023364.D

Acq: 30 Jul 2016 19:30


Tgt Ion:188 Resp: 1158953

Ion Ratio Lower Upper



188 100


94 10.0 5.2 7.8#

80 11.8 7.2 10.8#

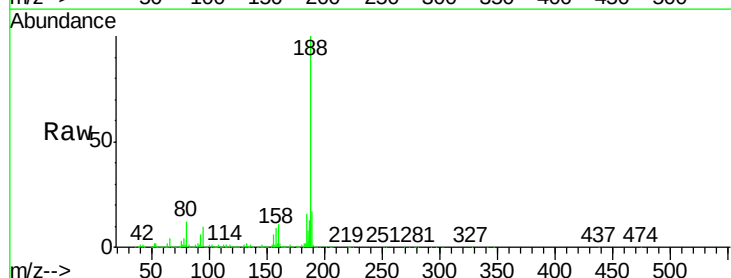

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

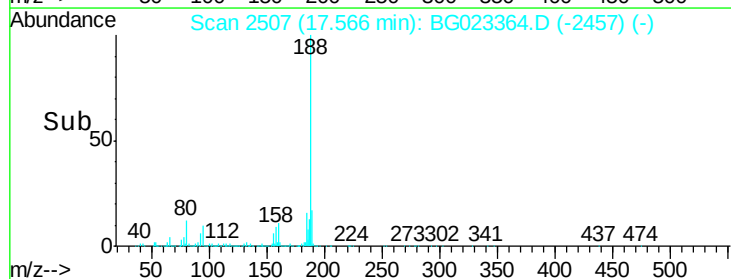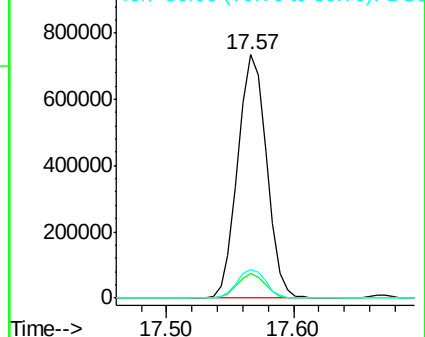

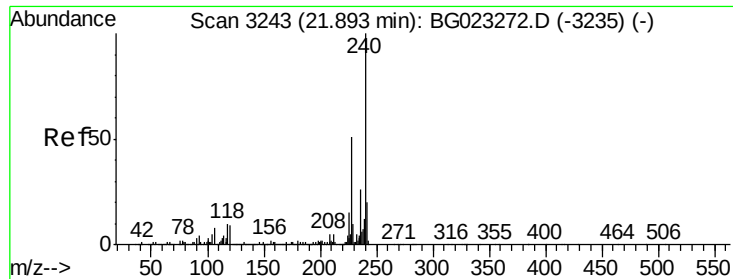

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.88 min Scan# 3242

Delta R.T. -0.01 min

Lab File: BG023364.D

Acq: 30 Jul 2016 19:30

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 1022438

Ion Ratio Lower Upper

240 100

120 9.8 4.1 6.1#




236 26.3 21.1 31.7

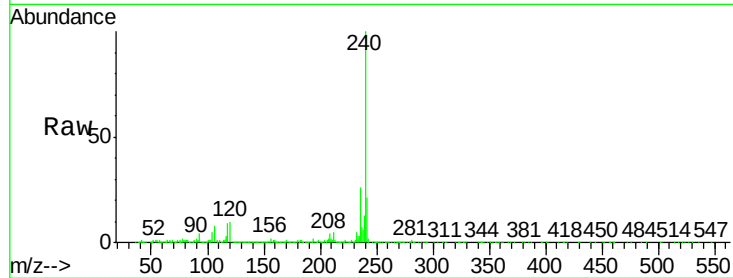

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

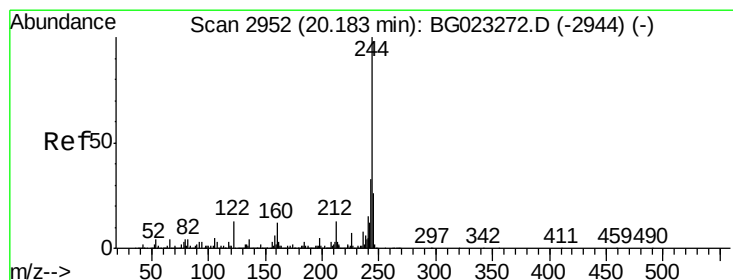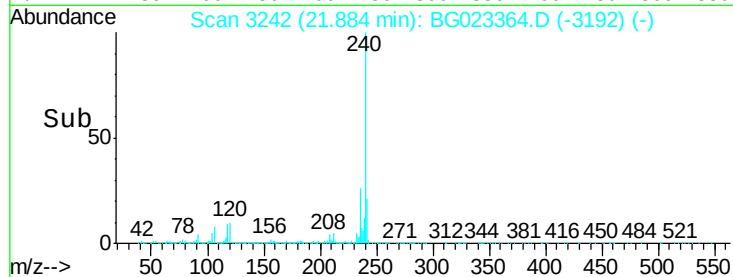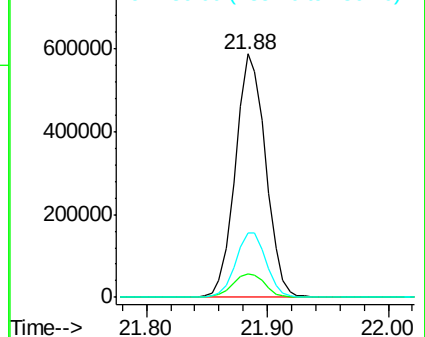

#78

Terphenyl-d14

Concen: 75.80 ng

RT: 20.17 min Scan# 2951

Delta R.T. -0.00 min

Lab File: BG023364.D

Acq: 30 Jul 2016 19:30


Tgt Ion:244 Resp: 2384147

Ion Ratio Lower Upper

244 100

212 11.4 10.8 16.2



122 13.6 8.0 12.0#

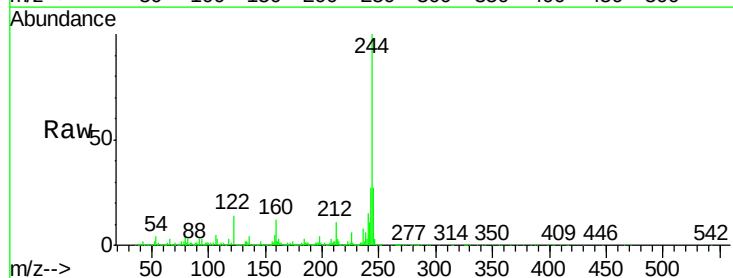


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

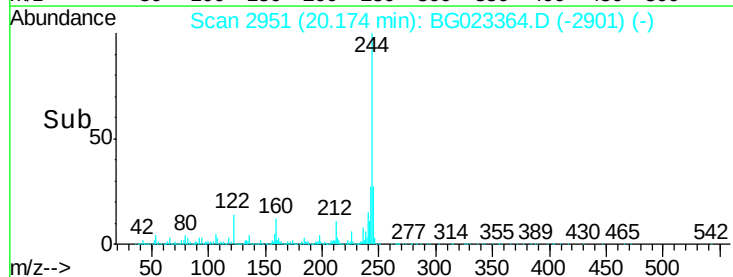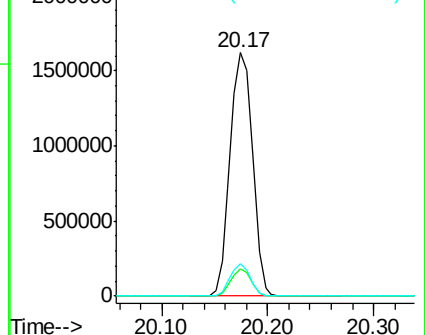

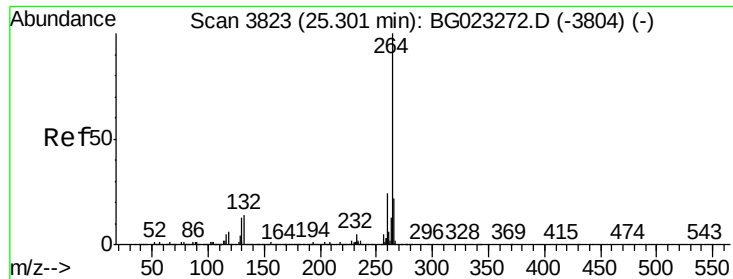

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.28 min Scan# 3821
Delta R.T. -0.02 min
Lab File: BG023364.D
Acq: 30 Jul 2016 19:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:264 Resp: 1040805

Ion	Ratio	Lower	Upper
264	100		
260	25.4	18.4	27.6
265	21.2	18.9	28.3

