
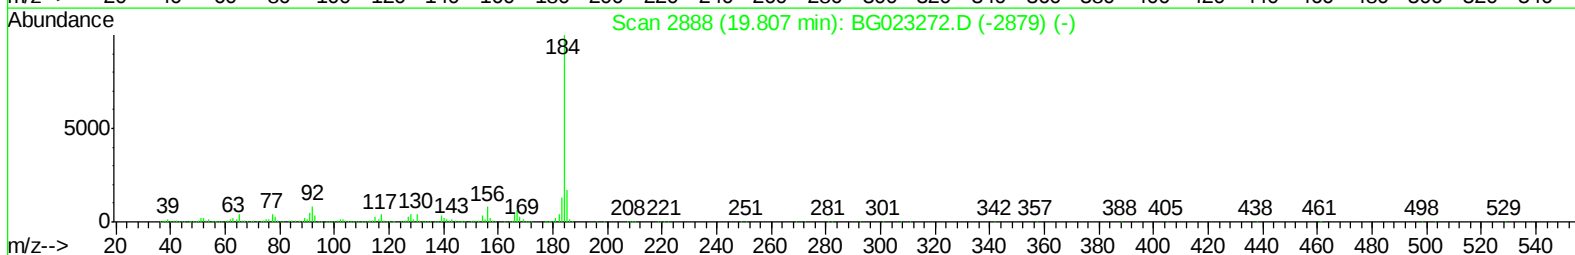
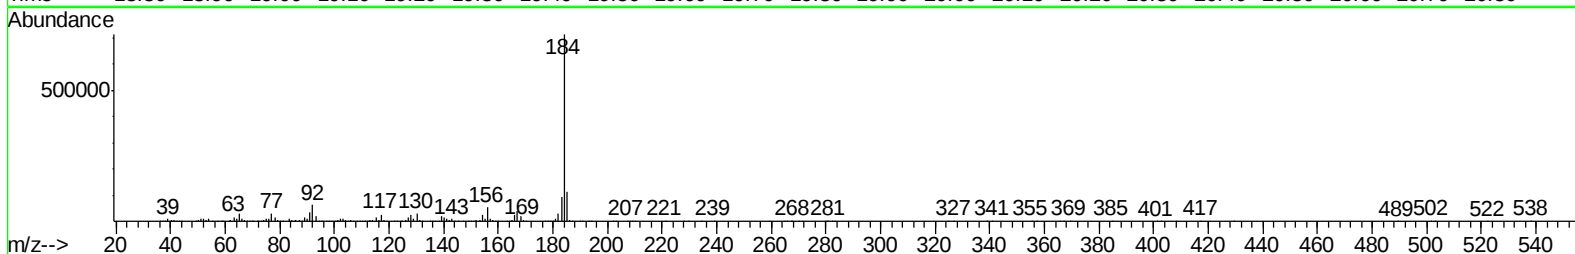


Data Path : Z:\HPCHEM1\BNA G\Data\BG073116\
Data File : BG023353.D
Acq On : 30 Jul 2016 12:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:43:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

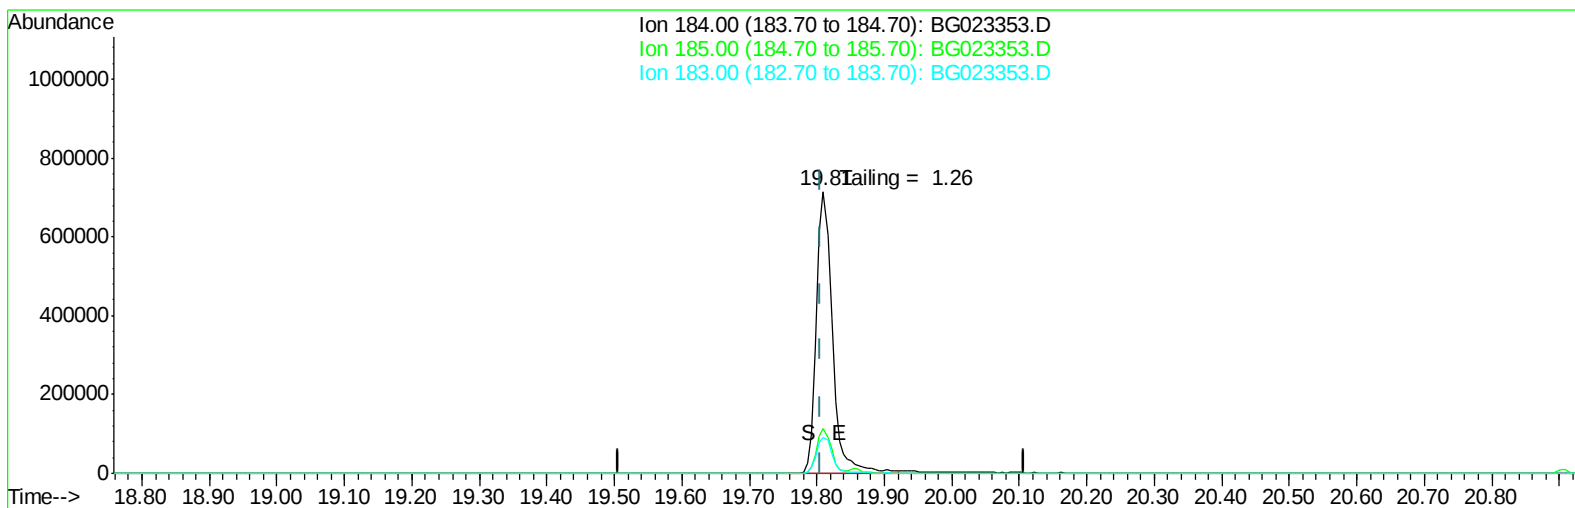

TIC: BG023353.D

(76) Benzidine




19.810min (+0.003) 268095.76ng

response 1161229

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.10
183.00	13.40	12.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG073116\
Data File : BG023353.D
Acq On : 30 Jul 2016 12:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:43:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

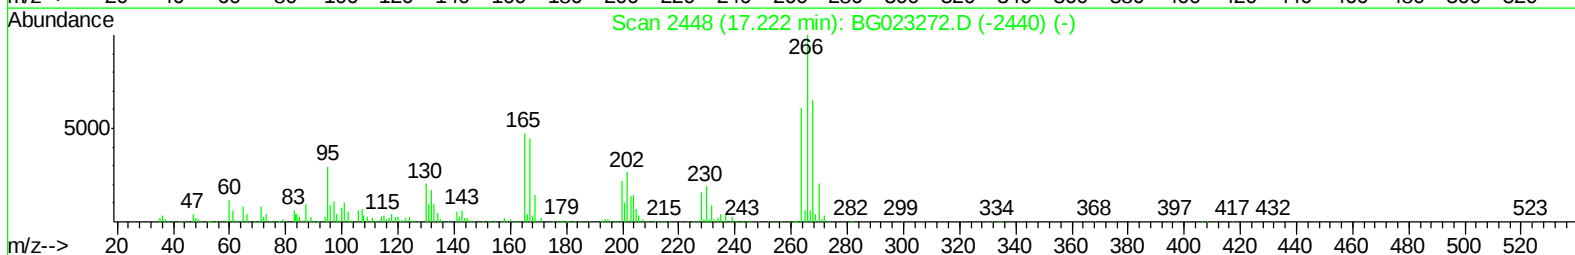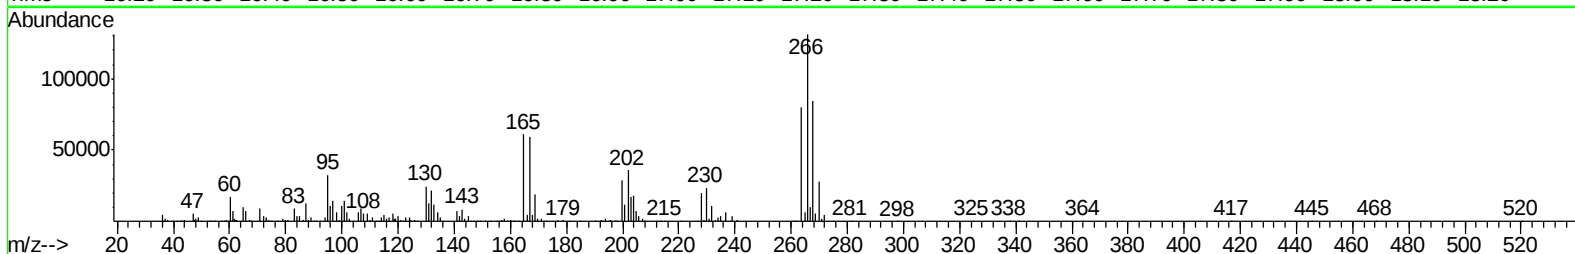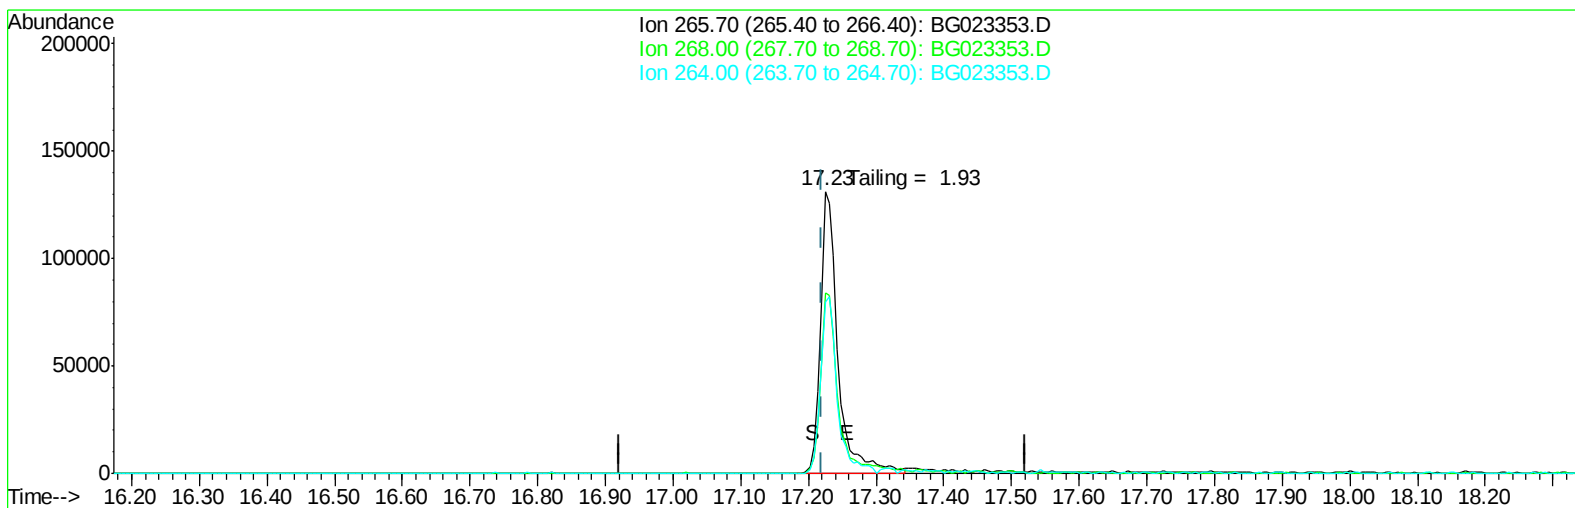

TIC: BG023353.D

(69) Pentachlorophenol (C)

17.225min (+0.004) 447705.56ng

response 238775

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.17
264.00	63.20	61.10
0.00	0.00	0.00