
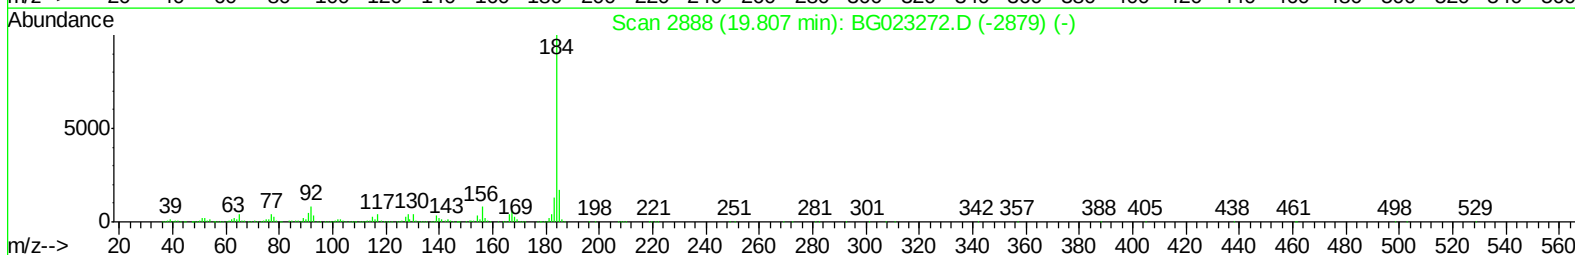
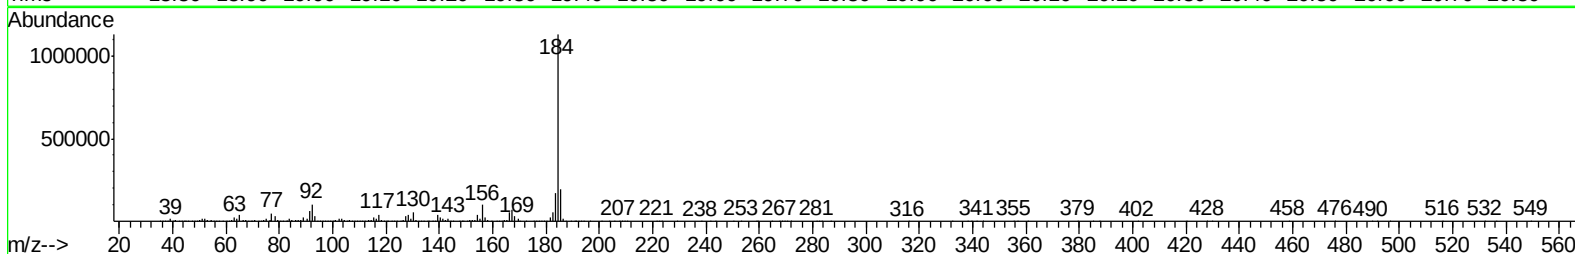


Data Path : Z:\HPCHEM1\BNA G\Data\BG073116\
 Data File : BG023365.D
 Acq On : 31 Jul 2016 11:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:44:42 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 27 17:30:33 2016
 Response via : Initial Calibration

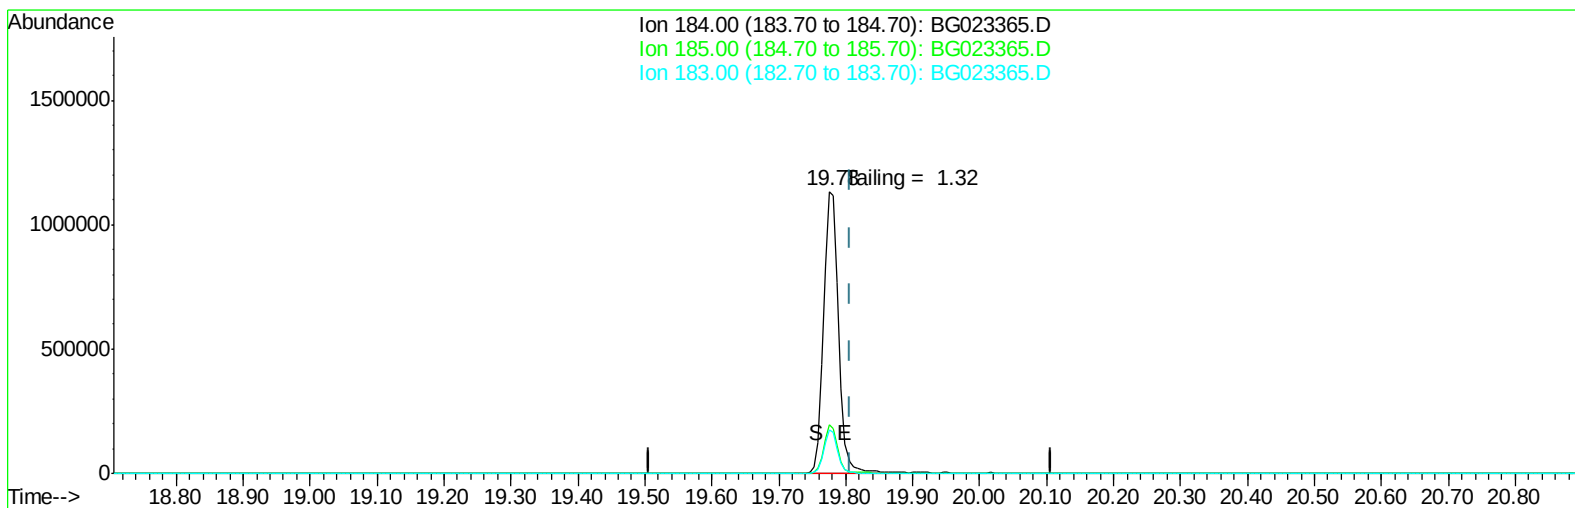

TIC: BG023365.D

(76) Benzidine




19.776min (-0.031) 400741.40ng

response 1792126

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	17.15
183.00	13.40	15.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG073116\
Data File : BG023365.D
Acq On : 31 Jul 2016 11:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:44:42 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG072616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 27 17:30:33 2016
Response via : Initial Calibration

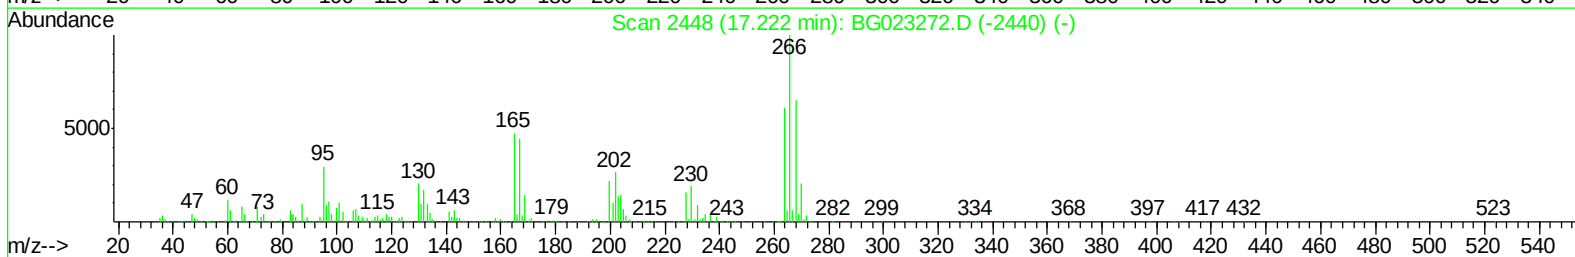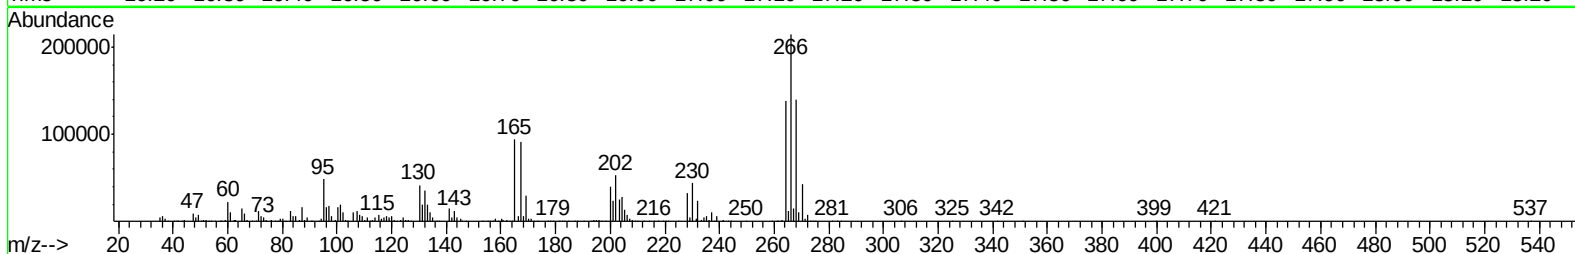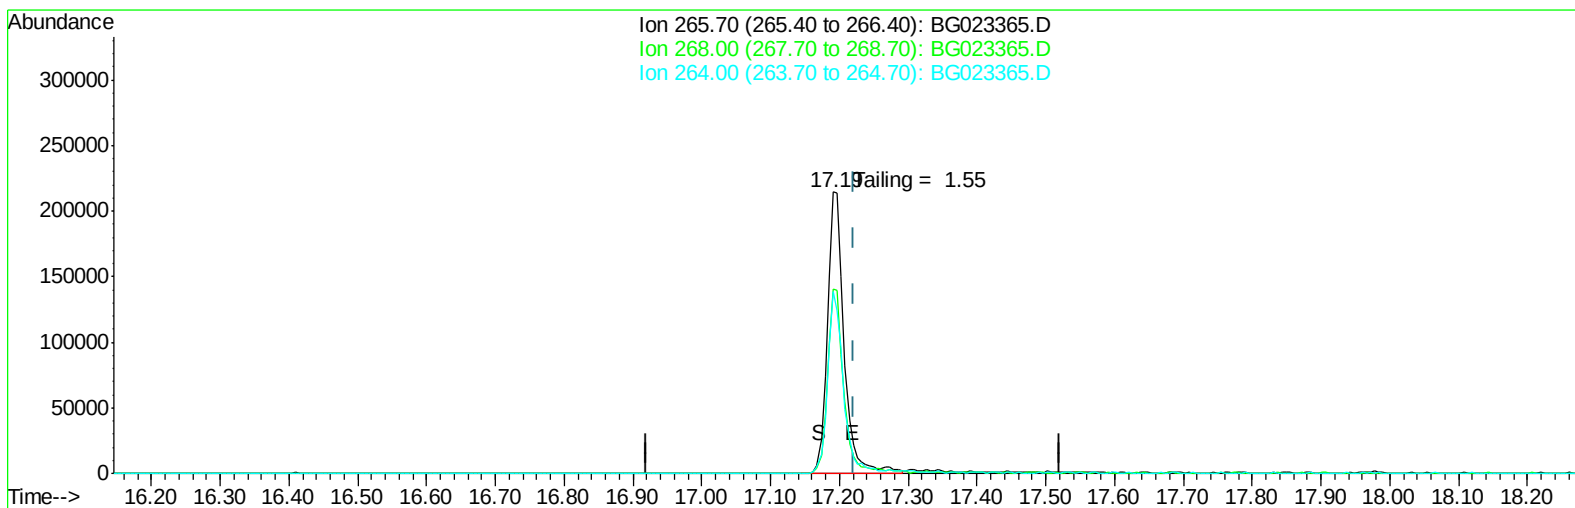

TIC: BG023365.D

(69) Pentachlorophenol (C)

17.191min (-0.030) 168630.42ng

response 360801

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.42
264.00	63.20	64.53
0.00	0.00	0.00