


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073116\
 Data File : BG023353.D
 Acq On : 30 Jul 2016 12:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:30:33 2016

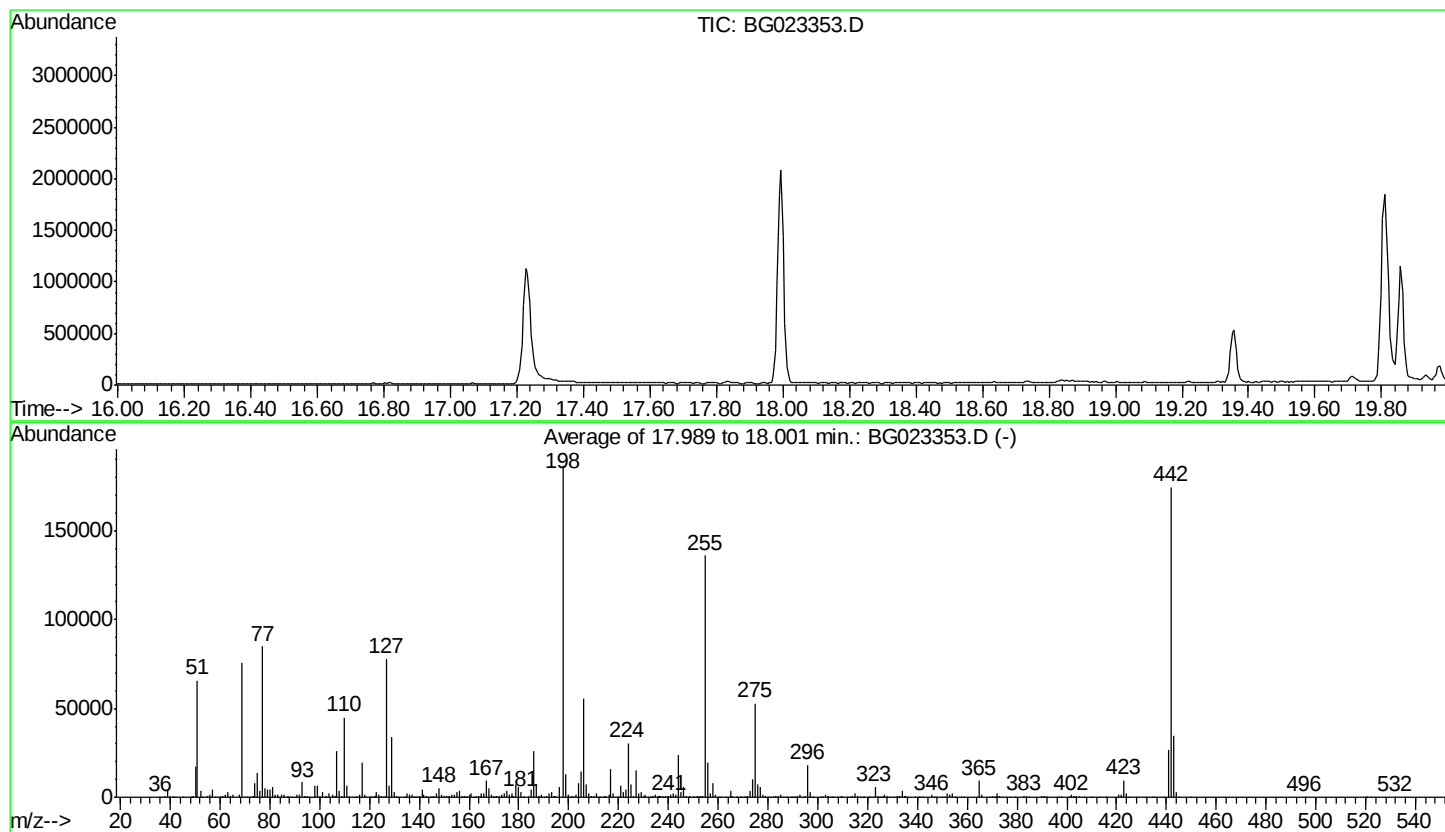

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	65750	PASS
68	69	0.00	2	1.9	1439	PASS
69	198	0.00	100	40.6	75776	PASS
70	69	0.00	2	0.4	336	PASS
127	198	10	80	41.7	77896	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	186752	PASS
199	198	5	9	7.1	13187	PASS
275	198	10	60	28.3	52890	PASS
365	198	1	100	5.0	9301	PASS
441	442	0.01	24	15.3	26762	PASS
442	198	50	100	93.5	174656	PASS
443	442	15	24	19.7	34421	PASS