


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073116\
Data File : BG023365.D
Acq On : 31 Jul 2016 11:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG072616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 27 17:30:33 2016

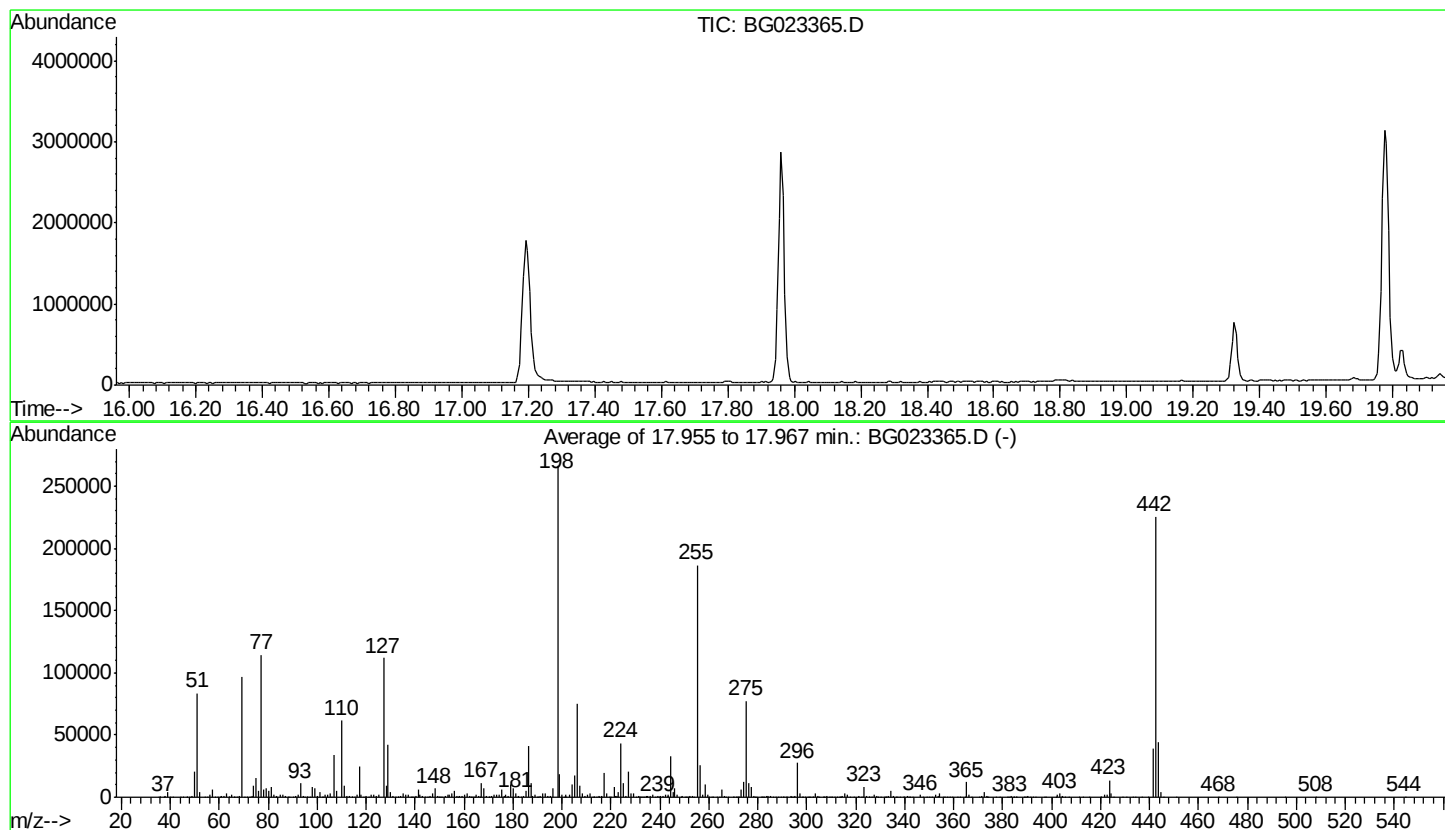

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	83345	PASS
68	69	0.00	2	0.8	781	PASS
69	198	0.00	100	36.4	97098	PASS
70	69	0.00	2	0.1	95	PASS
127	198	10	80	42.0	111952	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	266453	PASS
199	198	5	9	6.9	18316	PASS
275	198	10	60	29.1	77658	PASS
365	198	1	100	4.5	11896	PASS
441	442	0.01	24	17.4	39261	PASS
442	198	50	100	84.7	225770	PASS
443	442	15	24	19.4	43888	PASS