

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073117\
 Data File : BG028078.D
 Acq On : 31 Jul 2017 20:03
 Operator : SJ/JU
 Sample : I4373-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA2

Quant Time: Aug 01 01:37:33 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 28 19:32:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	26469	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	119273	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.97	164	95183	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.72	188	297377	20.00	ng/ul	0.00
78) Chrysene-d12	22.05	240	391142	20.00	ng/ul	0.00
86) Perylene-d12	25.57	264	389619	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.85	96	2611	6.39	ng/uL	0.00
5) Phenol-d5	7.51	99	10385	5.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	22669	22.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	33288	19.75	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	19814	11.10	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	20752	24.89	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	26862	25.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	49476	23.68	ng/ul	0.00
29) 4-Chloroaniline-d4	11.33	131	1884	0.89	ng/ul	0.01
44) Dimethylphthalate-d6	14.36	166	257568	29.90	ng/ul	0.00
47) Acenaphthylene-d8	14.67	160	242557	26.03	ng/ul	0.00
52) 4-Nitrophenol-d4	15.17	143	5993	4.63	ng/ul	0.01
58) Fluorene-d10	15.96	176	227556	28.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.07	200	49961	23.59	ng/ul	0.00
71) Anthracene-d10	17.82	188	391670	27.50	ng/ul	0.00
79) Pyrene-d10	20.09	212	546702	31.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.33	264	516076	28.80	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	14.40	163	17364	2.200 ng/ul# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073117\
Data File : BG028078.D
Acq On : 31 Jul 2017 20:03
Operator : SJ/JU
Sample : I4373-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA2

Quant Time: Aug 01 01:37:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 28 19:32:36 2017
Response via : Initial Calibration

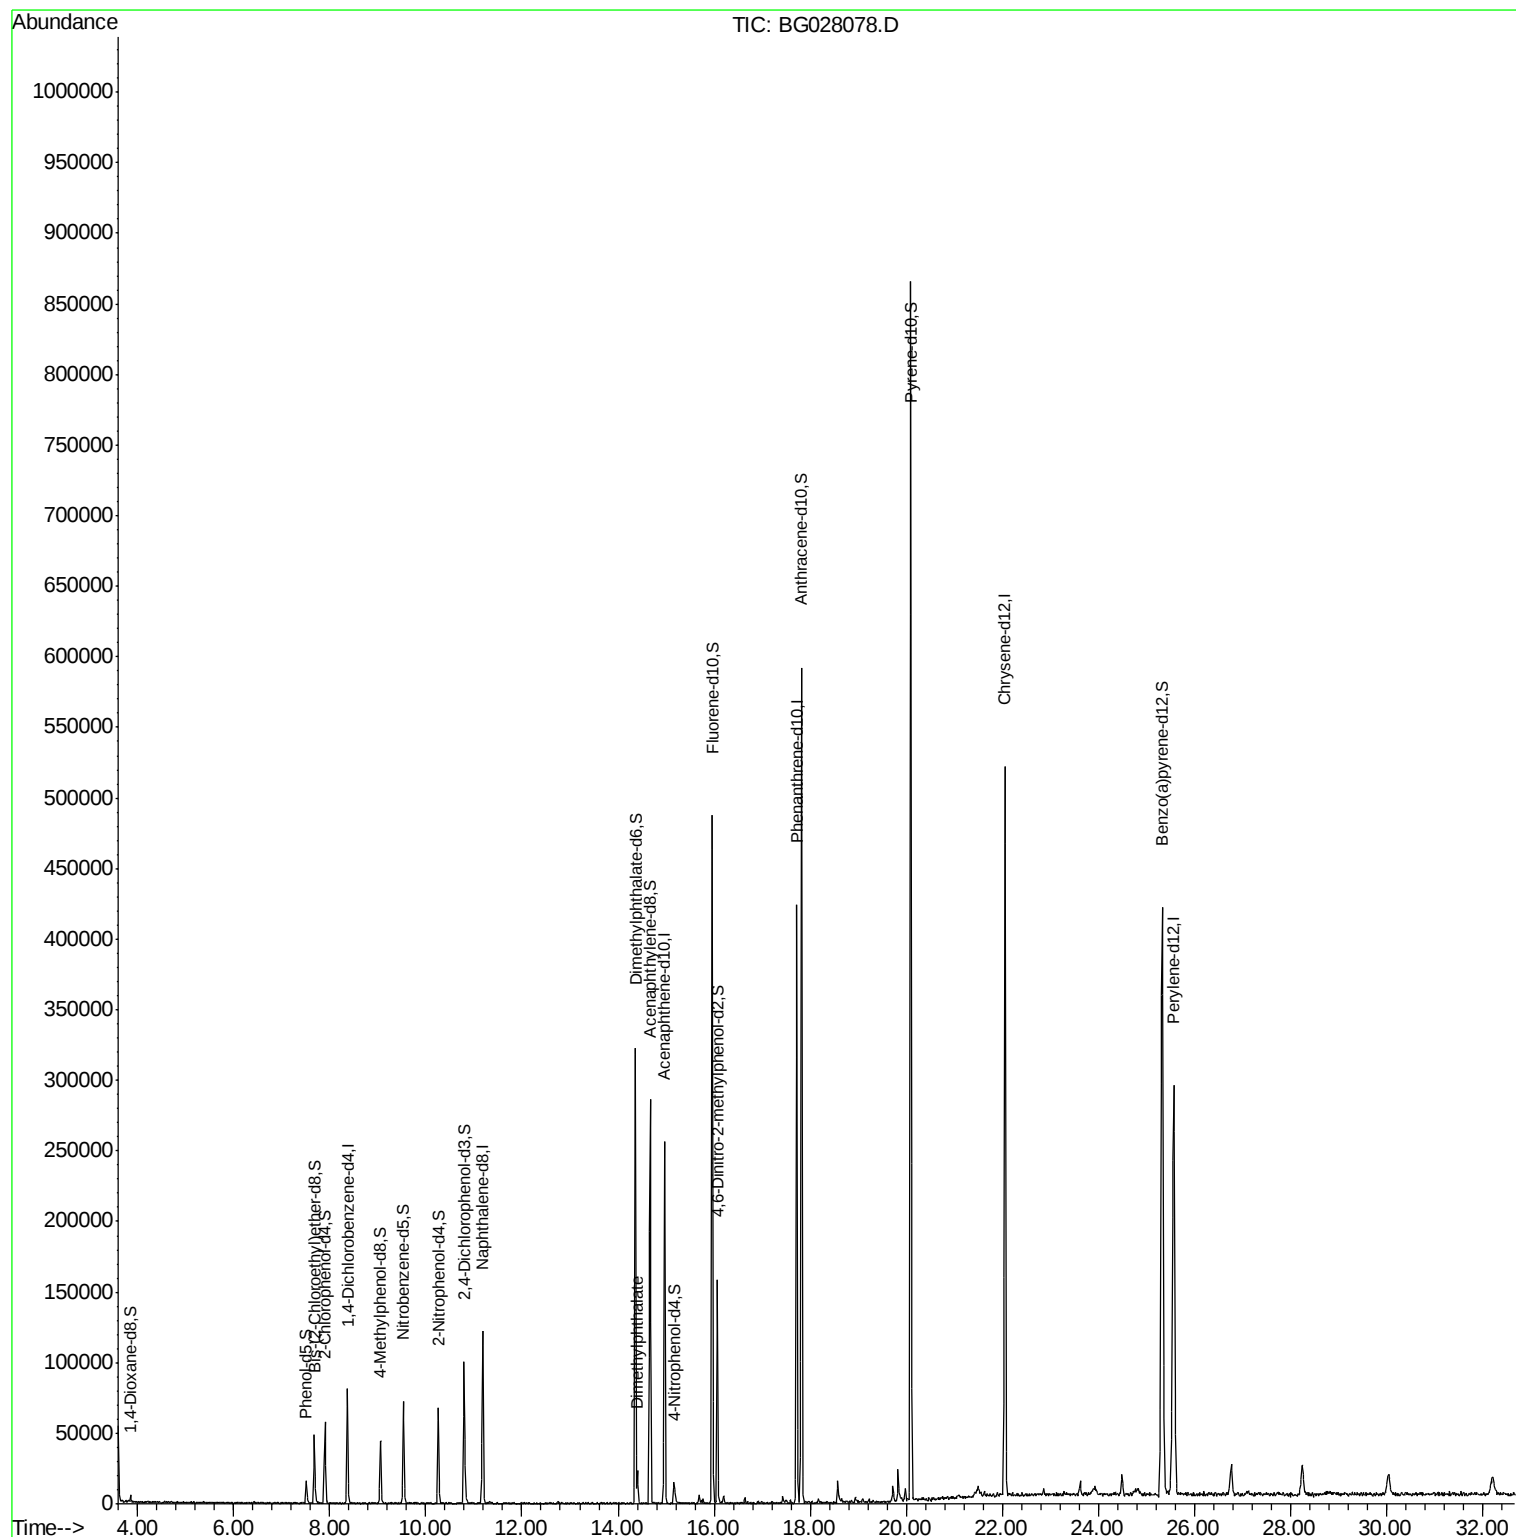

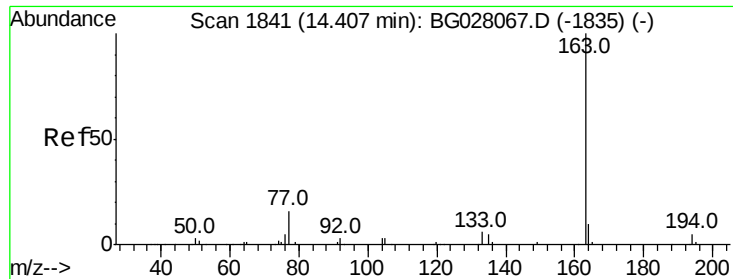

#45

Dimethylphthalate

Concen: 2.200 ng/ul

RT: 14.40 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BG028078.D

Acq: 31 Jul 2017 20:03

Instrument :

BNA_G

ClientSampleId :

C0AA2


Tot Ion:163 Resp: 17364

Ion Ratio Lower Upper

163 100

194 3.8 4.0 6.0#

164 9.4 8.4 12.6

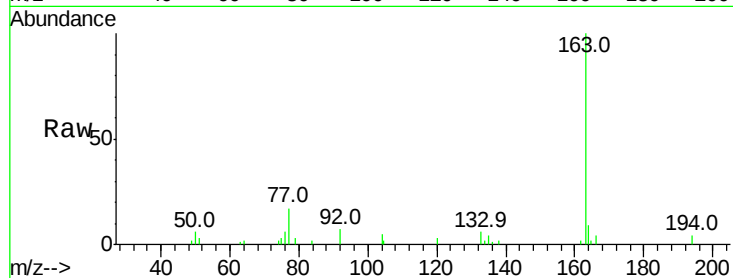

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

