

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073117\
 Data File : BG028081.D
 Acq On : 31 Jul 2017 22:01
 Operator : SJ/JU
 Sample : PB101070BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK70

Quant Time: Aug 01 01:38:39 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 28 19:32:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	30850	20.00	ng/ul	0.00
18) Naphthalene-d8	11.18	136	139225	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.97	164	114024	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.72	188	347169	20.00	ng/ul	0.00
78) Chrysene-d12	22.05	240	463953	20.00	ng/ul	0.00
86) Perylene-d12	25.57	264	469143	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.85	96	2719	5.71	ng/uL	0.00
5) Phenol-d5	7.51	99	60817	26.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	33974	29.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	57033	29.03	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	57991	27.88	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	30757	31.61	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	38650	31.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	69162	28.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	93270	37.91	ng/ul	0.00
44) Dimethylphthalate-d6	14.36	166	345079	33.44	ng/ul	0.00
47) Acenaphthylene-d8	14.67	160	341668	30.61	ng/ul	0.00
52) 4-Nitrophenol-d4	15.15	143	38525	24.85	ng/ul	0.00
58) Fluorene-d10	15.96	176	301708	31.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.07	200	66818	27.03	ng/ul	0.00
71) Anthracene-d10	17.82	188	552952	33.26	ng/ul	0.00
79) Pyrene-d10	20.09	212	711155	34.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.33	264	725216	33.61	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.05	70	1514	1.067	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG073117\
Data File : BG028081.D
Acq On : 31 Jul 2017 22:01
Operator : SJ/JU
Sample : PB101070BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK70

Quant Time: Aug 01 01:38:39 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 28 19:32:36 2017
Response via : Initial Calibration

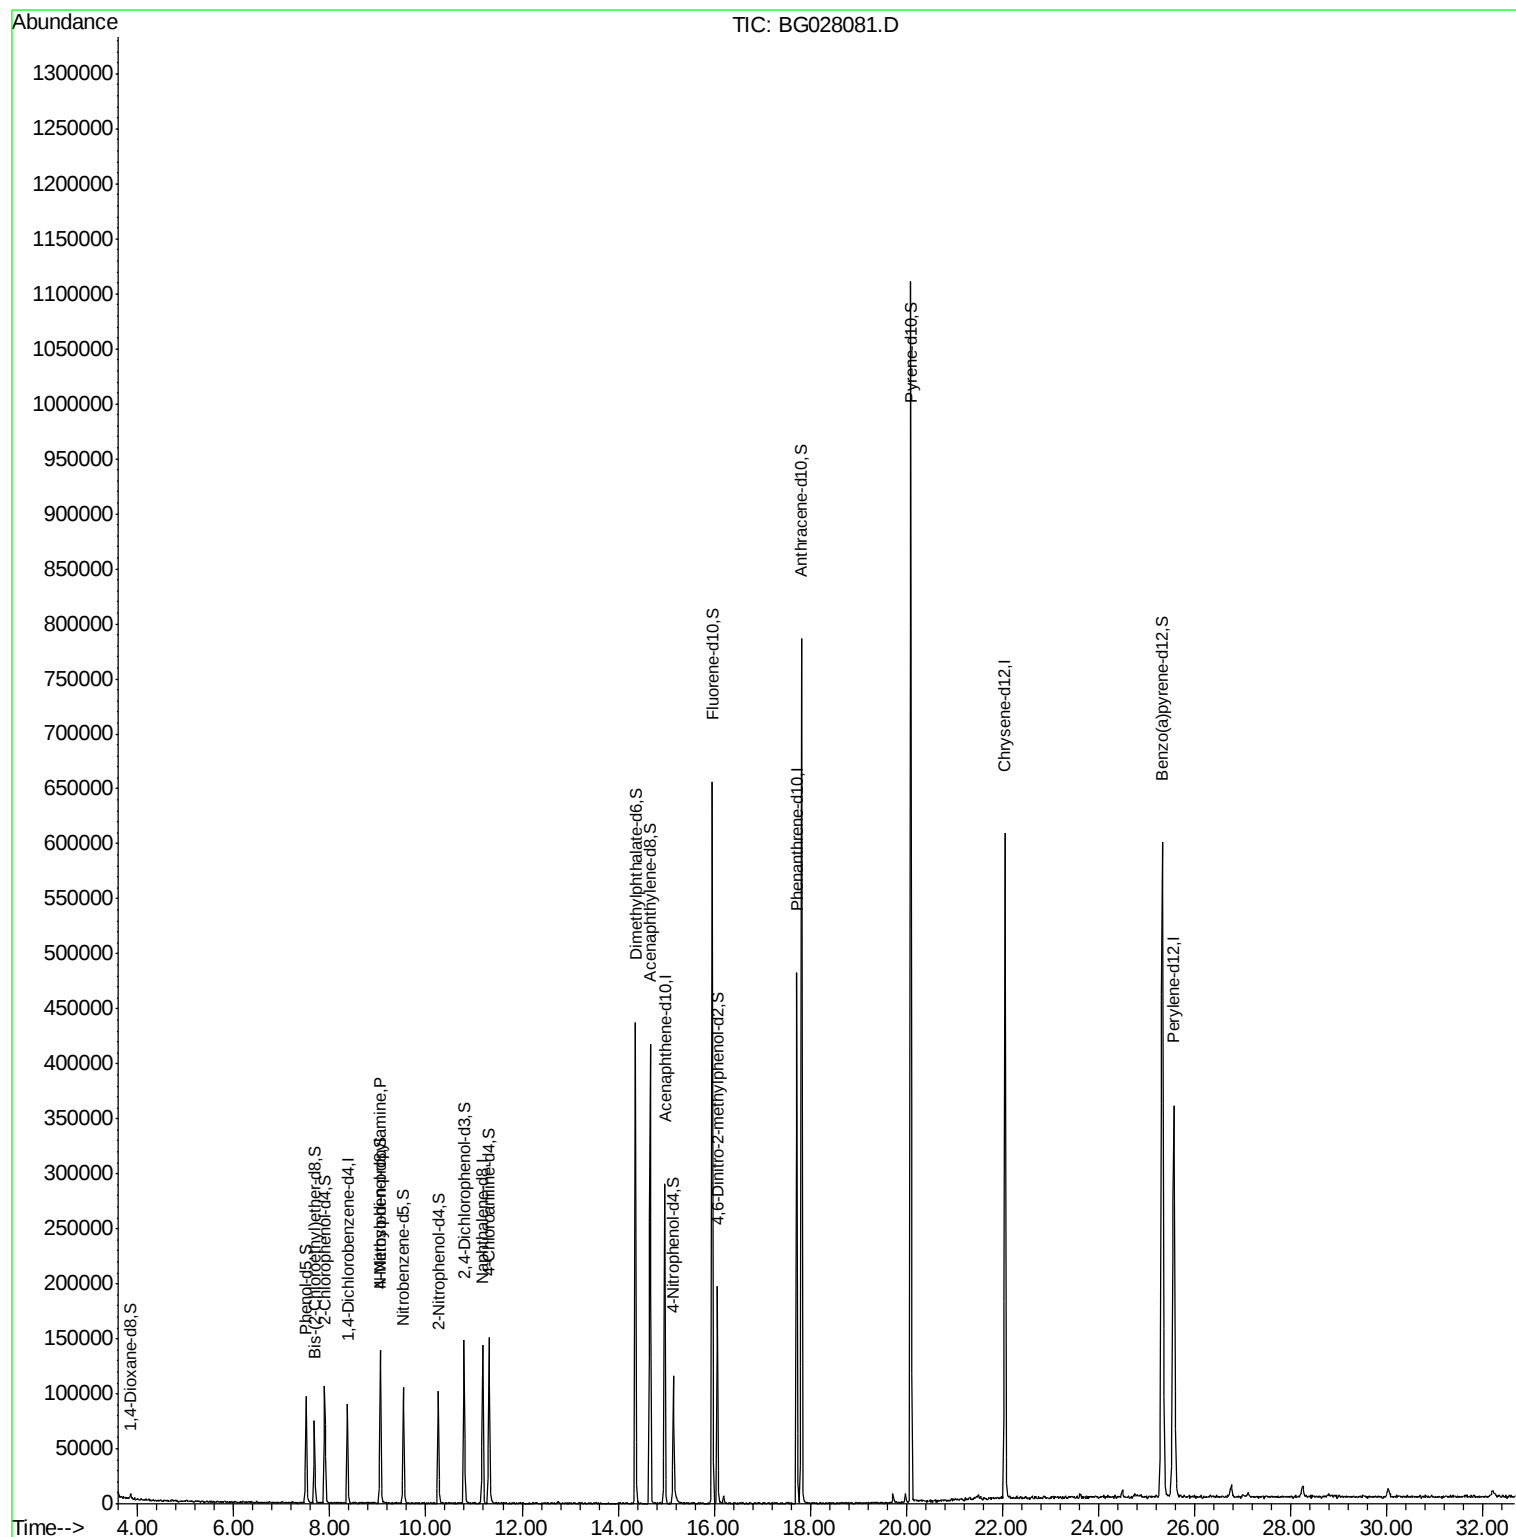

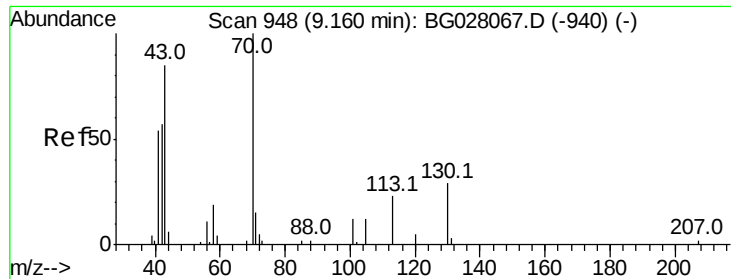

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.067 ng/ul
 RT: 9.05 min Scan# 930
 Delta R.T. -0.11 min
 Lab File: BG028081.D
 Acq: 31 Jul 2017 22:01

Instrument :
 BNA_G
 ClientSampleId :
 SBLK70

Tot Ion: 70 Resp: 1514
 Ion Ratio Lower Upper
 70 100
 42 205.3 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

