

Quantitation Report (QT Reviewed)


Instrument :
BNA_G
ClientSampled :
C0AE3

Manual Integrations
APPROVED

Sohil
8/1/2017 2:55:32 PM

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073117\
Data File : BG028090.D
Acq On : 1 Aug 2017 3:55
Operator : SJ/JU
Sample : I4504-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Aug 01 10:34:45 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG072717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 01 02:25:43 2017
Response via : Initial Calibration

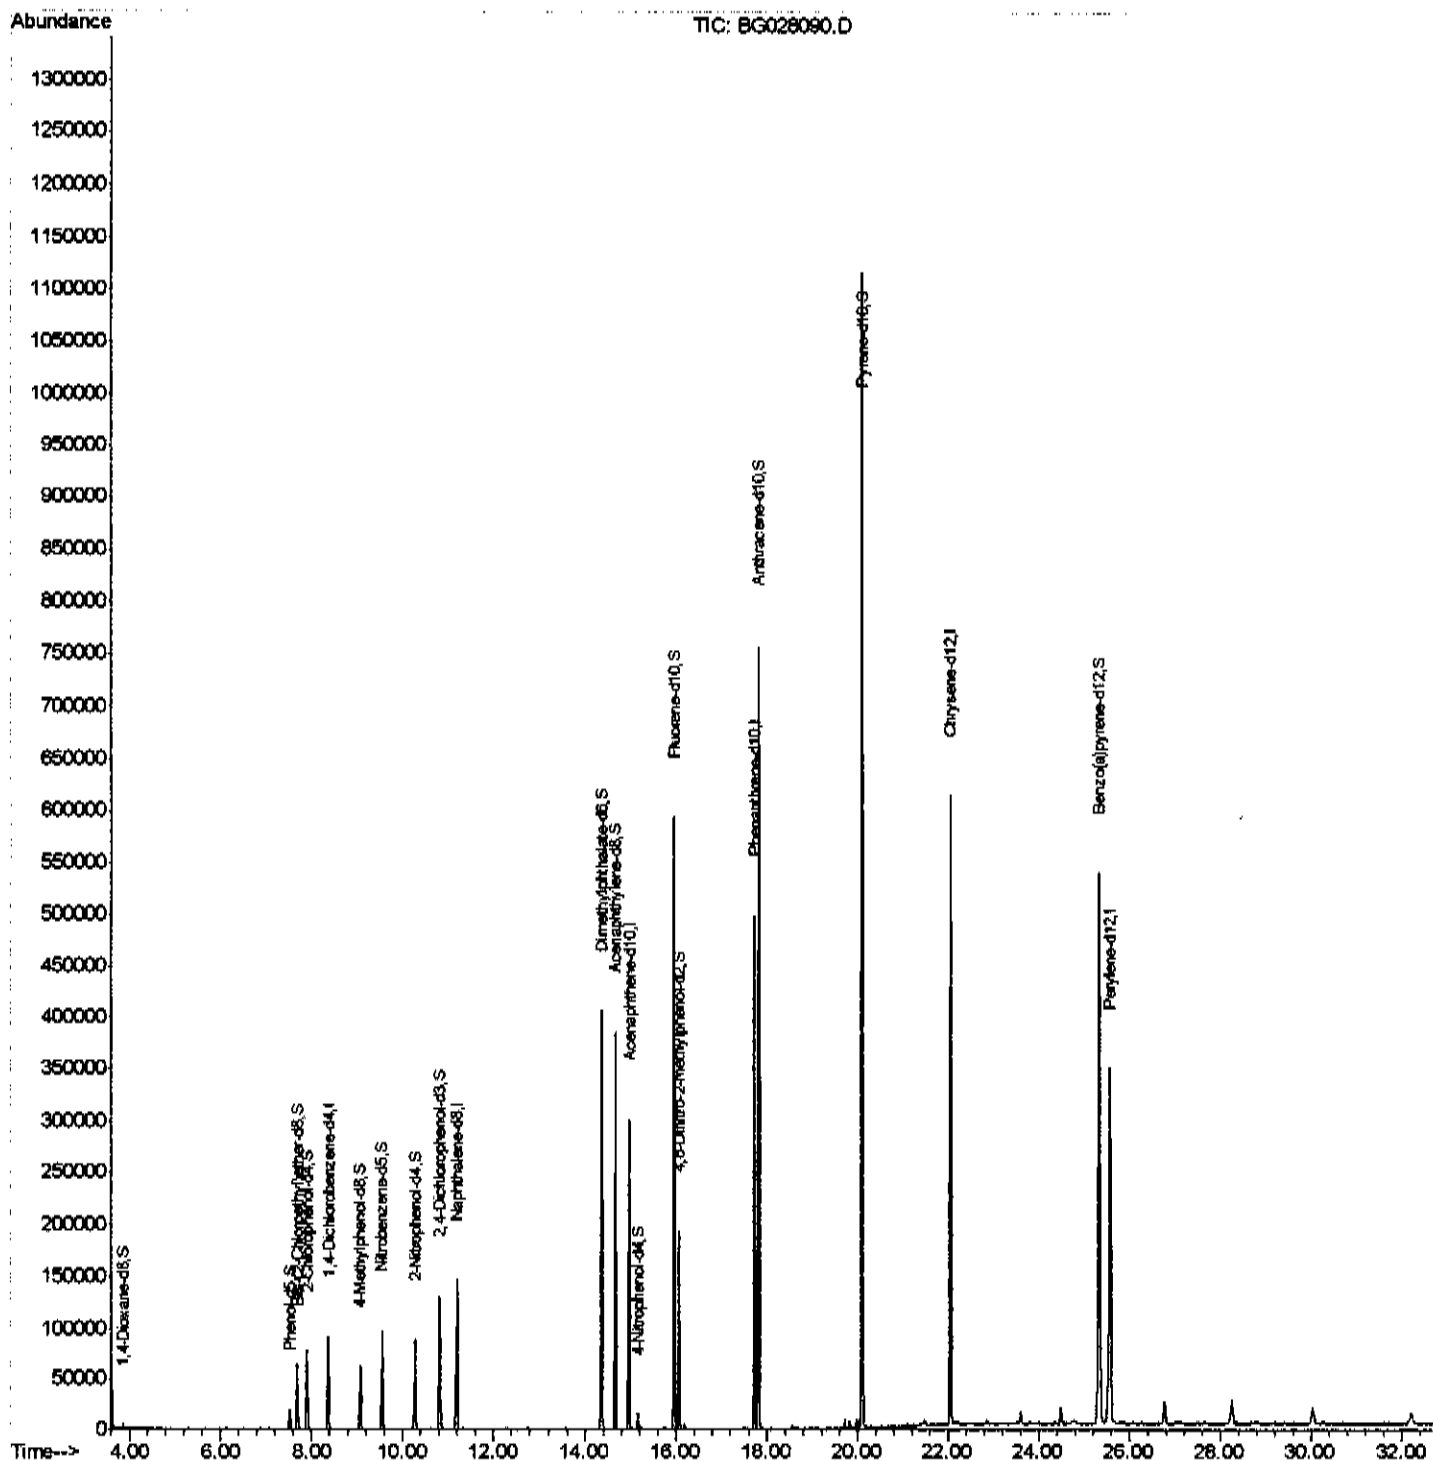

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG073117\
 Data File : BG028090.D
 Acq On : 1 Aug 2017 3:55
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 8/1/2017 2:55:32 PM

Quant Time: Aug 01 10:34:45 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 01 02:25:43 2017
 Response via : Initial Calibration

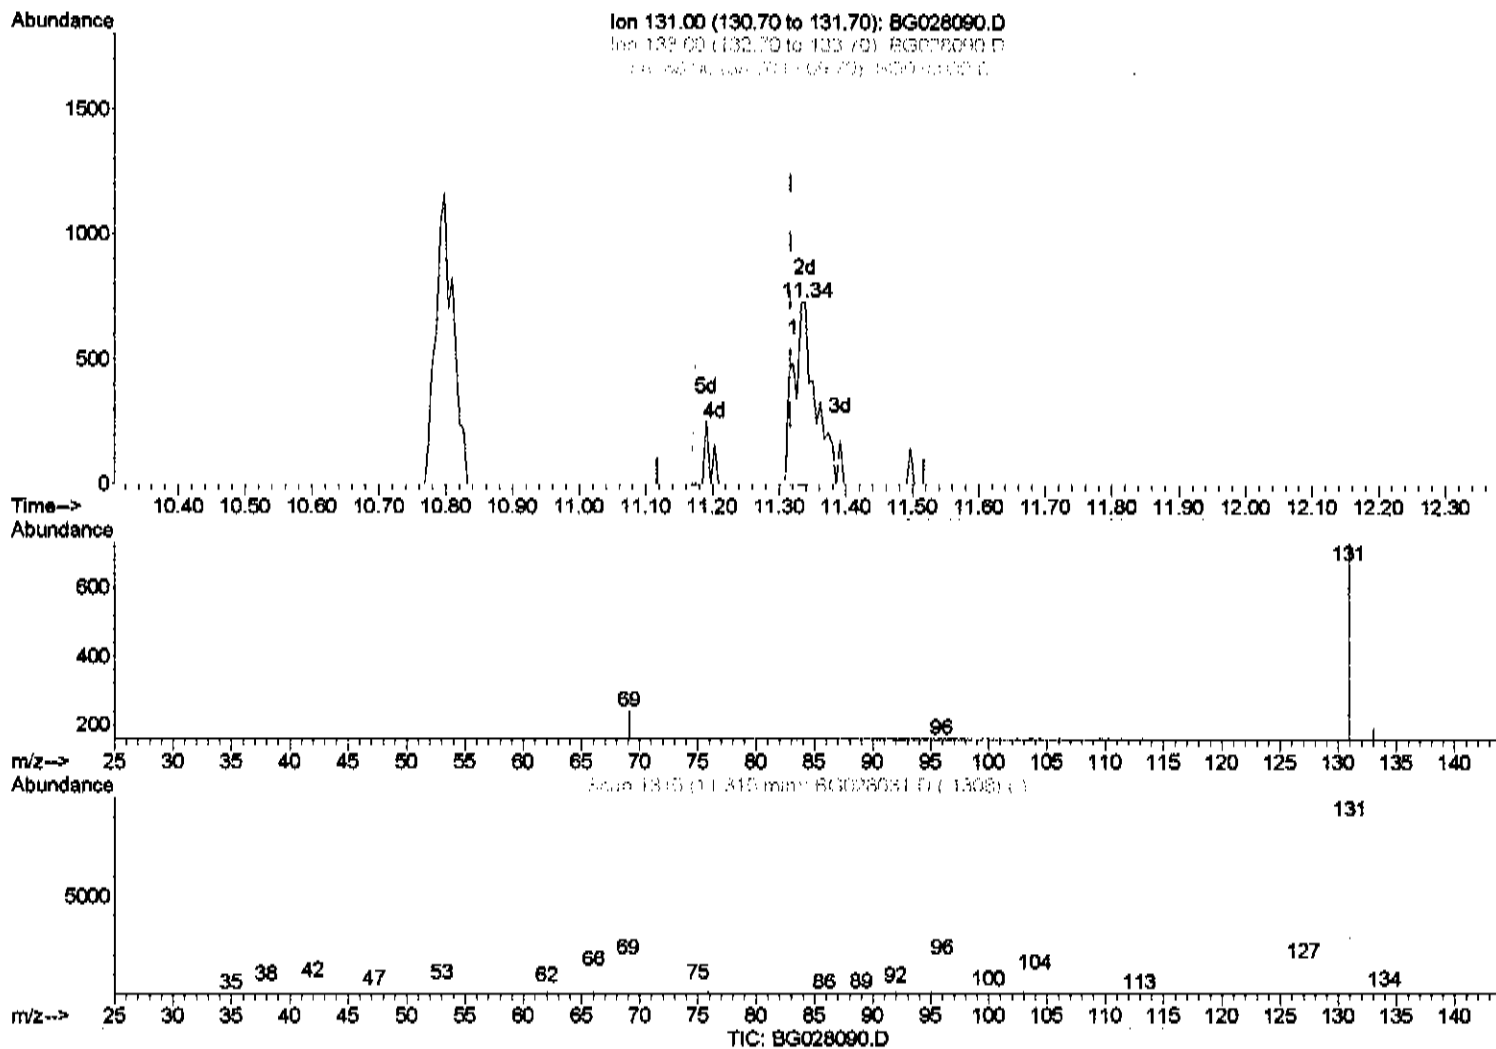

(29) 4-Chloroaniline-d4 (S)

11.338min (+0.021) 0.66ng/ul m

response 1665

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	26.19#
69.00	18.60	32.88#
0.00	0.00	0.00

[Handwritten signature]
 8/1/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG073117\
 Data File : BG028090.D
 Acq On : 1 Aug 2017 3:55
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 8/1/2017 2:55:32 PM

Quant Time: Aug 18 13:41:14 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG072717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 01 02:25:43 2017
 Response via : Initial Calibration

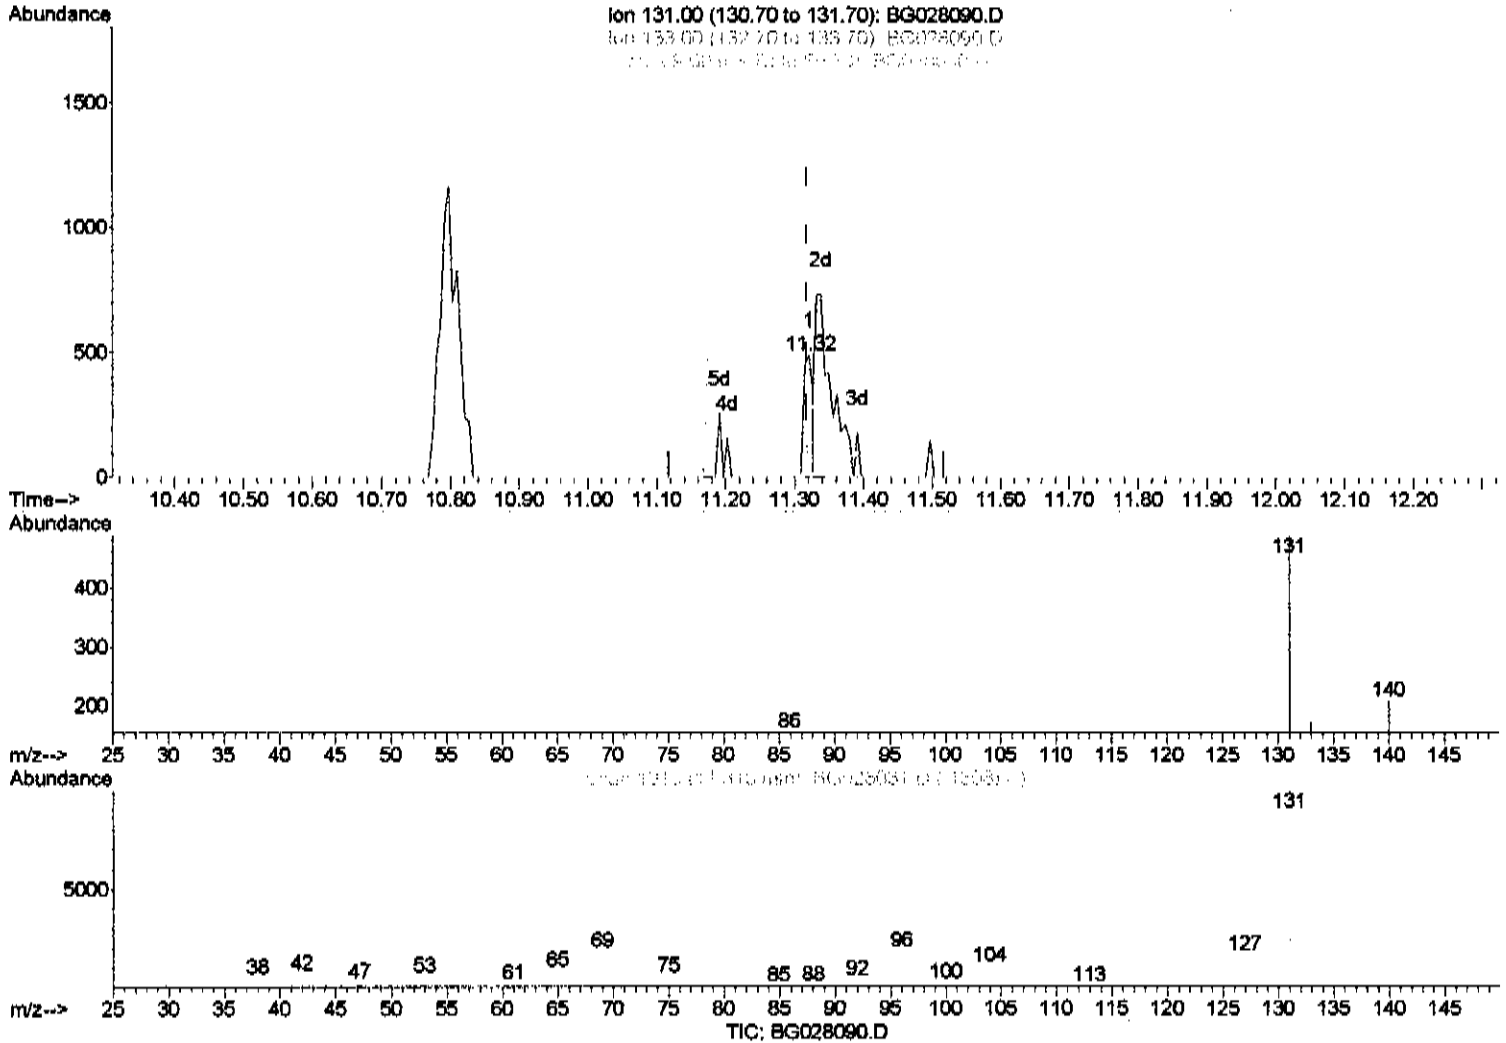

(29) 4-Chloroaniline-d4 (S)

11.320min (+0.004) 0.18ng/ul

response 453

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	34.97
69.00	18.60	0.00%
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_G
ClientSampled :
C0AE3

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG073117\
Data File : BG028090.D
Acq On : 1 Aug 2017 3:55
Operator : SJ/JU
Sample : I4504-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
8/1/2017 2:55:32 PM

Quant Time: Aug 01 10:34:45 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG072717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 01 02:25:43 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	31786	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	141847	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.97	164	118617	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.72	188	352038	20.00	ng/ul	0.00
78) Chrysene-d12	22.05	240	459855	20.00	ng/ul	0.00
86) Perylene-d12	25.57	264	470985	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.85	96	2705	5.51	ng/uL	0.00
5) Phenol-d5	7.51	99	13007	5.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	29295	24.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	43273	21.38	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	27888	13.01	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	27822	28.06	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	34693	27.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	61843	24.88	ng/ul	0.00
29) 4-Chloroaniline-d4	11.34	131	1665m	0.66	ng/ul	0.02
44) Dimethylphthalate-d6	14.36	166	321407	29.94	ng/ul	0.00
47) Acenaphthylene-d8	14.67	160	322937	27.81	ng/ul	0.00
52) 4-Nitrophenol-d4	15.16	143	6982	4.33	ng/ul	0.00
58) Fluorene-d10	15.96	176	285680	28.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.07	200	62486	24.92	ng/ul	0.00
71) Anthracene-d10	17.82	188	509825	30.24	ng/ul	0.00
79) Pyrene-d10	20.09	212	658519	32.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.32	264	650445	30.02	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed