


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG073119\
 Data File : BG041835.D
 Acq On : 31 Jul 2019 16:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 08:57:26 2019

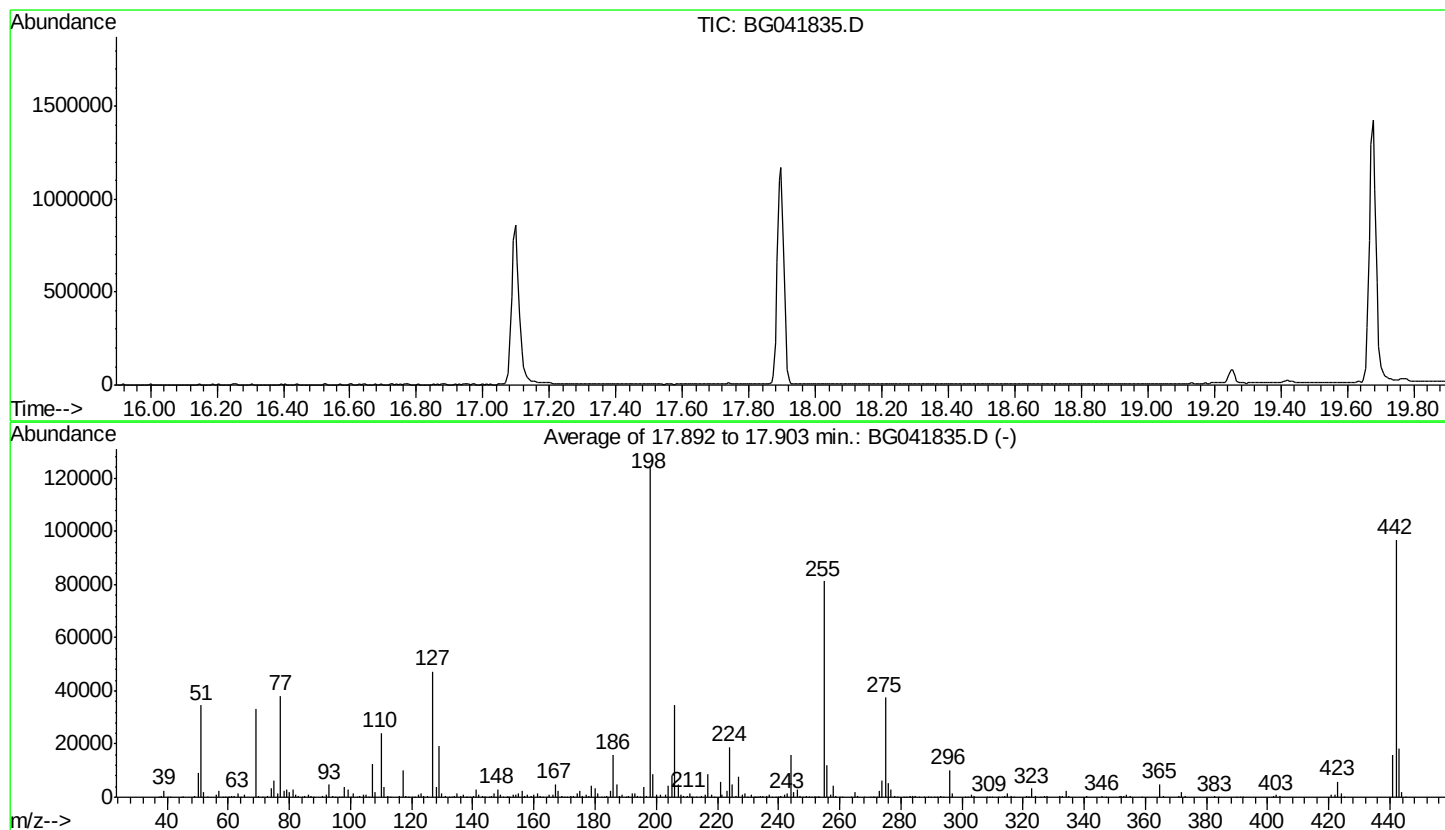

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	34432	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.7	33272	PASS
70	69	0.00	2	0.8	266	PASS
127	198	10	80	37.9	47253	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124661	PASS
199	198	5	9	7.0	8714	PASS
275	198	10	60	30.0	37410	PASS
365	198	1	100	3.9	4875	PASS
441	198	0.01	100	12.9	16028	PASS
442	198	50	100	77.6	96778	PASS
443	442	15	24	19.1	18480	PASS