
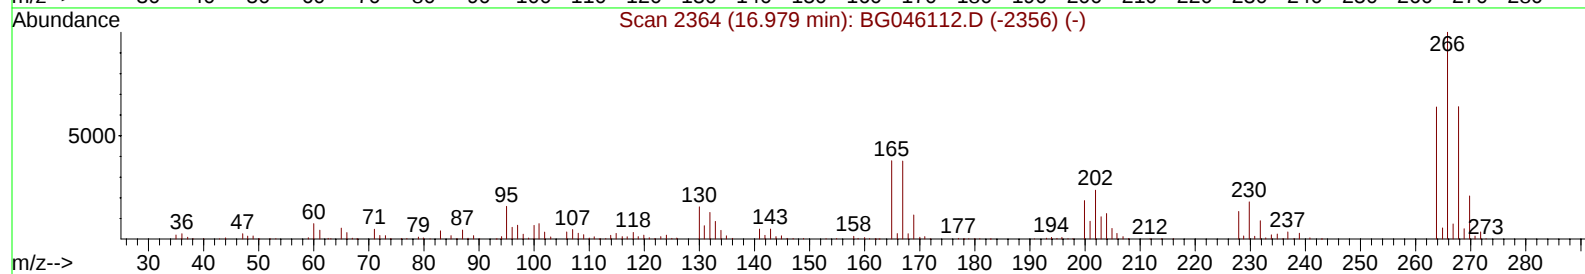
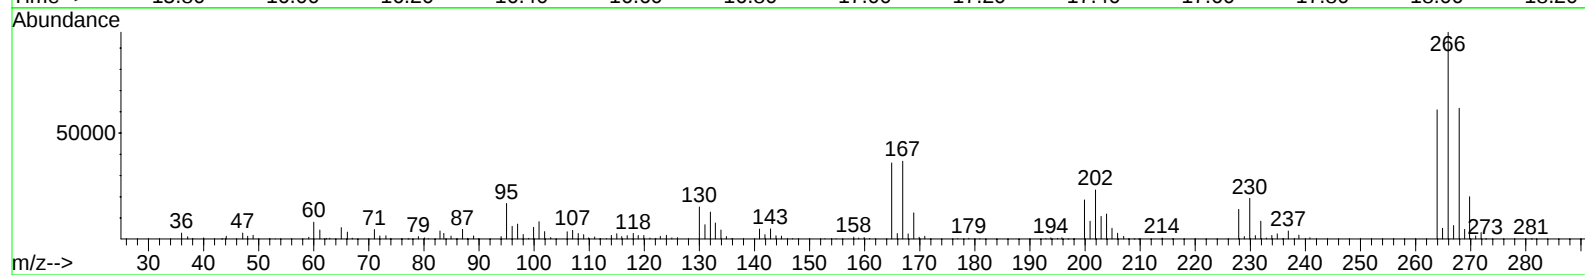


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
Data File : BG046117.D
Acq On : 31 Jul 2020 8:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:02:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

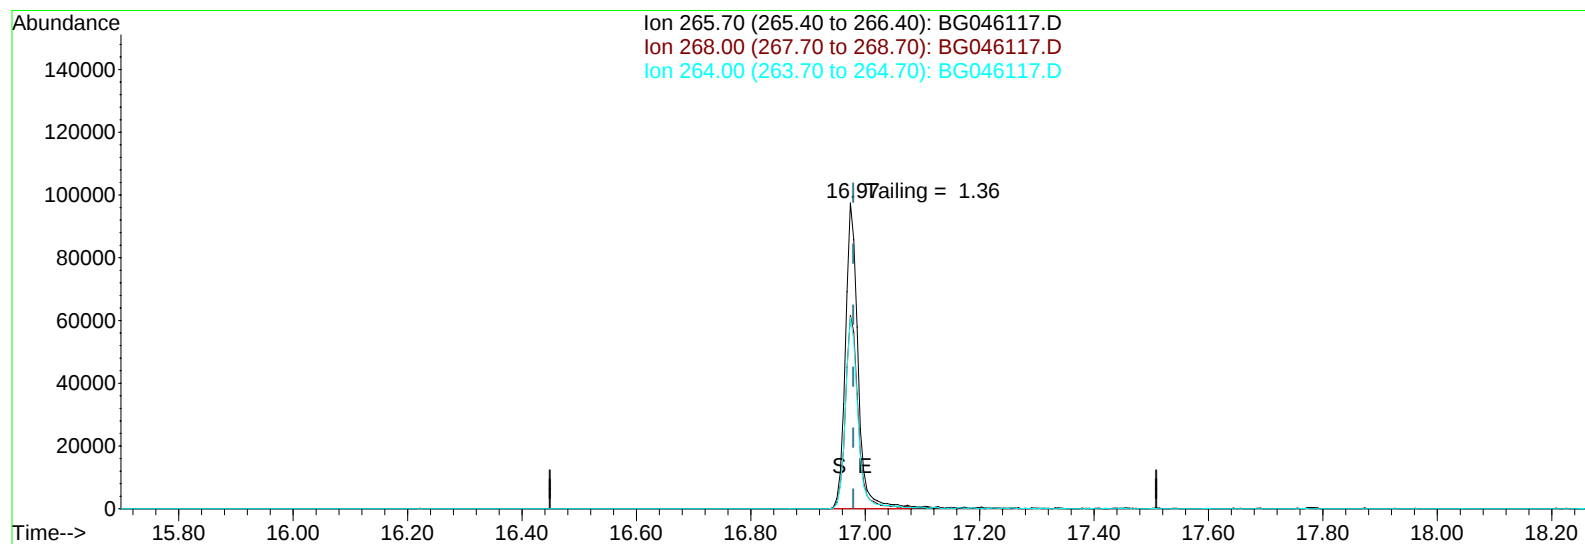

TIC: BG046117.D

(70) Pentachlorophenol (C)




16.974min (-0.005) 284063.92ng

response 150643

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.27
264.00	63.90	62.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
Data File : BG046117.D
Acq On : 31 Jul 2020 8:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:02:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

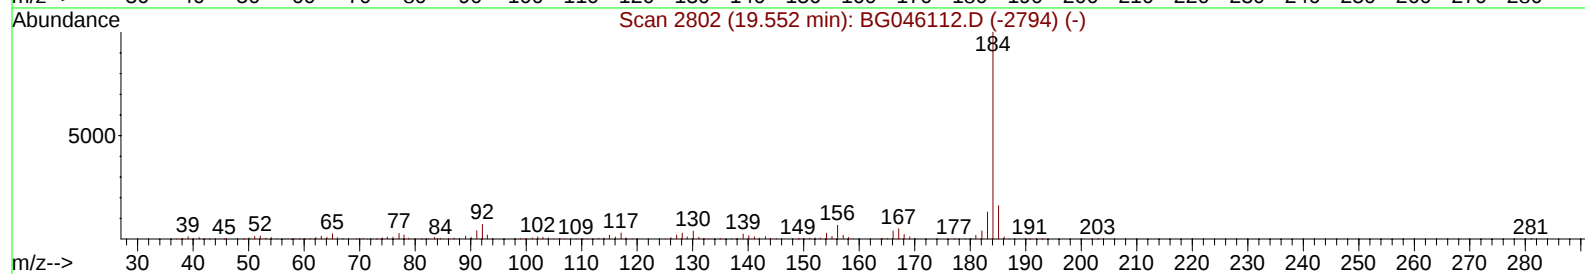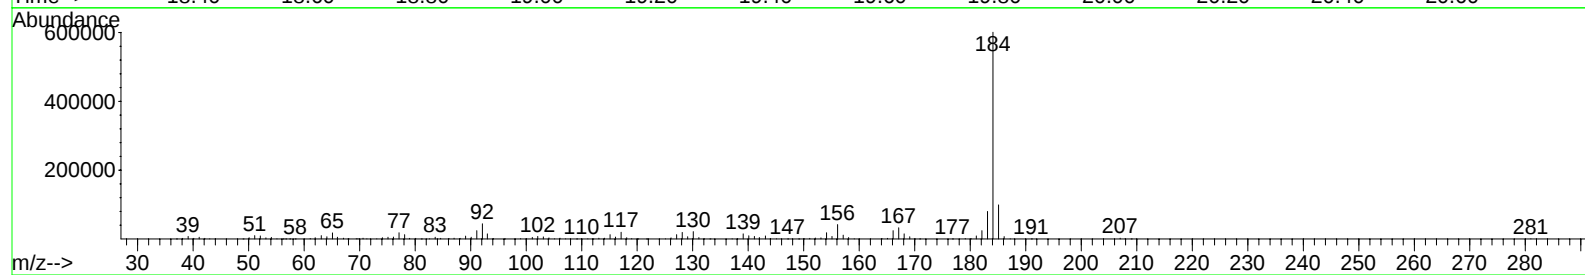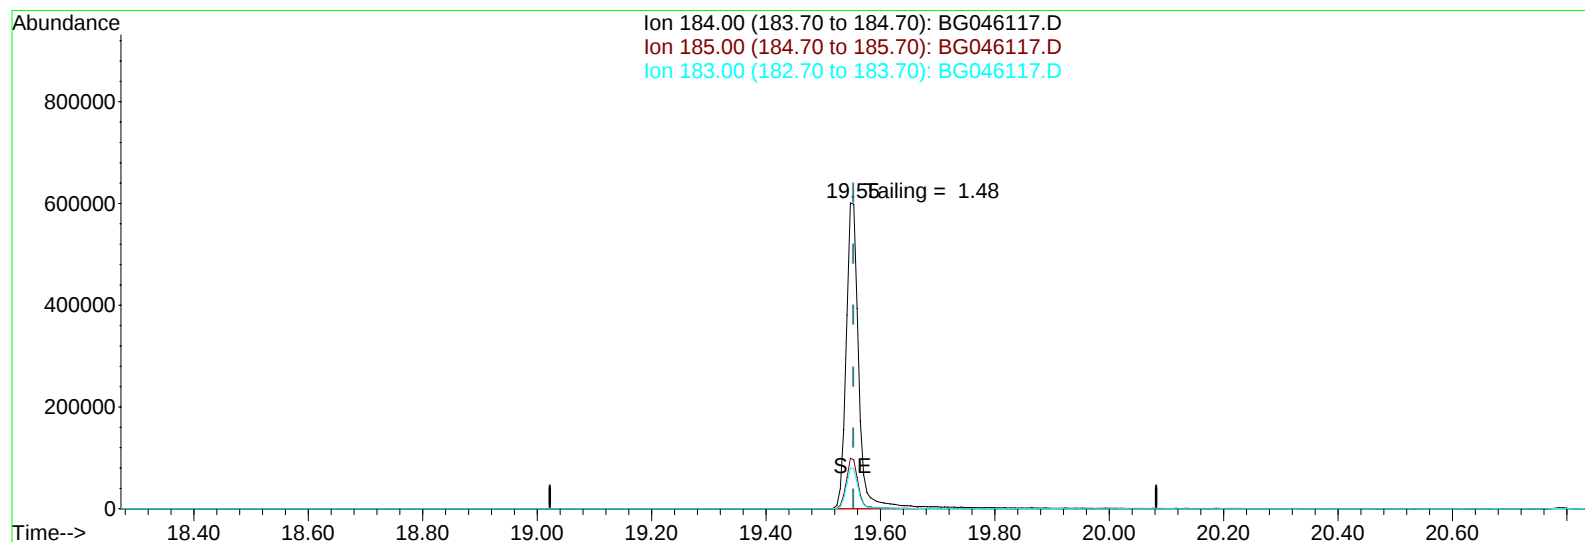

TIC: BG046117.D

(77) Benzidine

19.547min (-0.005) 6671.05ng

response 935739

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	16.54
183.00	13.10	13.33
0.00	0.00	0.00