
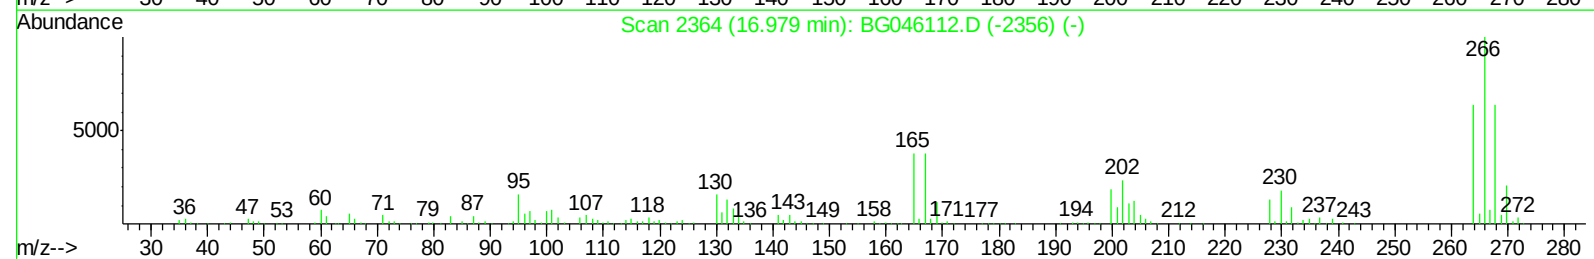
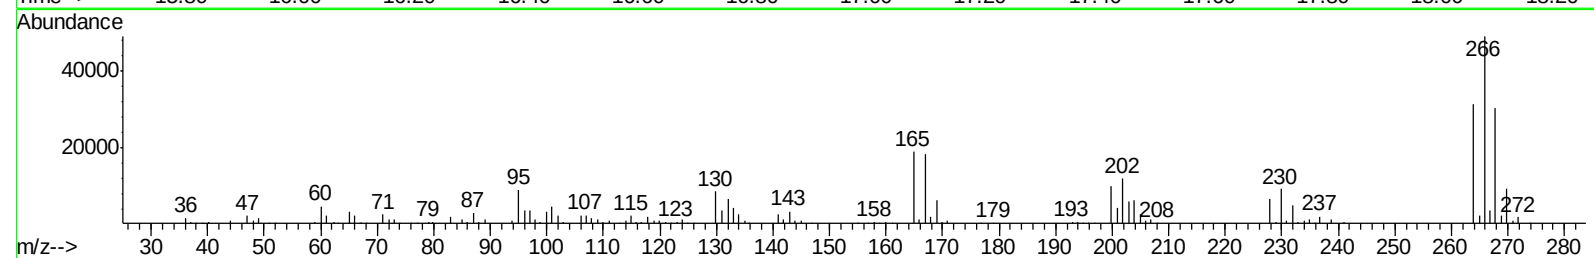


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
 Data File : BG046134.D
 Acq On : 31 Jul 2020 21:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 22:16:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

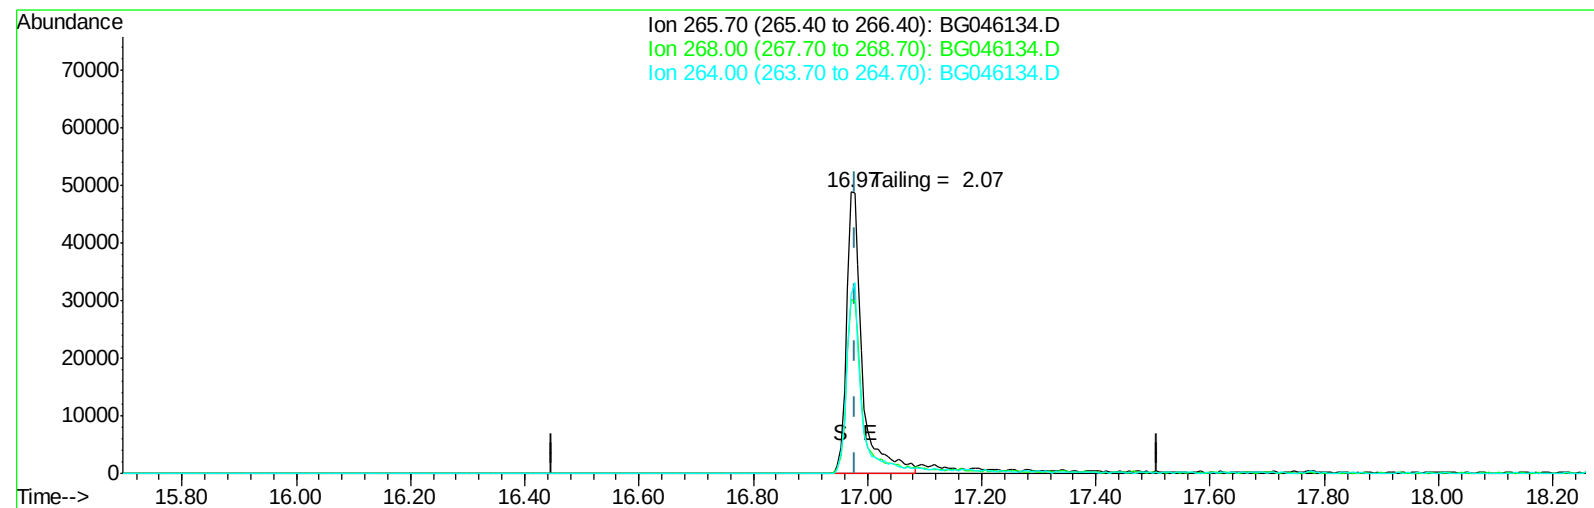

TIC: BG046134.D

(70) Pentachlorophenol (C)




16.971min (-0.008) 195512.64ng

response 93139

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.74
264.00	63.90	63.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
Data File : BG046134.D
Acq On : 31 Jul 2020 21:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 22:16:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

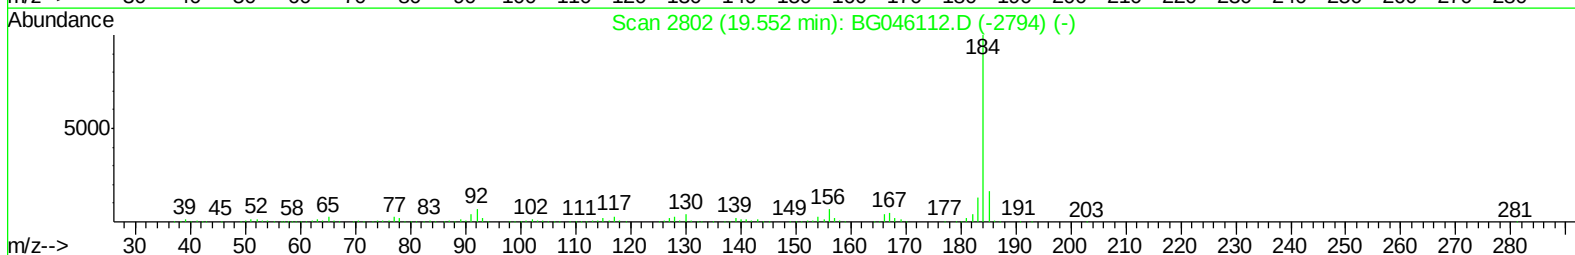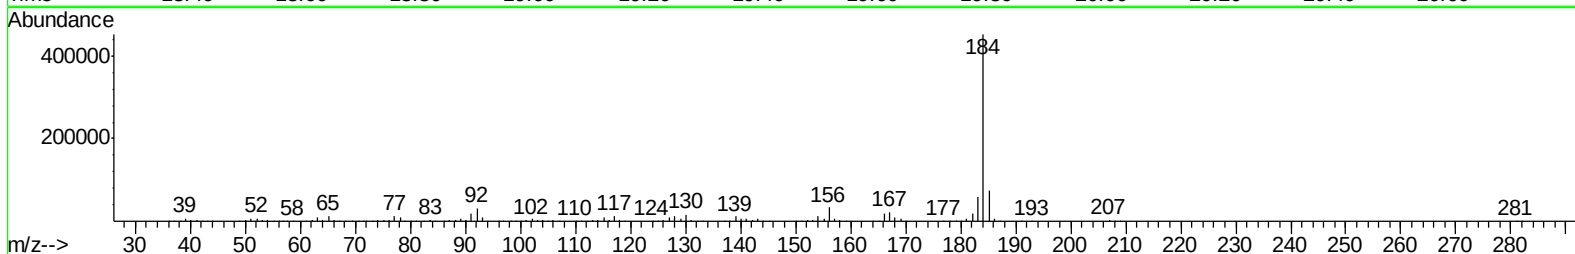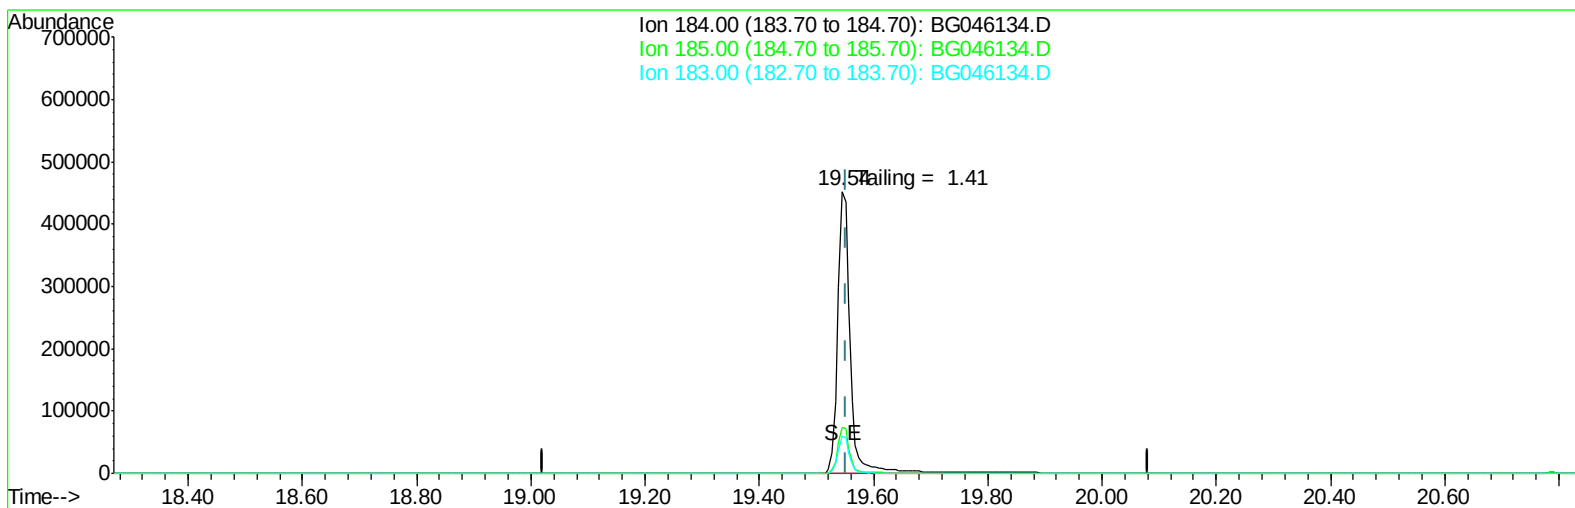

TIC: BG046134.D

(77) Benzidine

19.545min (-0.008) 295425.08ng

response 686185

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	16.56
183.00	13.10	12.99
0.00	0.00	0.00