

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
 Data File : BG046119.D
 Acq On : 31 Jul 2020 10:40
 Operator : CG/JU
 Sample : PB130544BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB130544BL

Quant Time: Jul 31 12:41:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	83672	20.00	ng	0.00
21) Naphthalene-d8	10.75	136	333981	20.00	ng	0.00
39) Acenaphthene-d10	14.58	164	216716	20.00	ng	0.00
64) Phenanthrene-d10	17.32	188	527854	20.00	ng	0.00
76) Chrysene-d12	21.57	240	639203	20.00	ng	0.00
86) Perylene-d12	24.67	264	627217	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	639854	132.94	ng	0.00
7) Phenol-d6	7.12	99	817018	124.55	ng	0.00
23) Nitrobenzene-d5	9.10	82	519149	84.16	ng	0.00
42) 2,4,6-Tribromophenol	16.07	330	394848	118.62	ng	0.00
45) 2-Fluorobiphenyl	13.21	172	1202670	80.61	ng	0.00
79) Terphenyl-d14	19.94	244	2119013	67.52	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
Data File : BG046119.D
Acq On : 31 Jul 2020 10:40
Operator : CG/JU
Sample : PB130544BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB130544BL

Quant Time: Jul 31 12:41:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

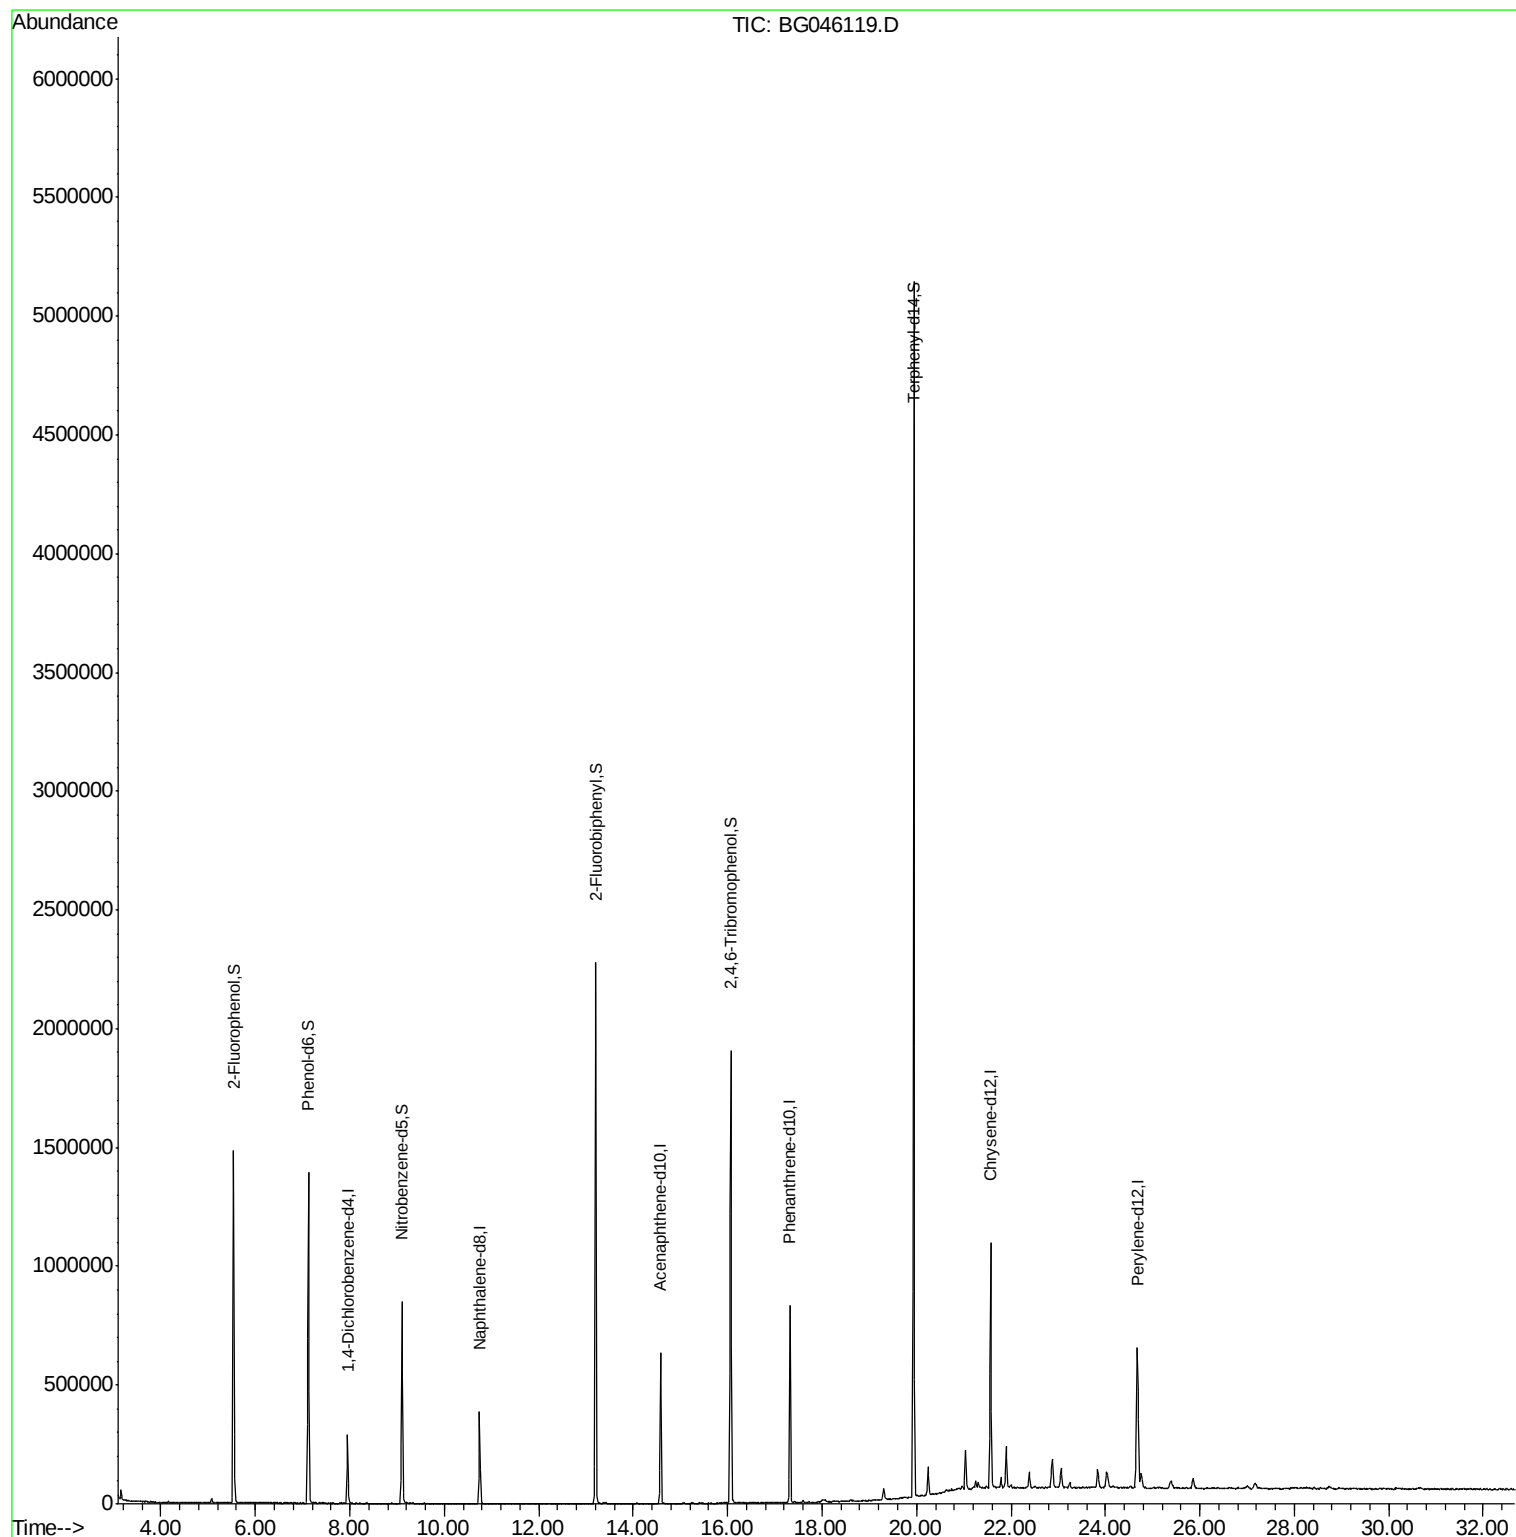

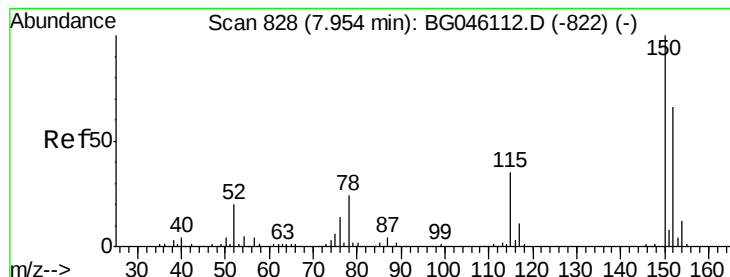


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.95 min Scan# 828
Delta R.T. -0.00 min
Lab File: BG046119.D
Acq: 31 Jul 2020 10:40

Instrument :
BNA_G
ClientSampleId :
PB130544BL

Tot Ion:152 Resp: 83672
Ion Ratio Lower Upper
152 100
150 157.3 122.1 183.1
115 53.7 43.2 64.8

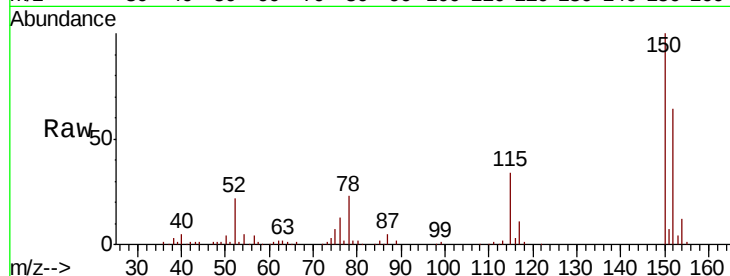


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

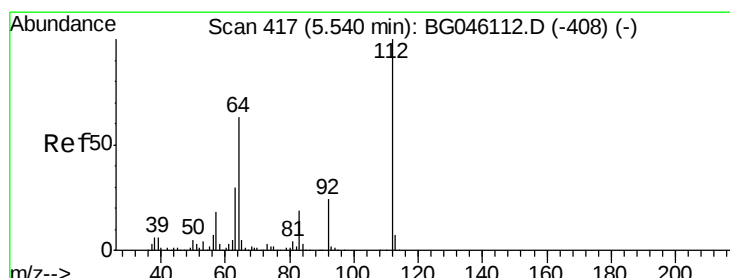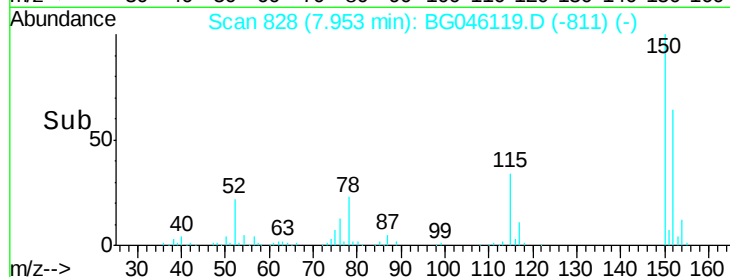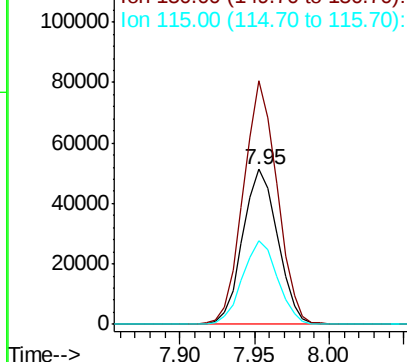



#5


2-Fluorophenol
Concen: 132.936 ng
RT: 5.54 min Scan# 417
Delta R.T. -0.00 min
Lab File: BG046119.D
Acq: 31 Jul 2020 10:40

Tgt Ion:112 Resp: 639854
Ion Ratio Lower Upper
112 100
64 64.4 50.2 75.2
63 32.6 24.2 36.4

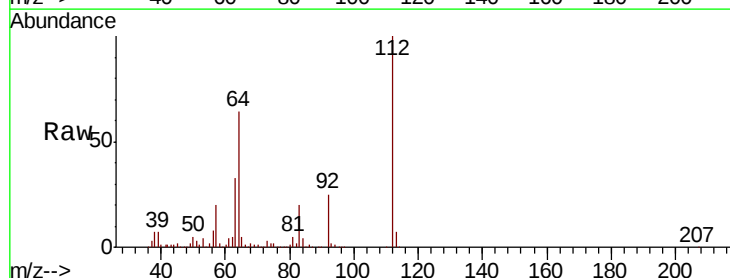

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

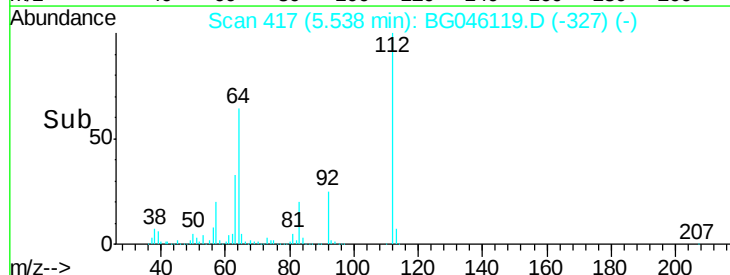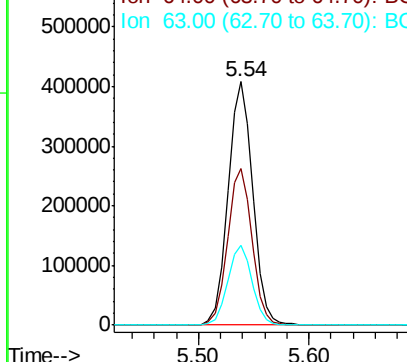

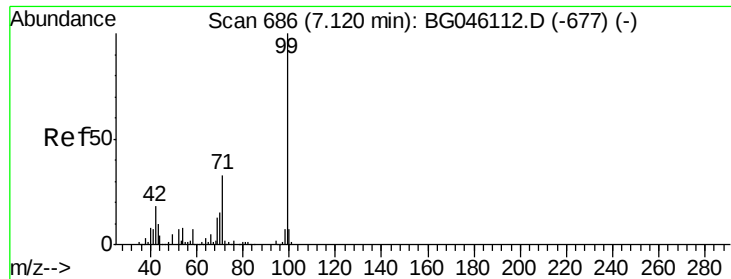

#7

Phenol-d6

Concen: 124.549 ng

RT: 7.12 min Scan# 686

Delta R.T. -0.00 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40

Instrument :

BNA_G

ClientSampleId :

PB130544BL


Tot Ion: 99 Resp: 817018

Ion Ratio Lower Upper




99 100

42 19.7 14.7 22.1

71 33.6 26.5 39.7

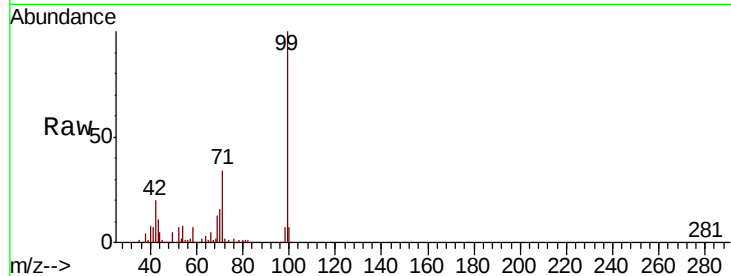

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

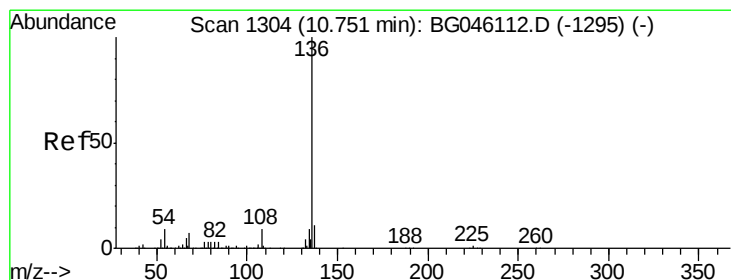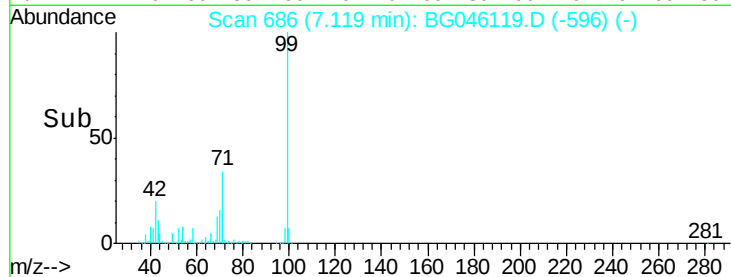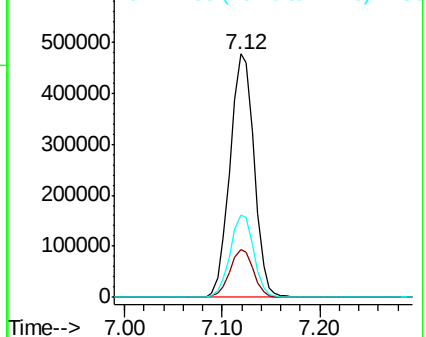

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.75 min Scan# 1304

Delta R.T. -0.00 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40

Tgt Ion: 136 Resp: 333981


Ion Ratio Lower Upper

136 100



137 11.5 8.8 13.2


54 9.3 7.0 10.4

68 6.1 5.3 7.9

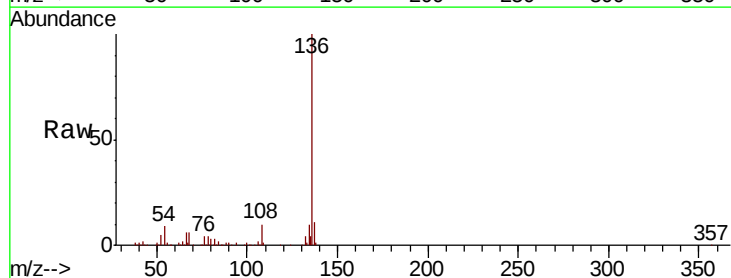

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



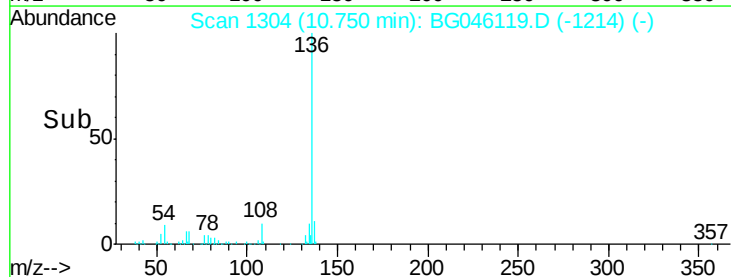
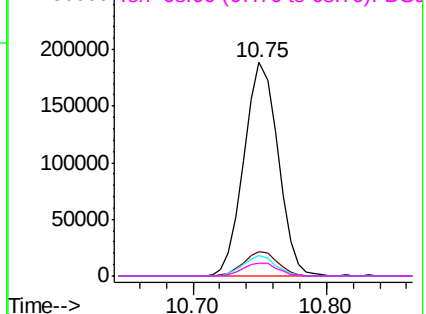


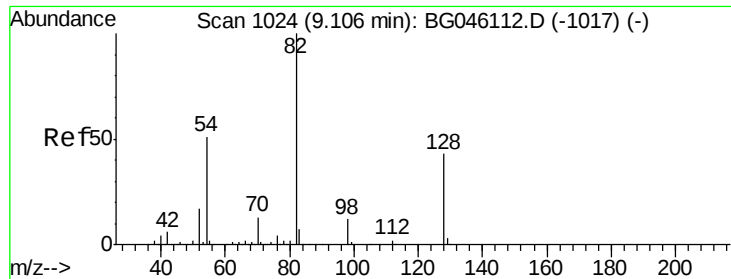

#23
 Nitrobenzene-d5
 Concen: 84.161 ng
 RT: 9.10 min Scan# 1024
 Delta R.T. -0.00 min
 Lab File: BG046119.D
 Acq: 31 Jul 2020 10:40




Instrument :
 BNA_G
 ClientSampleId :
 PB130544BL


Tot Ion	82	Resp	519149
Ion Ratio	Lower	Upper	
82	100		
128	42.7	34.4	51.6
54	53.3	40.8	61.2

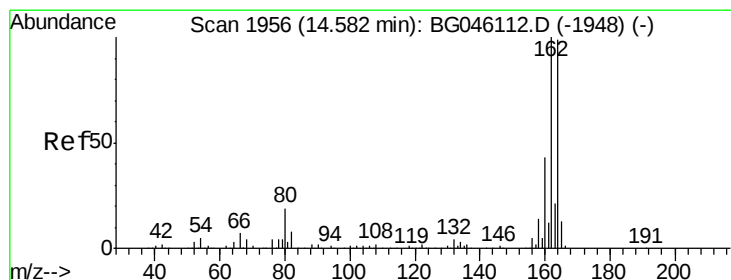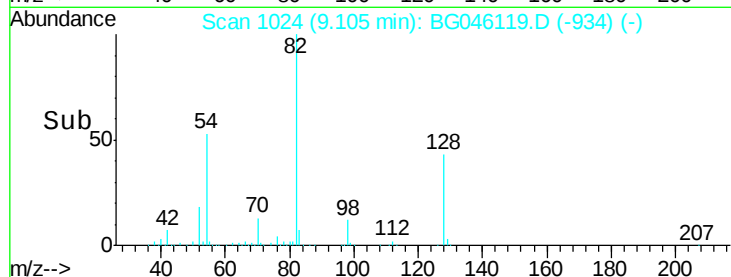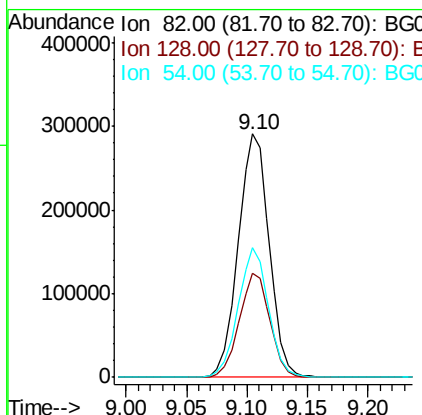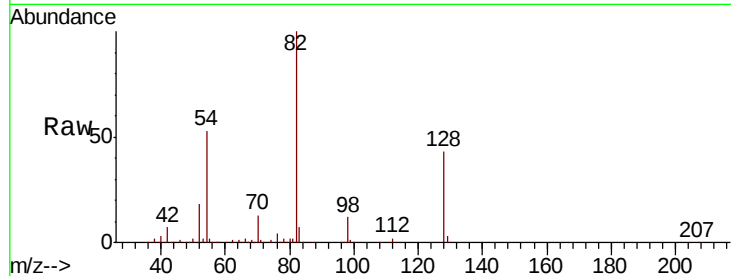

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.58 min Scan# 1956
 Delta R.T. -0.00 min
 Lab File: BG046119.D
 Acq: 31 Jul 2020 10:40

Tgt Ion	164	Resp	216716
Ion Ratio	Lower	Upper	
164	100		
162	107.0	80.6	121.0
160	44.4	34.9	52.3

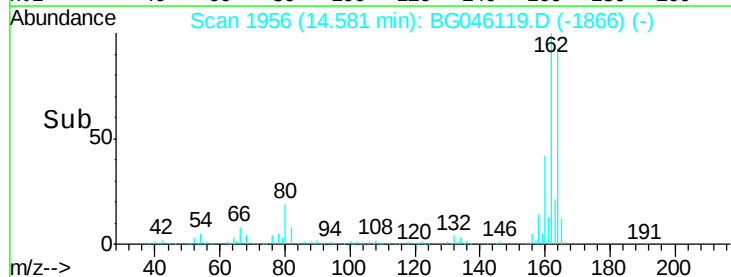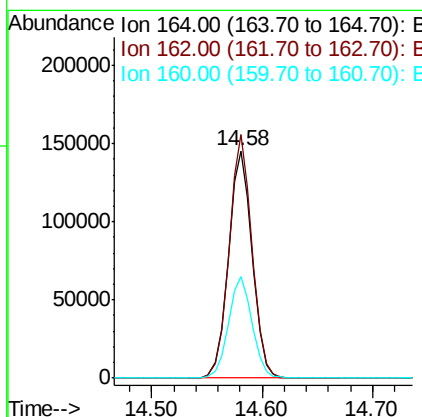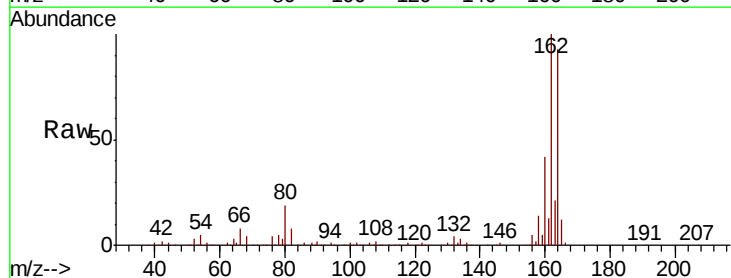


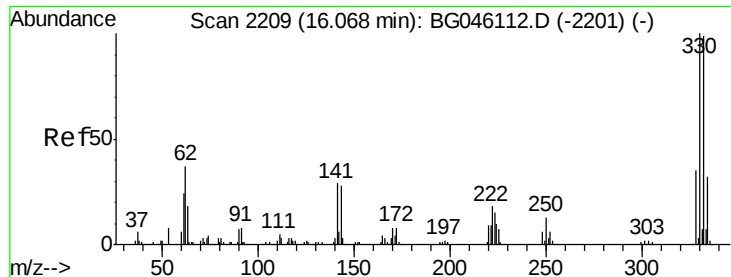




#42
 2,4,6-Tribromophenol
 Concen: 118.619 ng
 RT: 16.07 min Scan# 2209
 Delta R.T. -0.00 min
 Lab File: BG046119.D
 Acq: 31 Jul 2020 10:40

Instrument :
 BNA_G
 ClientSampleId :
 PB130544BL

Tot Ion:330 Resp: 394848
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.4 116.2
 141 30.6 23.4 35.0

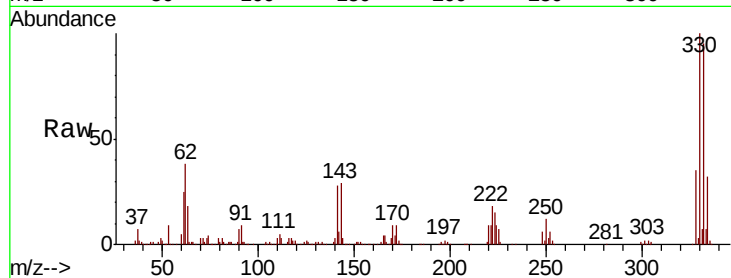


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

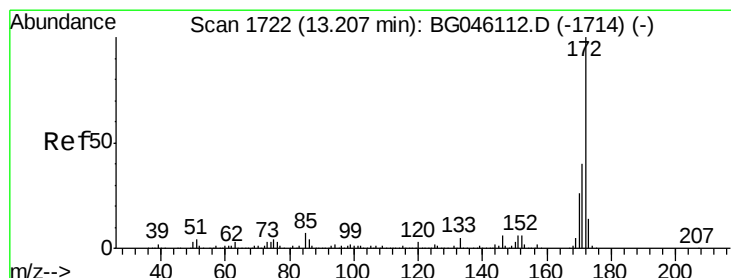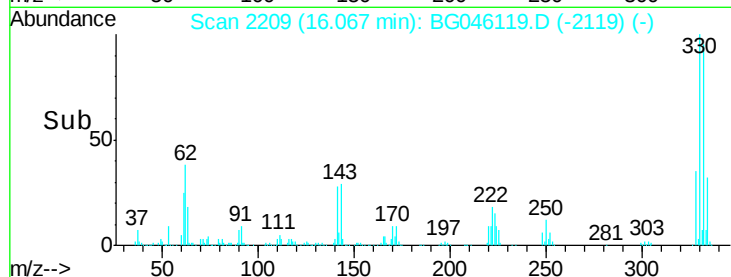
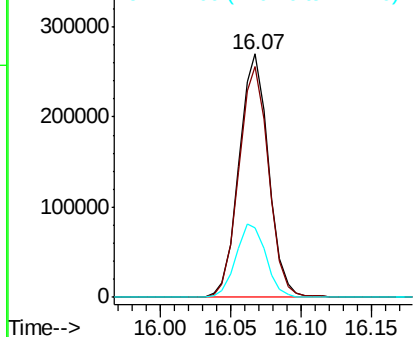



#45
 2-Fluorobiphenyl
 Concen: 80.614 ng
 RT: 13.21 min Scan# 1722
 Delta R.T. -0.00 min
 Lab File: BG046119.D
 Acq: 31 Jul 2020 10:40

Tgt Ion:172 Resp: 1202670
 Ion Ratio Lower Upper
 172 100
 171 38.7 31.7 47.5
 170 25.6 20.9 31.3

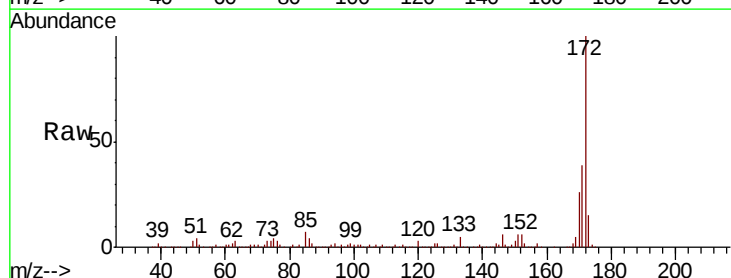

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

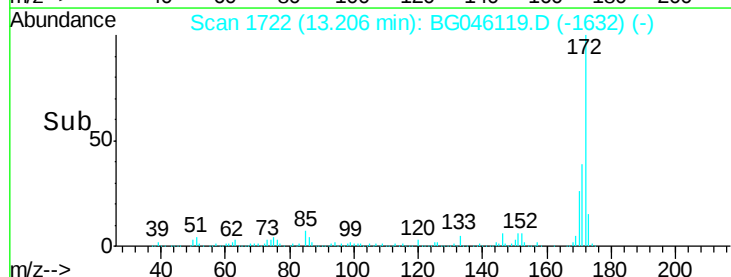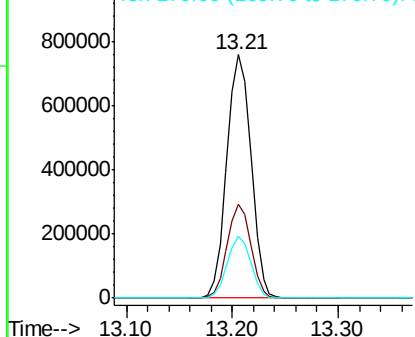

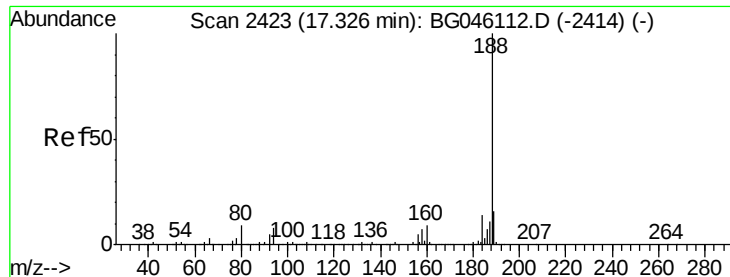

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.32 min Scan# 2422

Delta R.T. -0.01 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40

Instrument :

BNA_G

ClientSampleId :

PB130544BL


Tot Ion:188 Resp: 527854

Ion Ratio Lower Upper

188 100

94 7.9 6.4 9.6




80 9.2 7.4 11.0

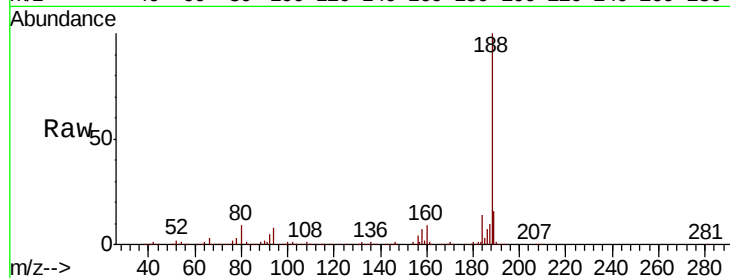

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

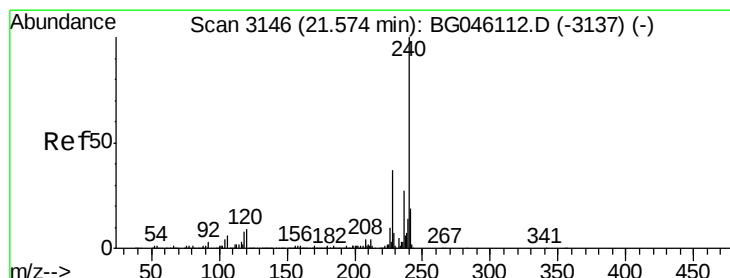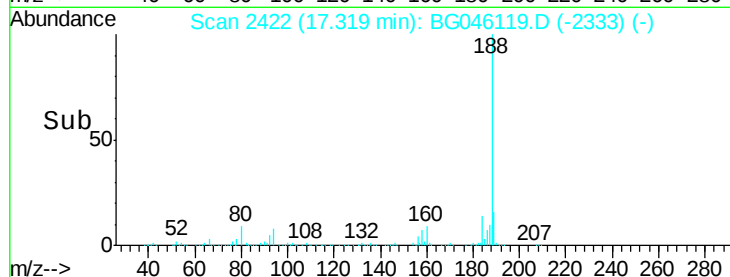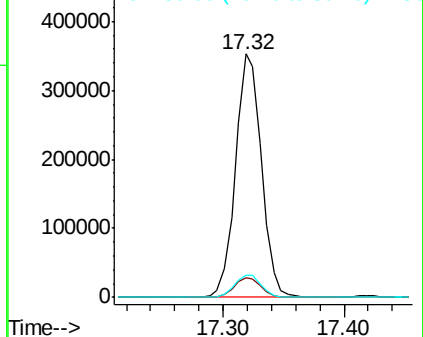

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.57 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40


Tgt Ion:240 Resp: 639203

Ion Ratio Lower Upper

240 100

120 8.9 7.1 10.7



236 26.6 21.7 32.5

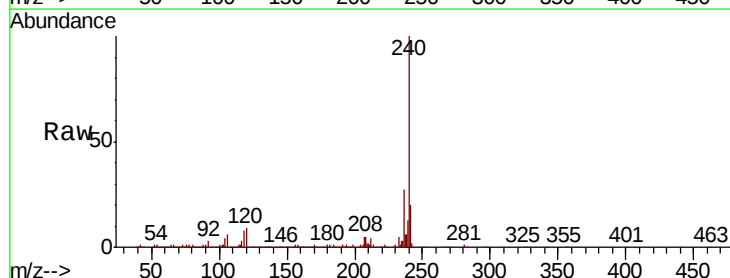


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

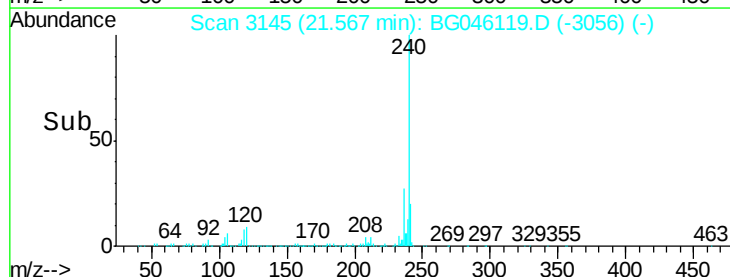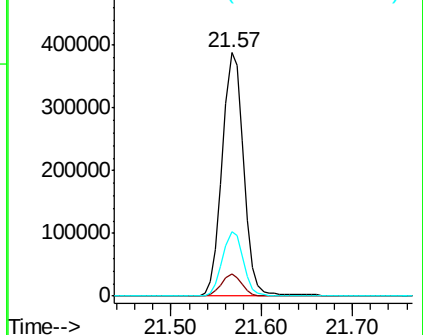

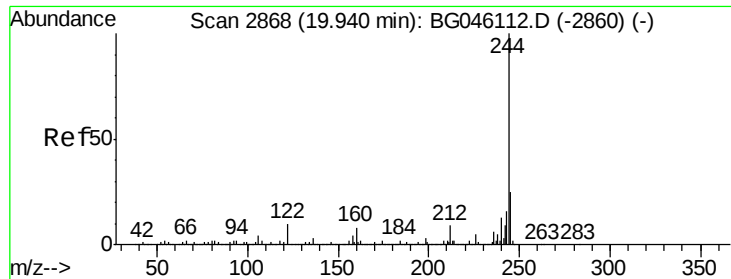

#79

Terphenyl-d14

Concen: 67.516 ng

RT: 19.94 min Scan# 2868

Delta R.T. -0.00 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40

Instrument :

BNA_G

ClientSampleId :

PB130544BL


Tot Ion:244 Resp: 2119013

Ion Ratio Lower Upper

244 100

212 9.5 7.2 10.8




122 11.4 8.3 12.5

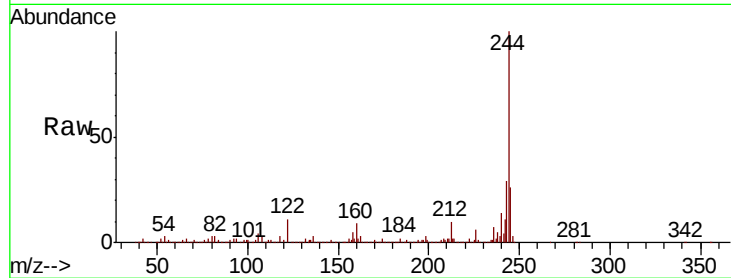

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

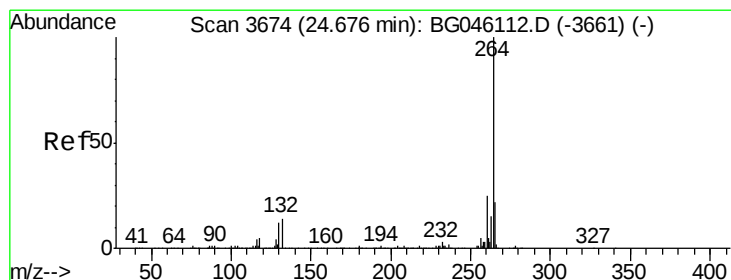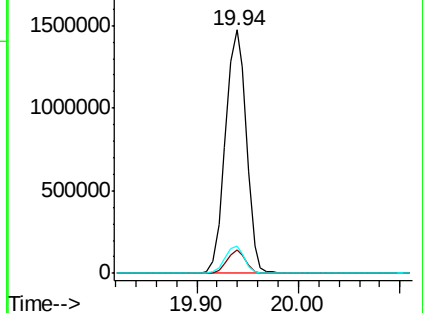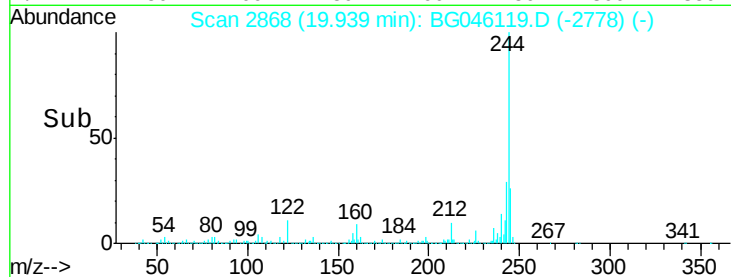

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.67 min Scan# 3674

Delta R.T. -0.00 min

Lab File: BG046119.D

Acq: 31 Jul 2020 10:40


Tgt Ion:264 Resp: 627217

Ion Ratio Lower Upper

264 100

260 24.8 19.7 29.5

265 21.8 17.6 26.4

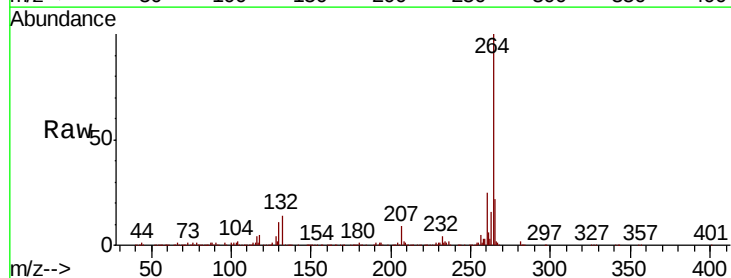

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

