


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073120\
 Data File : BG046117.D
 Acq On : 31 Jul 2020 8:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 18:43:49 2020

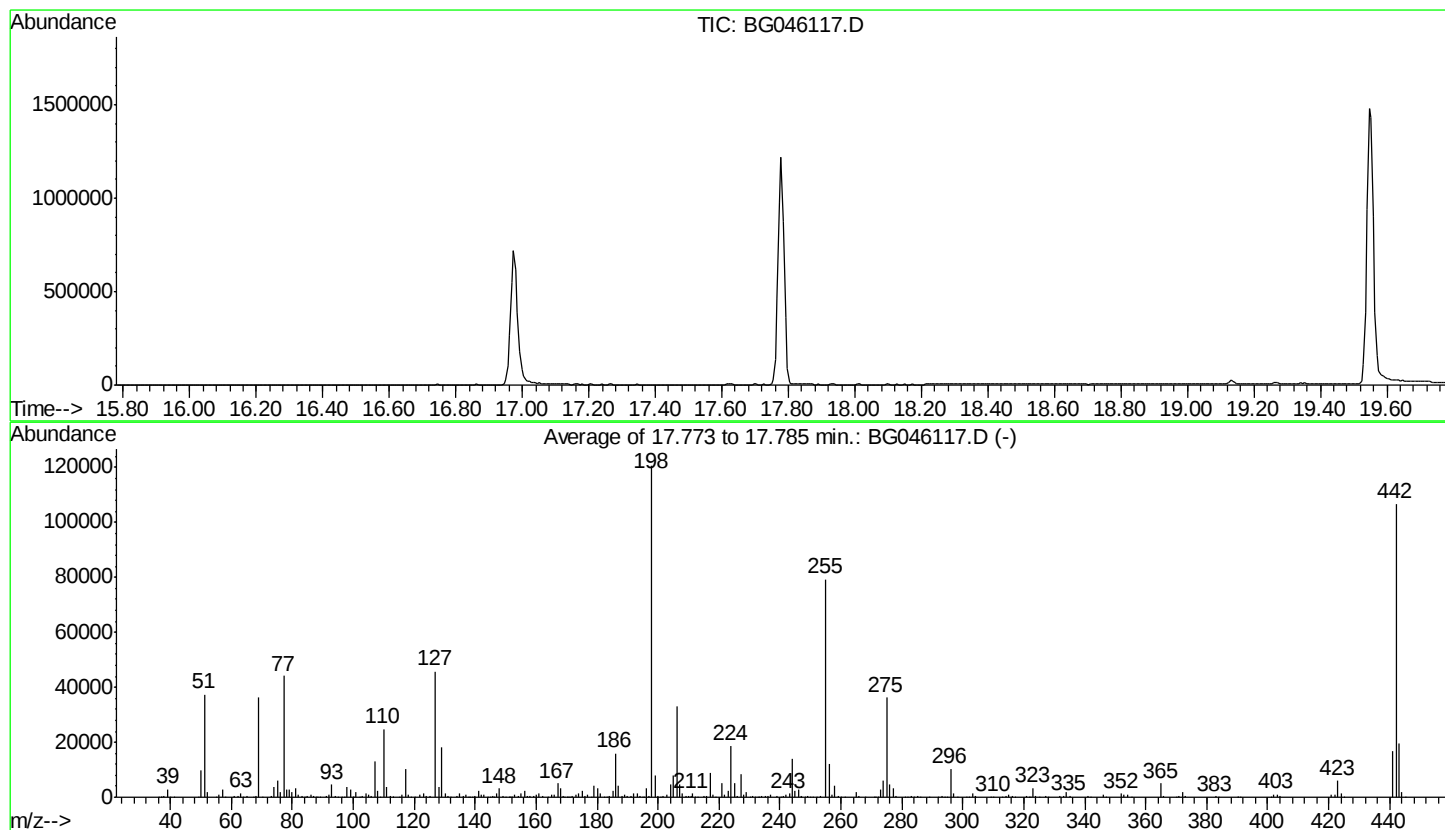

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	37282	PASS
68	69	0.00	2	0.8	302	PASS
69	198	0.00	100	30.2	36392	PASS
70	69	0.00	2	0.6	212	PASS
127	198	10	80	38.0	45832	PASS
197	198	0.00	2	0.3	365	PASS
198	198	100	100	100.0	120677	PASS
199	198	5	9	6.8	8161	PASS
275	198	10	60	30.0	36208	PASS
365	198	1	100	4.1	5004	PASS
441	198	0.01	100	13.9	16767	PASS
442	198	50	100	88.5	106792	PASS
443	442	15	24	18.5	19806	PASS