


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073120\
 Data File : BG046134.D
 Acq On : 31 Jul 2020 21:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 18:43:49 2020

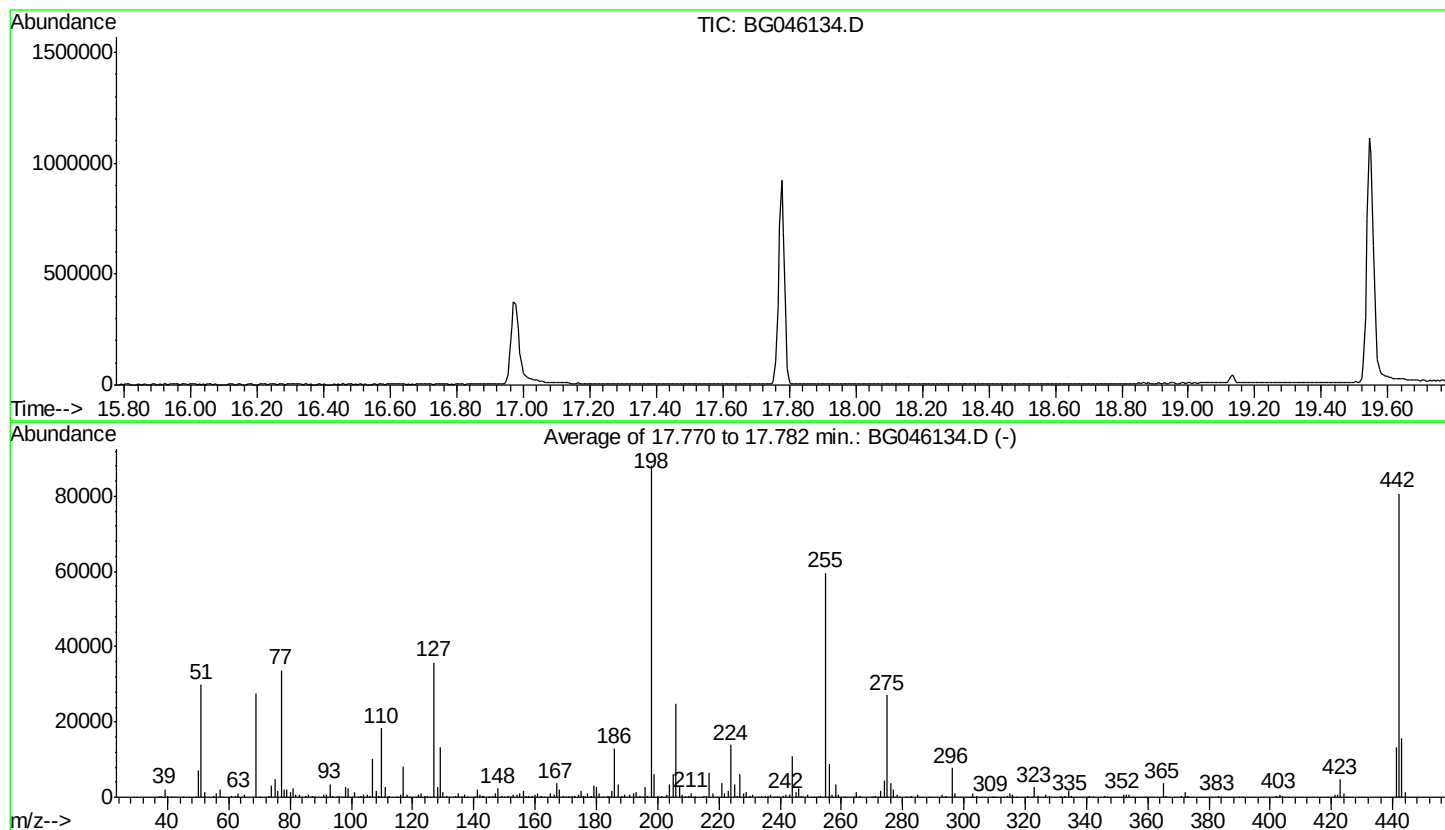

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	29878	PASS
68	69	0.00	2	0.4	105	PASS
69	198	0.00	100	31.4	27688	PASS
70	69	0.00	2	0.5	129	PASS
127	198	10	80	40.6	35770	PASS
197	198	0.00	2	0.3	265	PASS
198	198	100	100	100.0	88149	PASS
199	198	5	9	7.0	6135	PASS
275	198	10	60	30.8	27133	PASS
365	198	1	100	4.2	3697	PASS
441	198	0.01	100	15.3	13443	PASS
442	198	50	100	91.6	80704	PASS
443	442	15	24	19.5	15750	PASS