

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
 Data File : BG062230.D
 Acq On : 31 Jul 2024 23:10
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020588

Quant Time: Aug 01 04:06:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 01 03:46:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.978	152	41899	20.000	ng/ul	0.00
20) Naphthalene-d8	10.774	136	195072	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	146668	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.336	188	350702	20.000	ng/ul	0.00
79) Chrysene-d12	21.589	240	349105	20.000	ng/ul	0.00
88) Perylene-d12	24.696	264	384707	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.437	96	7045	7.156	ng/uL	0.00
4) Pyridine-d5	3.842	84	56753	18.877	ng/ul	0.00
7) Phenol-d5	7.126	99	75648	18.866	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.308	67	47233	19.101	ng/ul	0.00
11) 2-Chlorophenol-d4	7.508	132	55595	20.613	ng/ul	0.00
15) 4-Methylphenol-d8	8.671	113	63849	19.132	ng/ul	0.00
21) Nitrobenzene-d5	9.129	128	24185	29.892	ng/ul	0.00
24) 2-Nitrophenol-d4	9.852	143	24219	31.951	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.386	165	62409	21.989	ng/ul	0.00
31) 4-Chloroaniline-d4	10.897	131	93952	19.565	ng/ul	0.00
46) Dimethylphthalate-d6	14.011	166	220606	19.959	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	241082	19.757	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	34810	26.241	ng/ul	0.00
60) Fluorene-d10	15.591	176	194193	19.773	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.697	200	22106	26.591	ng/ul	0.00
73) Anthracene-d10	17.436	188	318521	19.709	ng/ul	0.00
81) Pyrene-d10	19.721	212	398044	20.373	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.479	264	382259	20.325	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.478	88	7899	6.505	ng/uL	88
5) Pyridine	3.860	79	59898	18.684	ng/ul	94
6) Benzaldehyde	7.114	77	50306	23.243	ng/ul	98
8) Phenol	7.155	94	76937	18.602	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.402	93	59826	19.171	ng/ul	99
12) 2-Chlorophenol	7.537	128	56573	20.193	ng/ul	98
13) 2-Methylphenol	8.407	108	60643	18.993	ng/ul	94
14) 2,2'-oxybis(1-Chloropr...	8.512	45	128697	19.381	ng/ul#	98
16) Acetophenone	8.794	105	104555	19.291	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.783	70	58221	19.499	ng/ul#	96
18) 4-Methylphenol	8.736	108	66808	18.996	ng/ul	97
19) Hexachloroethane	9.065	117	23670	21.224	ng/ul	93
22) Nitrobenzene	9.170	77	69848	28.818	ng/ul	95
23) Isophorone	9.699	82	164363	19.083	ng/ul	96
25) 2-Nitrophenol	9.881	139	29115	33.158	ng/ul#	92
26) 2,4-Dimethylphenol	9.940	107	74956	19.589	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.187	93	88002	18.879	ng/ul	99
29) 2,4-Dichlorophenol	10.416	162	62161	21.946	ng/ul	99
30) Naphthalene	10.827	128	212764	19.626	ng/ul	99
32) 4-Chloroaniline	10.927	127	90823	19.685	ng/ul	99
33) Hexachlorobutadiene	11.121	225	44395	19.799	ng/ul	96
34) Caprolactam	11.667	113	11304	9.368	ng/ul	84
35) 4-Chloro-3-methylphenol	12.037	107	71323	19.367	ng/ul	99
36) 2-Methylnaphthalene	12.431	142	140370	18.320	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
 Data File : BG062230.D
 Acq On : 31 Jul 2024 23:10
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 18 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 SSTD020588


Quant Time: Aug 01 04:06:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 01 03:46:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.648	142	150326	19.035	ng/ul#	95
39) 1,2,4,5-Tetrachloroben...	12.795	216	84152	19.387	ng/ul	98
40) Hexachlorocyclopentadiene	12.783	237	46912	20.812	ng/ul	97
41) 2,4,6-Trichlorophenol	13.024	196	50018	23.320	ng/ul	97
42) 2,4,5-Trichlorophenol	13.095	196	59590	24.568	ng/ul	99
43) 1,1'-Biphenyl	13.435	154	201318	19.028	ng/ul	98
44) 2-Chloronaphthalene	13.476	162	158579	19.111	ng/ul	97
45) 2-Nitroaniline	13.664	65	44078	30.045	ng/ul	98
47) Dimethylphthalate	14.058	163	222681	19.415	ng/ul	99
48) 2,6-Dinitrotoluene	14.164	165	33424	30.934	ng/ul	89
50) Acenaphthylene	14.316	152	269420	19.571	ng/ul	99
51) 3-Nitroaniline	14.487	138	35634	26.457	ng/ul#	83
52) Acenaphthene	14.663	153	190026	19.531	ng/ul	99
53) 2,4-Dinitrophenol	14.692	184	12417	21.935	ng/ul	89
55) 4-Nitrophenol	14.786	109	31033	24.189	ng/ul	92
56) Dibenzofuran	14.998	168	267006	19.805	ng/ul	99
57) 2,4-Dinitrotoluene	14.945	165	47504	32.182	ng/ul#	96
58) 2,3,4,6-Tetrachlorophenol	15.215	232	57118	24.742	ng/ul	97
59) Diethylphthalate	15.427	149	229408	19.509	ng/ul	100
61) Fluorene	15.644	166	214266	19.740	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.644	204	109313	19.897	ng/ul	98
63) 4-Nitroaniline	15.650	138	39721	26.528	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.709	198	23700	25.456	ng/ul#	97
67) N-Nitrosodiphenylamine	15.850	169	190639	19.535	ng/ul	98
68) 4-Bromophenyl-phenylether	16.537	248	72604	19.330	ng/ul	98
69) Hexachlorobenzene	16.643	284	81222	20.003	ng/ul	99
70) Atrazine	16.801	200	77835	20.725	ng/ul	98
71) Pentachlorophenol	16.983	266	46889	18.168	ng/ul	97
72) Phenanthrene	17.377	178	376986	19.924	ng/ul	99
74) Anthracene	17.471	178	385642	19.689	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.400	216	84901	19.627	ng/ul	98
76) Pentachlorobenzene	14.916	250	92730	20.271	ng/ul	99
77) Carbazole	17.735	167	332757	20.701	ng/ul	100
78) Di-n-butylphthalate	18.317	149	397691	19.950	ng/ul	99
80) Fluoranthene	19.386	202	453986	19.840	ng/ul	100
82) Pyrene	19.750	202	476968	19.996	ng/ul	99
83) Butylbenzylphthalate	20.655	149	172067	21.497	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.483	252	163467	21.536	ng/ul	97
85) Benzo(a)anthracene	21.565	228	489831	19.746	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.518	149	261891	20.931	ng/ul	100
87) Chrysene	21.630	228	461412	19.902	ng/ul	99
89) Di-n-octyl phthalate	22.705	149	456646	21.142	ng/ul	100
90) Benzo(b)fluoranthene	23.715	252	467645	19.539	ng/ul	99
91) Benzo(k)fluoranthene	23.780	252	483643	20.327	ng/ul	98
93) Benzo(a)pyrene	24.550	252	449141	19.843	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	28.221	276	522193	19.621	ng/ul	98
95) Dibenzo(a,h)anthracene	28.286	278	442591	19.834	ng/ul	100
96) Benzo(g,h,i)perylene	29.302	276	419868	19.654	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 01 04:06:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 01 03:46:07 2024
Response via : Initial Calibration




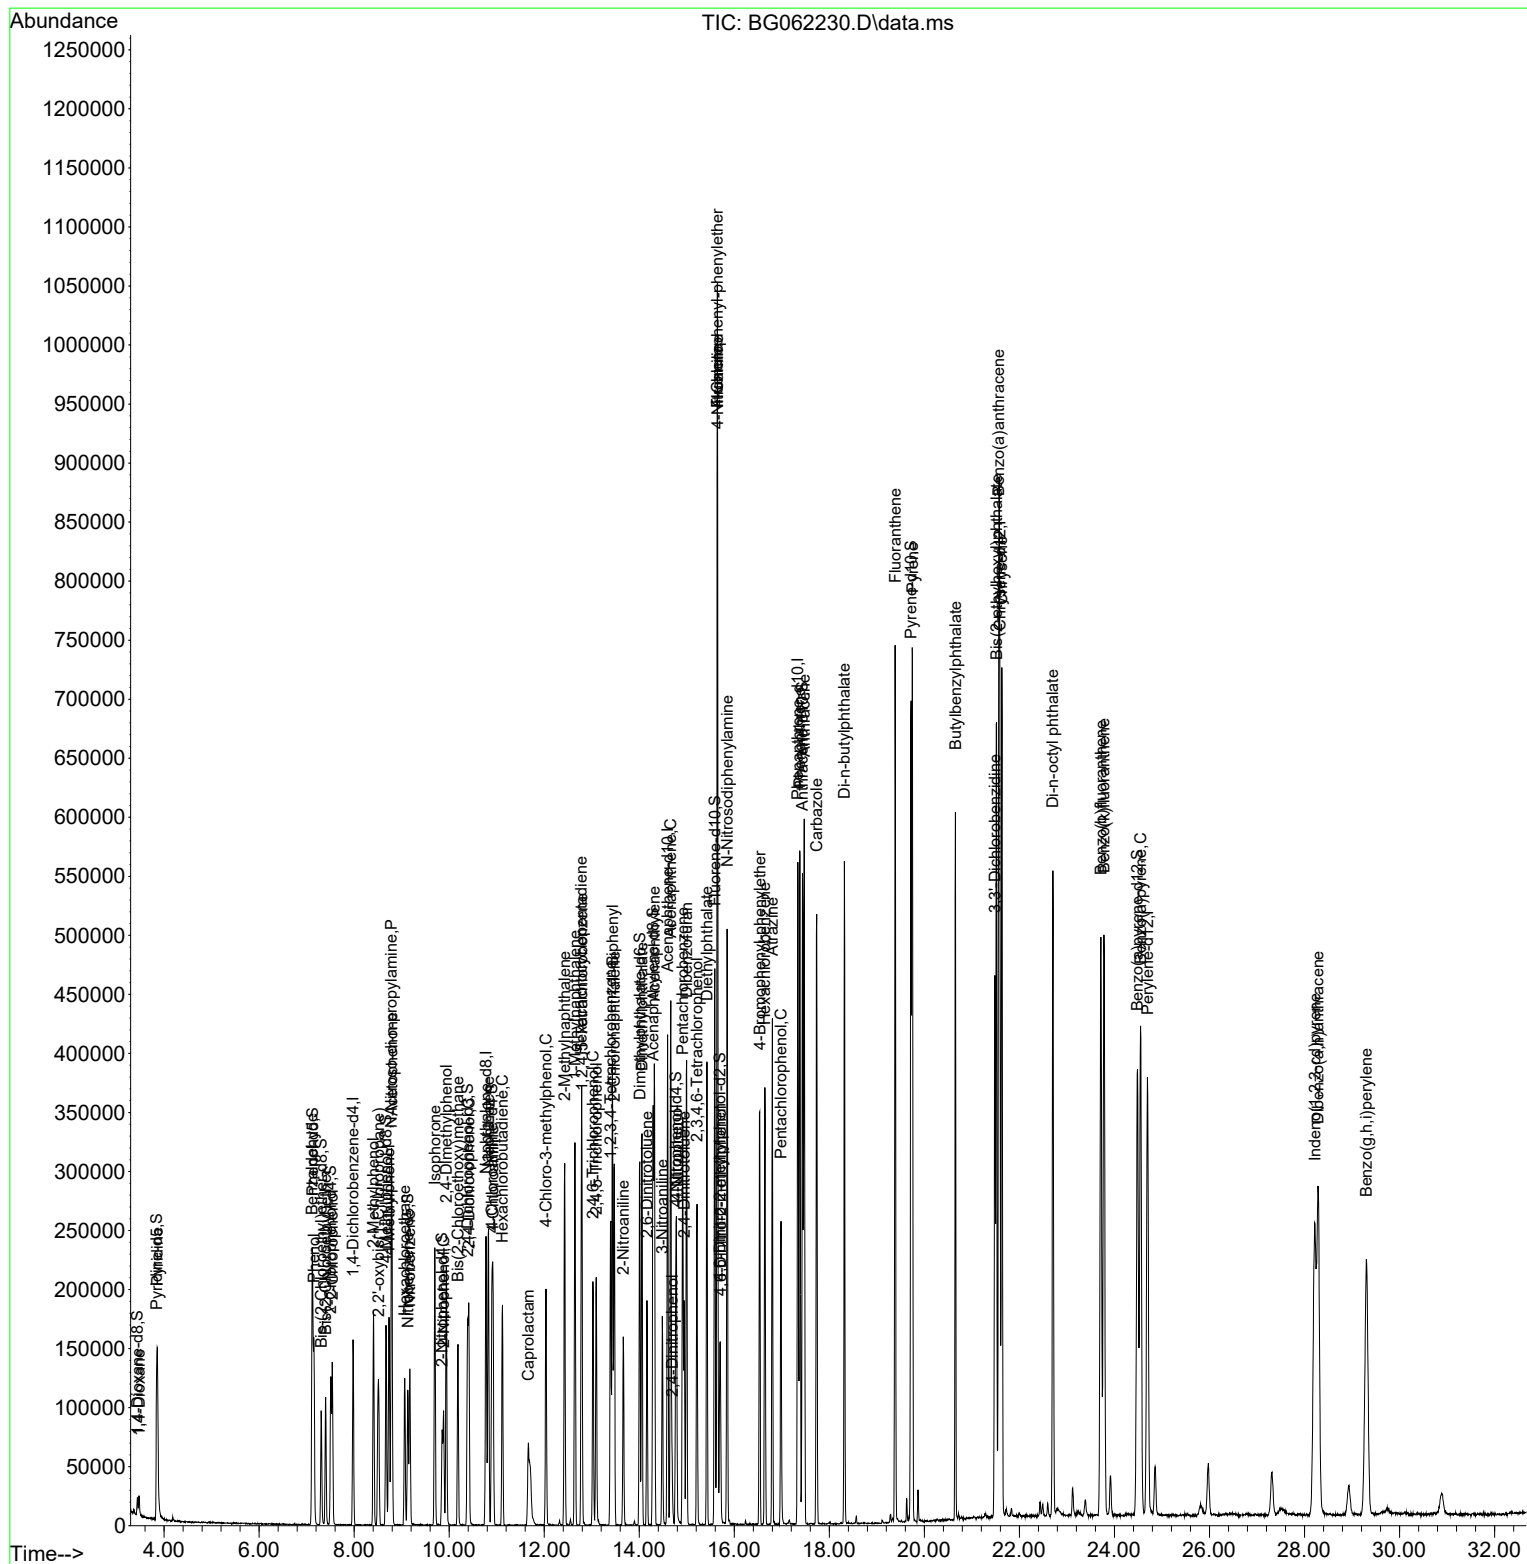




#2
1,4-Dioxane
Concen: 6.505 ng/uL
RT: 3.478 min Scan# 31
Delta R.T. 0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion: 88 Resp: 7899
Ion Ratio Lower Upper
88 100
43 35.3 26.4 39.6
58 72.8 69.7 104.5

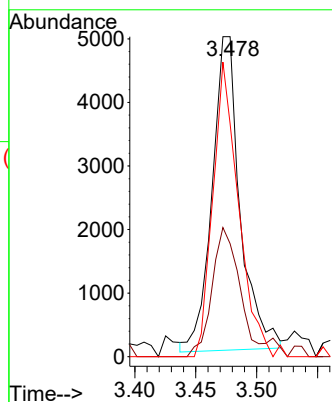

#5
Pyridine
Concen: 18.684 ng/uL
RT: 3.860 min Scan# 97
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion: 79 Resp: 59898
Ion Ratio Lower Upper
79 100
52 101.9 85.8 128.8
51 44.0 39.6 59.4









#6
Benzaldehyde
Concen: 23.243 ng/ul
RT: 7.114 min Scan# 611
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion: 77 Resp: 50306
Ion Ratio Lower Upper
77 100
105 93.1 75.0 112.6
106 88.2 68.2 102.4

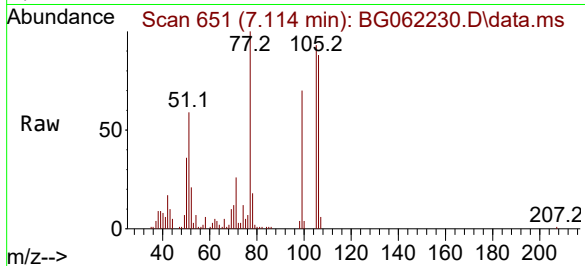

#8
Phenol
Concen: 18.602 ng/ul
RT: 7.155 min Scan# 658
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion: 94 Resp: 76937
Ion Ratio Lower Upper
94 100
65 32.0 24.5 36.7
66 39.5 30.8 46.2



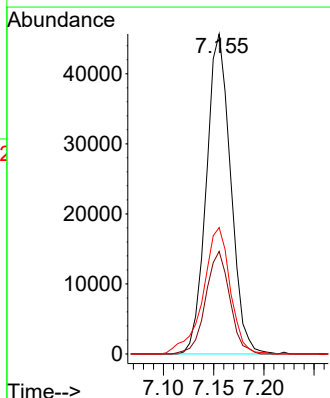
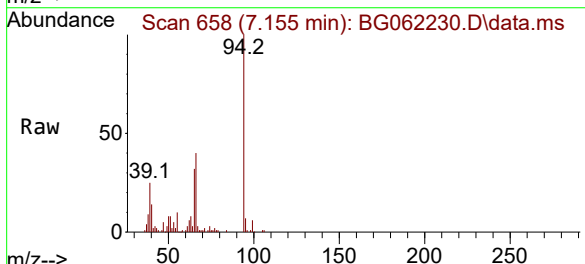




#10
Bis(2-Chloroethyl)ether
Concen: 19.171 ng/ul
RT: 7.402 min Scan# 700
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion: 93	Resp: 59826
Ion Ratio	Lower Upper
93 100	
63 84.9	68.0 102.0
95 33.9	26.4 39.6

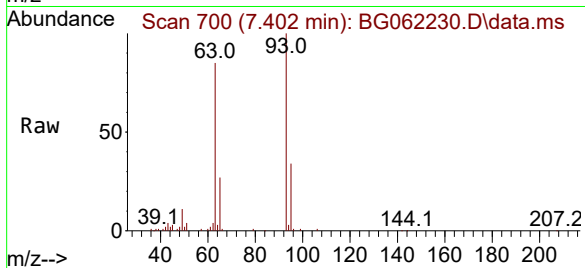

#12
2-Chlorophenol
Concen: 20.193 ng/ul
RT: 7.537 min Scan# 723
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:128	Resp: 56573
Ion Ratio	Lower Upper
128 100	
64 53.3	40.6 61.0
130 31.6	25.5 38.3

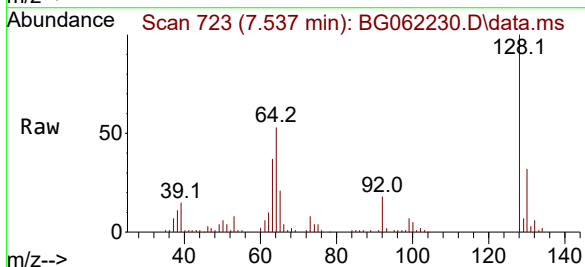



#13

2-Methylphenol

Concen: 18.993 ng/ul

RT: 8.407 min Scan# 81

Delta R.T. -0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :





SSTD020588

Tgt Ion:108 Resp: 60643

Ion Ratio Lower Upper

108 100

107 91.0 68.2 102.4

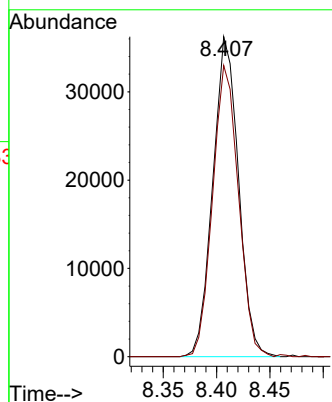

#14

2,2'-oxybis(1-Chloropropane)

Concen: 19.381 ng/ul

RT: 8.512 min Scan# 889

Delta R.T. 0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion: 45 Resp: 128697


Ion Ratio Lower Upper

45 100

77 9.7 7.8 11.6

79 8.0 5.1 7.7#









#16
Acetophenone
Concen: 19.291 ng/ul
RT: 8.794 min Scan# 91
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:105 Resp: 104555
Ion Ratio Lower Upper
105 100
77 80.0 64.8 97.2
51 34.8 28.6 42.8



#17
N-Nitroso-di-n-propylamine
Concen: 19.499 ng/ul
RT: 8.783 min Scan# 935
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion: 70 Resp: 58221
Ion Ratio Lower Upper
70 100
42 75.0 62.9 94.3
101 9.1 5.9 8.9#
130 17.2 14.2 21.2



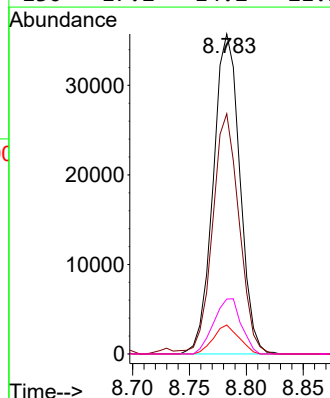





#18
4-Methylphenol
Concen: 18.996 ng/ul
RT: 8.736 min Scan# 91
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:108 Resp: 66808
Ion Ratio Lower Upper
108 100
107 113.5 88.3 132.5



#19
Hexachloroethane
Concen: 21.224 ng/ul
RT: 9.065 min Scan# 983
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:117 Resp: 23670
Ion Ratio Lower Upper
117 100
201 112.8 94.3 141.5
199 67.7 61.4 92.2









#22
Nitrobenzene
Concen: 28.818 ng/ul
RT: 9.170 min Scan# 1002
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion: 77 Resp: 69848
Ion Ratio Lower Upper
77 100
123 42.4 31.1 46.7
65 14.2 11.0 16.4



#23
Isophorone
Concen: 19.083 ng/ul
RT: 9.699 min Scan# 1091
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion: 82 Resp: 164363
Ion Ratio Lower Upper
82 100
95 7.5 5.4 8.0
138 14.2 13.1 19.7









#25
2-Nitrophenol
Concen: 33.158 ng/ul
RT: 9.881 min Scan# 1123
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:139 Resp: 29115
Ion Ratio Lower Upper
139 100
65 54.7 46.2 69.2
109 29.4 30.2 45.2#

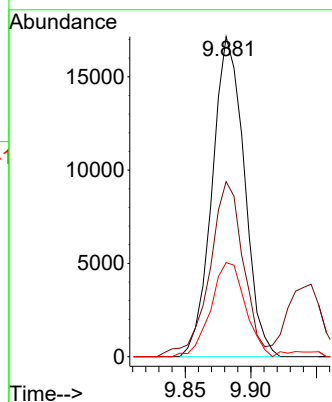

#26
2,4-Dimethylphenol
Concen: 19.589 ng/ul
RT: 9.940 min Scan# 1132
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:107 Resp: 74956
Ion Ratio Lower Upper
107 100
121 50.7 40.2 60.2
122 87.1 68.7 103.1


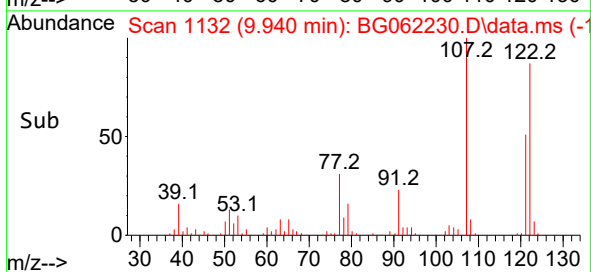
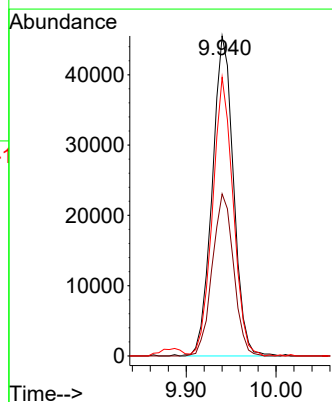





#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.879 ng/ul
 RT: 10.187 min Scan# 1174
 Delta R.T. -0.000 min
 Lab File: BG062230.D
 Acq: 31 Jul 2024 23:10




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020588


Tgt Ion: 93 Resp: 88002
 Ion Ratio Lower Upper
 93 100
 95 31.7 25.8 38.6
 123 11.4 9.0 13.4

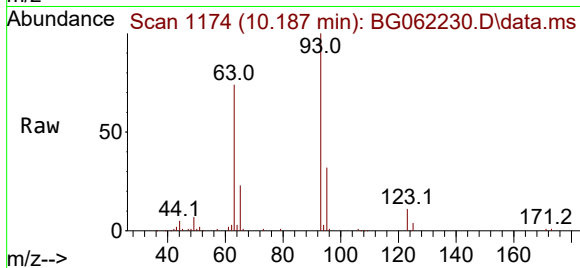

#29
 2,4-Dichlorophenol
 Concen: 21.946 ng/ul
 RT: 10.416 min Scan# 1213
 Delta R.T. -0.000 min
 Lab File: BG062230.D
 Acq: 31 Jul 2024 23:10

Tgt Ion:162 Resp: 62161
 Ion Ratio Lower Upper
 162 100
 164 66.0 52.2 78.4
 98 36.6 28.8 43.2




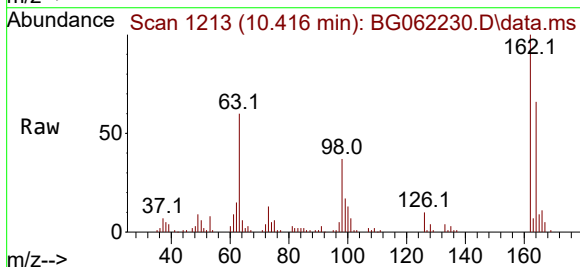




#30
Naphthalene
Concen: 19.626 ng/ul
RT: 10.827 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:128 Resp: 212764
Ion Ratio Lower Upper
128 100
129 11.1 9.1 13.7
127 13.9 11.0 16.4



#32
4-Chloroaniline
Concen: 19.685 ng/ul
RT: 10.927 min Scan# 1300
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:127 Resp: 90823
Ion Ratio Lower Upper
127 100
129 30.6 24.8 37.2









#33
Hexachlorobutadiene
Concen: 19.799 ng/ul
RT: 11.121 min Scan# 11
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:225 Resp: 44395
Ion Ratio Lower Upper
225 100
223 66.0 48.6 72.8
227 67.2 52.6 78.8



#34
Caprolactam
Concen: 9.368 ng/ul
RT: 11.667 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:113 Resp: 11304
Ion Ratio Lower Upper
113 100
55 259.0 177.0 265.4
56 154.2 117.6 176.4









#35
 4-Chloro-3-methylphenol
 Concen: 19.367 ng/ul
 RT: 12.037 min Scan# 1489
 Delta R.T. -0.000 min
 Lab File: BG062230.D
 Acq: 31 Jul 2024 23:10




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020588


Tgt Ion:	107	Resp:	71323
Ion	Ratio	Lower	Upper
107	100		
144	24.2	19.0	28.4
142	73.6	57.8	86.8



#36
 2-Methylnaphthalene
 Concen: 18.320 ng/ul
 RT: 12.431 min Scan# 1556
 Delta R.T. -0.000 min
 Lab File: BG062230.D
 Acq: 31 Jul 2024 23:10

Tgt Ion:	142	Resp:	140370
Ion	Ratio	Lower	Upper
142	100		
141	93.1	73.7	110.5





#37

1-Methylnaphthalene

Concen: 19.035 ng/ul

RT: 12.648 min Scan# 1

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:142 Resp: 150326

Ion Ratio Lower Upper

142 100

141 97.5 74.0 111.0

116 4.3 2.7 4.1#



#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.387 ng/ul

RT: 12.795 min Scan# 1618

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Tgt Ion:216 Resp: 84152




Ion Ratio Lower Upper


216 100

214 78.7 64.0 96.0

179 19.7 17.4 26.2

108 14.5 12.8 19.2



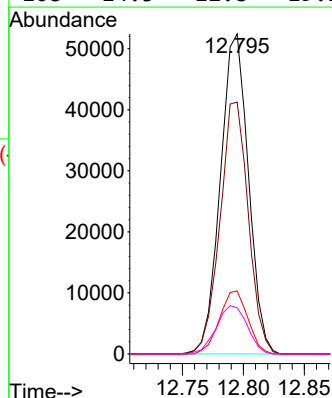





#40
Hexachlorocyclopentadiene
Concen: 20.812 ng/ul
RT: 12.783 min Scan# 1616
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:237 Resp: 46912
Ion Ratio Lower Upper
237 100
235 59.1 48.9 73.3
272 11.3 10.4 15.6



#41
2,4,6-Trichlorophenol
Concen: 23.320 ng/ul
RT: 13.024 min Scan# 1657
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:196 Resp: 50018
Ion Ratio Lower Upper
196 100
198 104.2 81.0 121.6
200 34.0 25.2 37.8





#42

2,4,5-Trichlorophenol

Concen: 24.568 ng/ul

RT: 13.095 min Scan# 1

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:196 Resp: 59590

Ion Ratio Lower Upper

196 100

198 102.7 81.7 122.5

200 32.6 25.8 38.6



#43

1,1'-Biphenyl

Concen: 19.028 ng/ul

RT: 13.435 min Scan# 1727

Delta R.T. -0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion:154 Resp: 201318


Ion Ratio Lower Upper

154 100

153 40.6 31.3 46.9

76 13.4 10.6 15.8







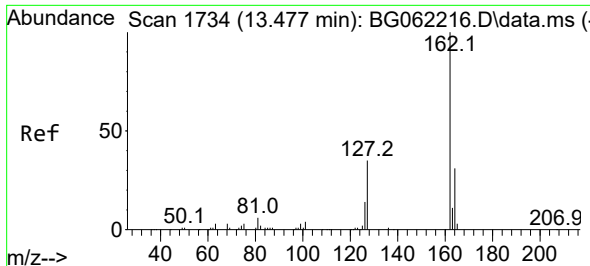

#44
2-Chloronaphthalene
Concen: 19.111 ng/ul
RT: 13.476 min Scan# 11
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:162 Resp: 158579
Ion Ratio Lower Upper
162 100
164 33.8 25.2 37.8
127 37.8 30.9 46.3

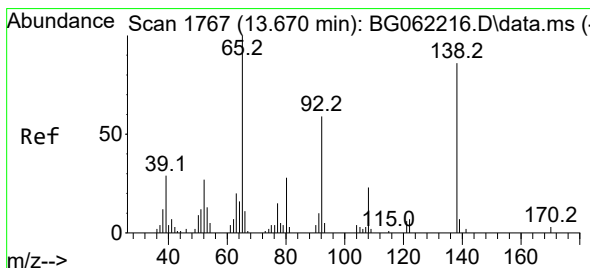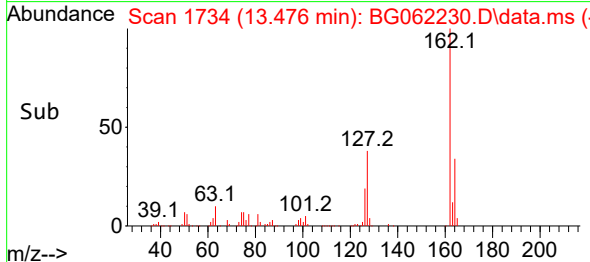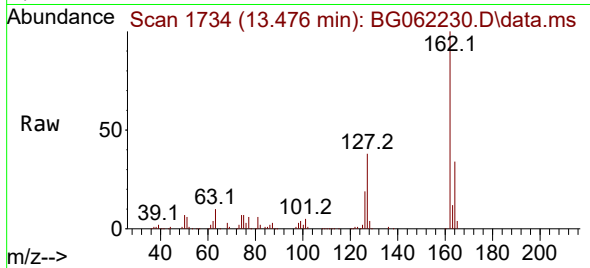

#45
2-Nitroaniline
Concen: 30.045 ng/ul
RT: 13.664 min Scan# 1766
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion: 65 Resp: 44078
Ion Ratio Lower Upper
65 100
92 62.5 47.2 70.8
138 85.7 68.6 103.0

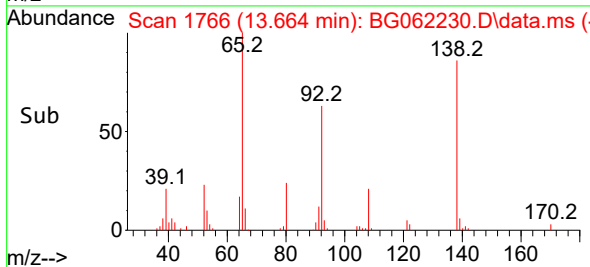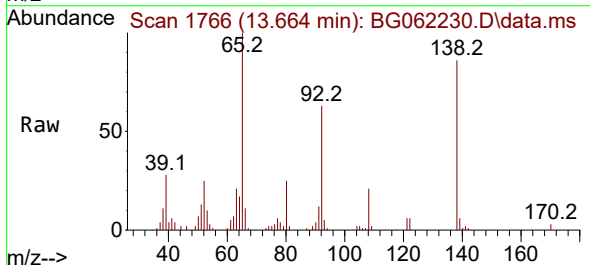



#47

Dimethylphthalate

Concen: 19.415 ng/ul

RT: 14.058 min Scan# 1833

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:163 Resp: 222681

Ion Ratio Lower Upper

163 100

194 3.6 3.0 4.6

164 10.0 7.6 11.4

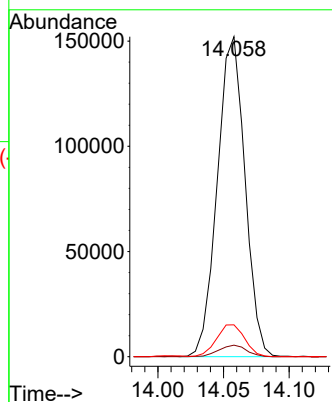

#48

2,6-Dinitrotoluene

Concen: 30.934 ng/ul

RT: 14.164 min Scan# 1851

Delta R.T. -0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion:165 Resp: 33424


Ion Ratio Lower Upper

165 100

89 58.2 55.0 82.4

121 21.5 19.4 29.2


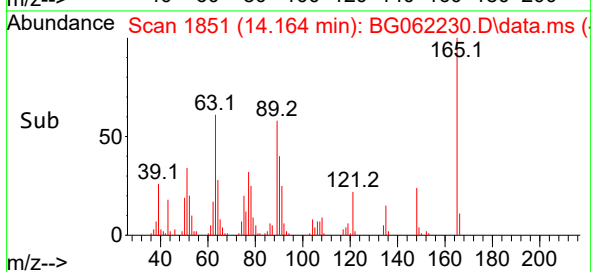
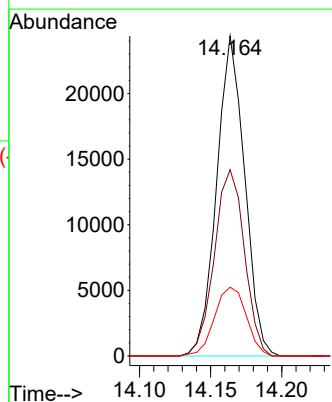





#50
Acenaphthylene
Concen: 19.571 ng/ul
RT: 14.316 min Scan# 1877
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:152 Resp: 269420
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.4
153 14.5 11.0 16.4



#51
3-Nitroaniline
Concen: 26.457 ng/ul
RT: 14.487 min Scan# 1906
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:138 Resp: 35634
Ion Ratio Lower Upper
138 100
108 19.4 26.0 39.0#
92 147.2 103.4 155.2









#52
Acenaphthene
Concen: 19.531 ng/ul
RT: 14.663 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:153 Resp: 190026
Ion Ratio Lower Upper
153 100
152 44.2 35.0 52.4
154 85.0 66.9 100.3



#53
2,4-Dinitrophenol
Concen: 21.935 ng/ul
RT: 14.692 min Scan# 1941
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:184 Resp: 12417
Ion Ratio Lower Upper
184 100
63 64.8 55.3 82.9
154 77.1 72.9 109.3









#55
4-Nitrophenol
Concen: 24.189 ng/ul
RT: 14.786 min Scan# 1957
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:109 Resp: 31033
Ion Ratio Lower Upper
109 100
139 118.6 91.2 136.8
65 134.2 97.0 145.4

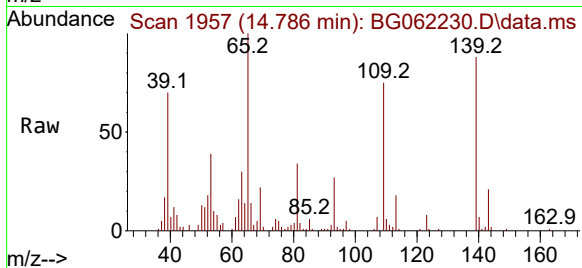

#56
Dibenzofuran
Concen: 19.805 ng/ul
RT: 14.998 min Scan# 1993
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:168 Resp: 267006
Ion Ratio Lower Upper
168 100
139 36.5 29.8 44.8




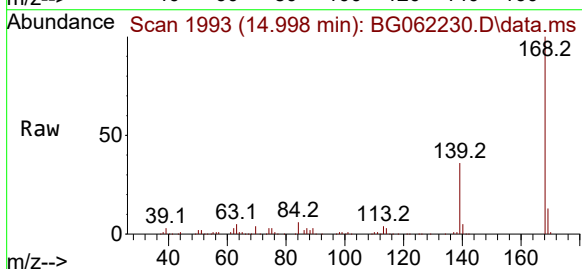




#57
2,4-Dinitrotoluene
Concen: 32.182 ng/ul
RT: 14.945 min Scan# 1984
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:165 Resp: 47504
Ion Ratio Lower Upper
165 100
63 51.1 43.4 65.0
182 2.2 2.2 3.4#



#58
2,3,4,6-Tetrachlorophenol
Concen: 24.742 ng/ul
RT: 15.215 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:232 Resp: 57118
Ion Ratio Lower Upper
232 100
131 40.0 29.9 44.9
130 2.0 1.8 2.6
166 28.2 22.8 34.2







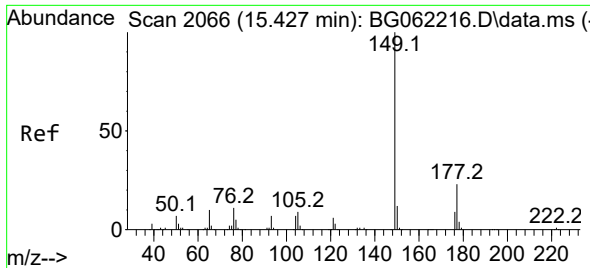

#59
Diethylphthalate
Concen: 19.509 ng/ul
RT: 15.427 min Scan# 2066
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:149 Resp: 229408
Ion Ratio Lower Upper
149 100
177 22.6 18.2 27.4
150 12.1 9.7 14.5

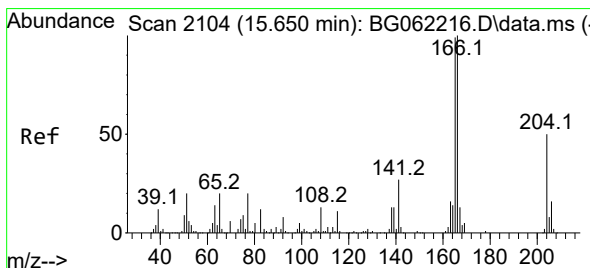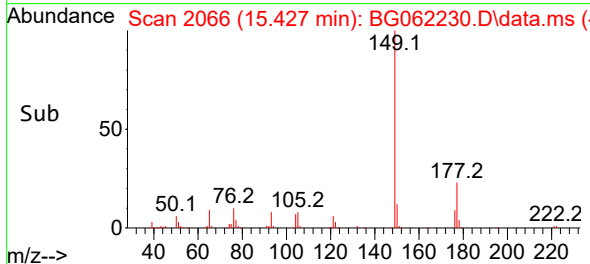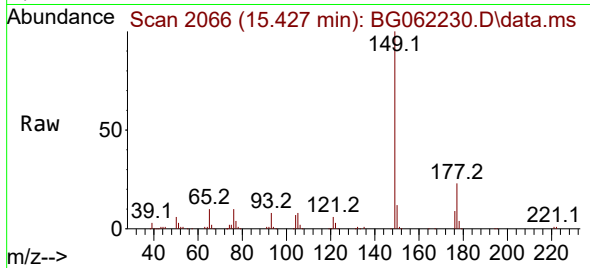

#61
Fluorene
Concen: 19.740 ng/ul
RT: 15.644 min Scan# 2103
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:166 Resp: 214266
Ion Ratio Lower Upper
166 100
165 100.5 79.4 119.2
167 12.6 10.1 15.1


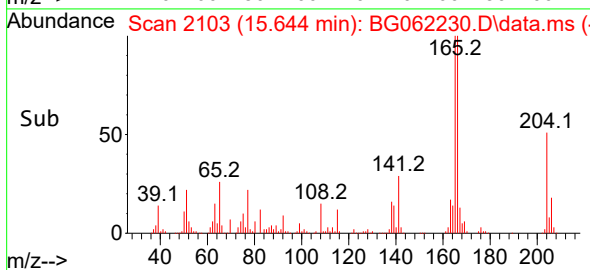

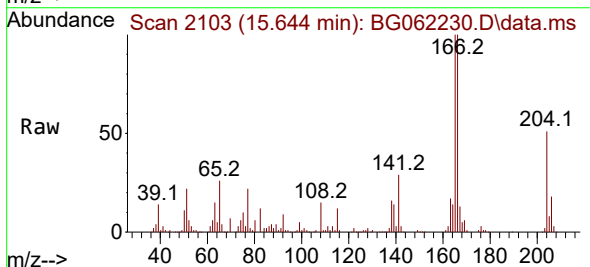




#62
4-Chlorophenyl-phenylether
Concen: 19.897 ng/ul
RT: 15.644 min Scan# 2103
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:204 Resp: 109313
Ion Ratio Lower Upper
204 100
206 35.9 26.2 39.2
141 57.6 46.4 69.6

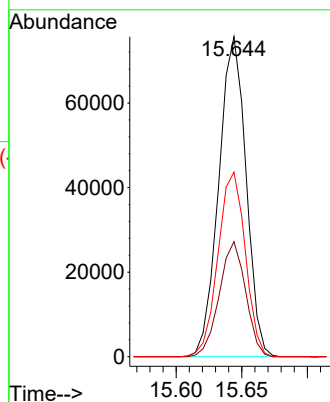

#63
4-Nitroaniline
Concen: 26.528 ng/ul
RT: 15.650 min Scan# 2104
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:138 Resp: 39721
Ion Ratio Lower Upper
138 100
92 63.4 48.6 73.0
108 98.5 78.6 118.0




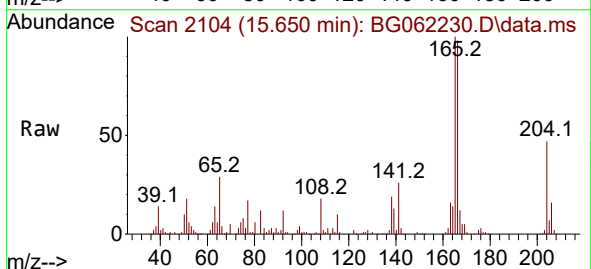




#66
4,6-Dinitro-2-methylphenol
Concen: 25.456 ng/ul
RT: 15.709 min Scan# 2114
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:198 Resp: 23700
Ion Ratio Lower Upper
198 100
182 5.5 3.1 4.7#
77 22.5 19.0 28.6



#67
N-Nitrosodiphenylamine
Concen: 19.535 ng/ul
RT: 15.850 min Scan# 2138
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:169 Resp: 190639
Ion Ratio Lower Upper
169 100
168 70.6 57.4 86.0
167 37.6 28.5 42.7









#68
4-Bromophenyl-phenylether
Concen: 19.330 ng/ul
RT: 16.537 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:248 Resp: 72604
Ion Ratio Lower Upper
248 100
250 98.4 80.0 120.0
141 67.9 56.3 84.5



#69
Hexachlorobenzene
Concen: 20.003 ng/ul
RT: 16.643 min Scan# 2273
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:284 Resp: 81222
Ion Ratio Lower Upper
284 100
142 32.4 25.4 38.2
249 33.4 26.9 40.3





#70

Atrazine

Concen: 20.725 ng/ul

RT: 16.801 min Scan# 21

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:200 Resp: 77835

Ion Ratio Lower Upper

200 100

173 24.1 20.6 30.8

215 48.2 37.8 56.6

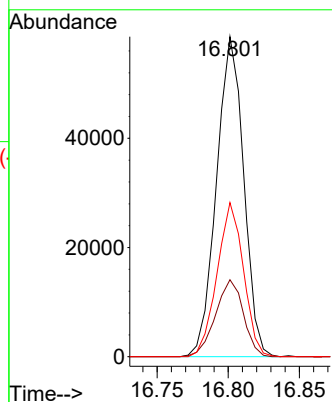

#71

Pentachlorophenol

Concen: 18.168 ng/ul

RT: 16.983 min Scan# 2331

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion:266 Resp: 46889


Ion Ratio Lower Upper

266 100

264 66.2 52.7 79.1

268 63.7 47.1 70.7









#72
Phenanthrene
Concen: 19.924 ng/ul
RT: 17.377 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:178 Resp: 376986
Ion Ratio Lower Upper
178 100
179 14.9 12.2 18.2
176 19.0 15.3 22.9

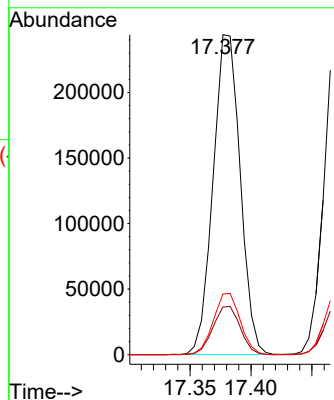

#74
Anthracene
Concen: 19.689 ng/ul
RT: 17.471 min Scan# 2414
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:178 Resp: 385642
Ion Ratio Lower Upper
178 100
179 15.9 12.6 18.8
176 18.6 14.9 22.3



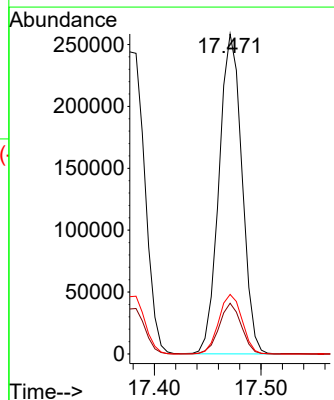





#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.627 ng/ul
RT: 13.400 min Scan# 1721
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:216 Resp: 84901
Ion Ratio Lower Upper
216 100
214 79.9 62.8 94.2
218 48.6 36.7 55.1

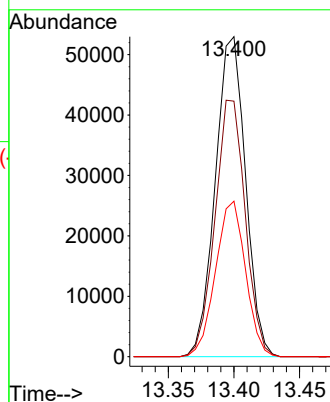

#76
Pentachlorobenzene
Concen: 20.271 ng/ul
RT: 14.916 min Scan# 1979
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:250 Resp: 92730
Ion Ratio Lower Upper
250 100
248 61.4 49.8 74.8
252 62.5 49.7 74.5







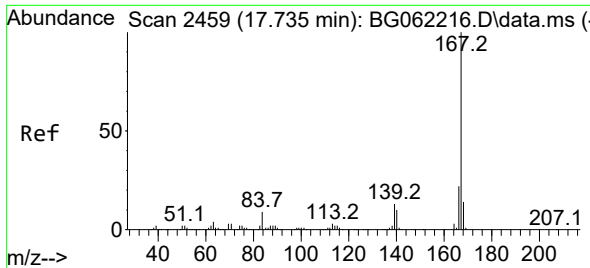

#77
Carbazole
Concen: 20.701 ng/ul
RT: 17.735 min Scan# 2459
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:167 Resp: 332757
Ion Ratio Lower Upper
167 100
166 22.0 17.7 26.5
139 12.6 10.4 15.6

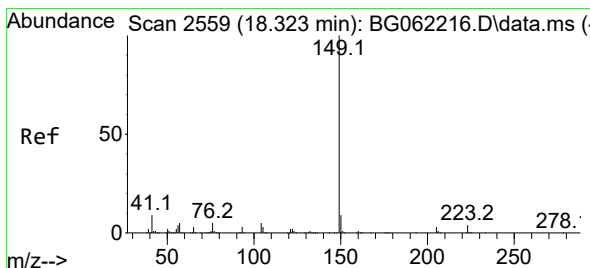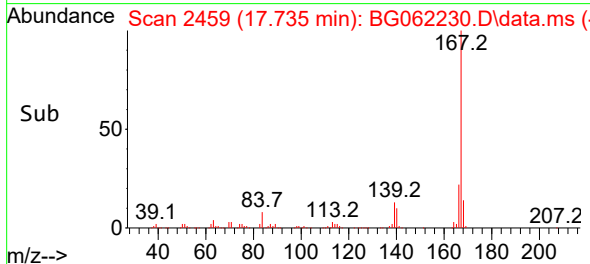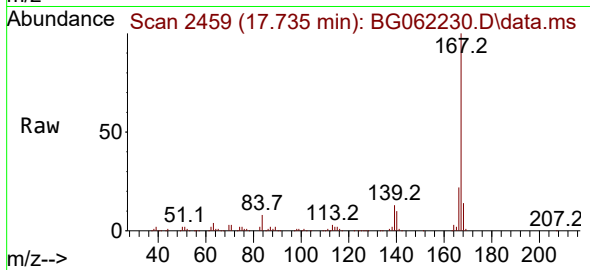

#78
Di-n-butylphthalate
Concen: 19.950 ng/ul
RT: 18.317 min Scan# 2558
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:149 Resp: 397691
Ion Ratio Lower Upper
149 100
150 9.2 7.1 10.7
104 4.9 4.2 6.2


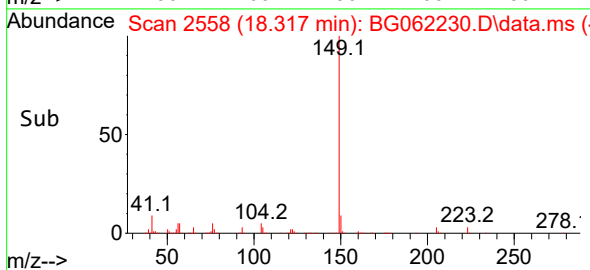

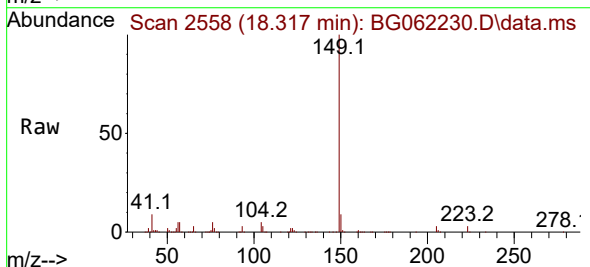




#80
Fluoranthene
Concen: 19.840 ng/ul
RT: 19.386 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:202 Resp: 453986
Ion Ratio Lower Upper
202 100
101 10.3 8.2 12.4
100 8.4 6.9 10.3



#82
Pyrene
Concen: 19.996 ng/ul
RT: 19.750 min Scan# 2802
Delta R.T. -0.000 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:202 Resp: 476968
Ion Ratio Lower Upper
202 100
101 11.2 9.0 13.6
100 9.4 8.0 12.0





#83

Butylbenzylphthalate

Concen: 21.497 ng/ul

RT: 20.655 min Scan# 2956

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:149 Resp: 172067

Ion Ratio Lower Upper

149 100

91 69.9 60.0 90.0

206 23.4 17.2 25.8

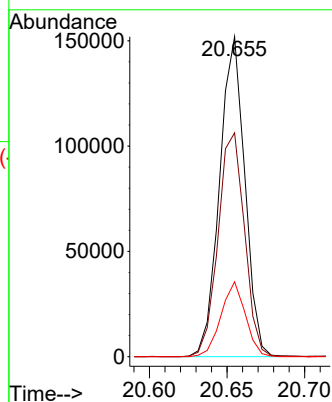

#84

3,3'-Dichlorobenzidine

Concen: 21.536 ng/ul

RT: 21.483 min Scan# 3097

Delta R.T. -0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion:252 Resp: 163467


Ion Ratio Lower Upper

252 100

254 64.3 49.7 74.5

126 9.4 6.9 10.3




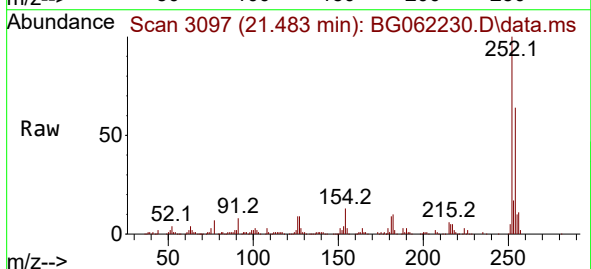




#85
Benzo(a)anthracene
Concen: 19.746 ng/ul
RT: 21.565 min Scan# 3111
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:228 Resp: 489831
Ion Ratio Lower Upper
228 100
229 19.1 15.9 23.9
226 27.6 21.8 32.6

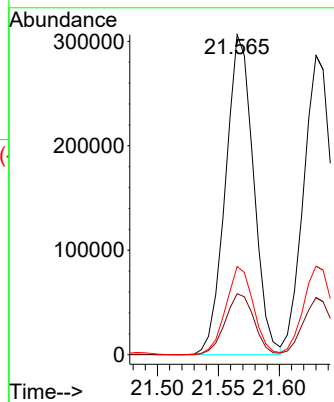

#86
Bis(2-ethylhexyl)phthalate
Concen: 20.931 ng/ul
RT: 21.518 min Scan# 3103
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:149 Resp: 261891
Ion Ratio Lower Upper
149 100
167 26.5 21.4 32.0
279 3.8 2.8 4.2

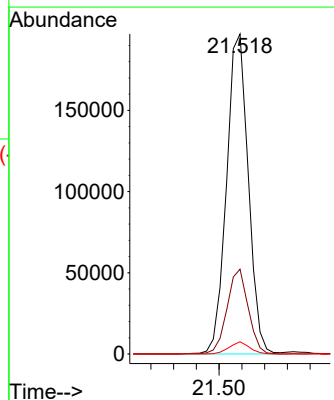



#87

Chrysene

Concen: 19.902 ng/ul

RT: 21.630 min Scan# 31

Delta R.T. -0.006 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:228 Resp: 461412

Ion Ratio Lower Upper

228 100

226 29.6 24.2 36.4

229 19.1 15.5 23.3

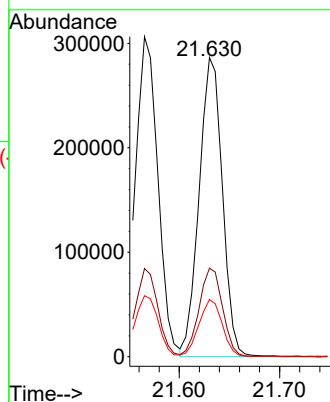

#89

Di-n-octyl phthalate

Concen: 21.142 ng/ul




RT: 22.705 min Scan# 3305


Delta R.T. -0.012 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Tgt Ion:149 Resp: 456646









#90
Benzo(b)fluoranthene
Concen: 19.539 ng/ul
RT: 23.715 min Scan# 3477
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10




Instrument :
BNA_G
ClientSampleId :
SSTD020588


Tgt Ion:252 Resp: 467645
Ion Ratio Lower Upper
252 100
253 22.0 17.0 25.6
125 8.7 6.7 10.1



#91
Benzo(k)fluoranthene
Concen: 20.327 ng/ul
RT: 23.780 min Scan# 3488
Delta R.T. -0.006 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:252 Resp: 483643
Ion Ratio Lower Upper
252 100
253 21.4 17.5 26.3
125 8.0 7.3 10.9





#93

Benzo(a)pyrene

Concen: 19.843 ng/ul

RT: 24.550 min Scan# 3

Delta R.T. -0.012 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10

Instrument :

BNA_G

ClientSampleId :

SSTD020588





Tgt Ion:252 Resp: 449141

Ion Ratio Lower Upper

252 100

253 21.5 17.4 26.0

125 9.5 7.5 11.3

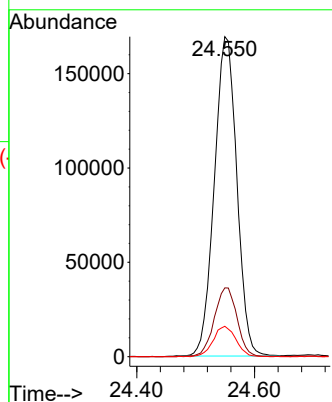

#94

Indeno(1,2,3-cd)pyrene

Concen: 19.621 ng/ul

RT: 28.221 min Scan# 4244

Delta R.T. -0.000 min

Lab File: BG062230.D

Acq: 31 Jul 2024 23:10




Tgt Ion:276 Resp: 522193


Ion Ratio Lower Upper

276 100

138 16.7 13.5 20.3

277 23.5 19.8 29.6









#95
Dibenzo(a,h)anthracene
Concen: 19.834 ng/ul
RT: 28.286 min Scan# 41
Delta R.T. -0.012 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Instrument :
BNA_G
ClientSampleId :
SSTD020588

Tgt Ion:278 Resp: 442591
Ion Ratio Lower Upper
278 100
139 12.6 10.2 15.2
279 23.2 18.8 28.2

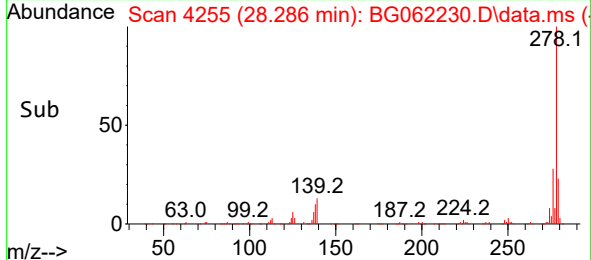

#96
Benzo(g,h,i)perylene
Concen: 19.654 ng/ul
RT: 29.302 min Scan# 4428
Delta R.T. -0.018 min
Lab File: BG062230.D
Acq: 31 Jul 2024 23:10

Tgt Ion:276 Resp: 419868
Ion Ratio Lower Upper
276 100
138 17.6 15.4 23.2
277 25.7 19.4 29.0

