

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
 Data File : BG062221.D
 Acq On : 31 Jul 2024 17:01
 Operator : MA/JU
 Sample : PB162104BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.435	22	25	31	rVB2	10271	15004	1.05%	0.111%
2	3.611	53	55	58	rBV4	1534	1551	0.11%	0.011%
3	3.840	90	94	108	rBV	140874	231938	16.16%	1.713%
4	4.187	150	153	158	rVB3	2676	4573	0.32%	0.034%
5	6.795	593	597	600	rBV3	1146	1645	0.11%	0.012%
6	7.130	647	654	665	rVB	161459	276896	19.29%	2.045%
7	7.306	678	684	693	rBV	119083	200536	13.97%	1.481%
8	7.506	711	718	730	rVB	144663	246242	17.16%	1.818%
9	7.982	792	799	808	rVB	140913	240229	16.74%	1.774%
10	8.669	909	916	931	rVB	202894	346779	24.16%	2.561%
11	9.127	987	994	1005	rBV	129597	231526	16.13%	1.710%
12	9.198	1005	1006	1013	rVB3	1222	1821	0.13%	0.013%
13	9.850	1111	1117	1125	rBV	86226	150660	10.50%	1.113%
14	10.384	1201	1208	1218	rBV	182822	327260	22.80%	2.417%
15	10.778	1267	1275	1284	rVB	217098	386686	26.94%	2.855%
16	10.901	1288	1296	1305	rBV	230354	402577	28.05%	2.973%
17	12.352	1540	1543	1549	rVB3	2728	4428	0.31%	0.033%
18	14.009	1819	1825	1833	rVB	459729	654627	45.61%	4.834%
19	14.291	1866	1873	1880	rBV	461281	727013	50.65%	5.368%
20	14.602	1919	1926	1934	rVB	408129	633258	44.12%	4.676%
21	14.766	1948	1954	1966	rBV	191797	306924	21.38%	2.266%
22	15.589	2088	2094	2102	rVB	647773	944882	65.83%	6.977%
23	15.695	2105	2112	2123	rBV	78044	117384	8.18%	0.867%
24	15.830	2132	2135	2139	rVB2	1881	1982	0.14%	0.015%
25	16.376	2224	2228	2231	rBV2	1920	2340	0.16%	0.017%
26	17.339	2384	2392	2400	rBV	588349	858163	59.79%	6.337%
27	17.439	2402	2409	2418	rVB2	754451	1127465	78.55%	8.326%
28	19.284	2719	2723	2728	rBV2	9721	13838	0.96%	0.102%
29	19.354	2731	2735	2742	rBV2	9476	15829	1.10%	0.117%
30	19.719	2791	2797	2807	rVB	964455	1401123	97.62%	10.346%
31	20.711	2964	2966	2970	rBV4	2924	3889	0.27%	0.029%
32	20.776	2975	2977	2979	rBV2	1857	2289	0.16%	0.017%
33	20.987	3011	3013	3016	rBV3	1958	2746	0.19%	0.020%
34	21.587	3108	3115	3126	rVB2	617694	987529	68.80%	7.292%
35	21.833	3155	3157	3162	rVB6	2653	3290	0.23%	0.024%
36	22.444	3257	3261	3268	rVB5	5871	8561	0.60%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
Data File : BG062221.D
Acq On : 31 Jul 2024 17:01
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
Title : SVOA CALIBRATION

37	23.079	3367	3369	3372	rBV3	1808	1999	0.14%	0.015%
38	23.132	3372	3378	3384	rVB4	9092	19868	1.38%	0.147%
39	23.343	3413	3414	3416	rBV2	2226	1622	0.11%	0.012%
40	23.925	3506	3513	3523	rBV3	14410	31537	2.20%	0.233%
41	24.489	3598	3609	3622	rBV3	539885	1435283	100.00%	10.599%
42	24.700	3634	3645	3657	rVB	387518	1043614	72.71%	7.706%
43	24.865	3665	3673	3680	rVB3	15886	39916	2.78%	0.295%
44	25.987	3857	3864	3872	rVB6	16482	42097	2.93%	0.311%
45	26.650	3975	3977	3980	rVB4	2167	1947	0.14%	0.014%
46	27.320	4084	4091	4092	rBV3	13112	21414	1.49%	0.158%
47	28.395	4272	4274	4277	rBV3	2087	2611	0.18%	0.019%
48	28.953	4365	4369	4371	rBV4	4000	5307	0.37%	0.039%
49	29.417	4445	4448	4451	rBV5	2311	2907	0.20%	0.021%
50	29.447	4451	4453	4454	rBV	2024	1518	0.11%	0.011%
51	30.892	4696	4699	4700	rBV2	3524	3723	0.26%	0.027%
52	31.514	4803	4805	4808	rBV4	1730	1781	0.12%	0.013%
53	32.172	4915	4917	4919	rBV3	2030	1639	0.11%	0.012%




Sum of corrected areas: 13542266

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
Data File : BG062221.D
Acq On : 31 Jul 2024 17:01
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

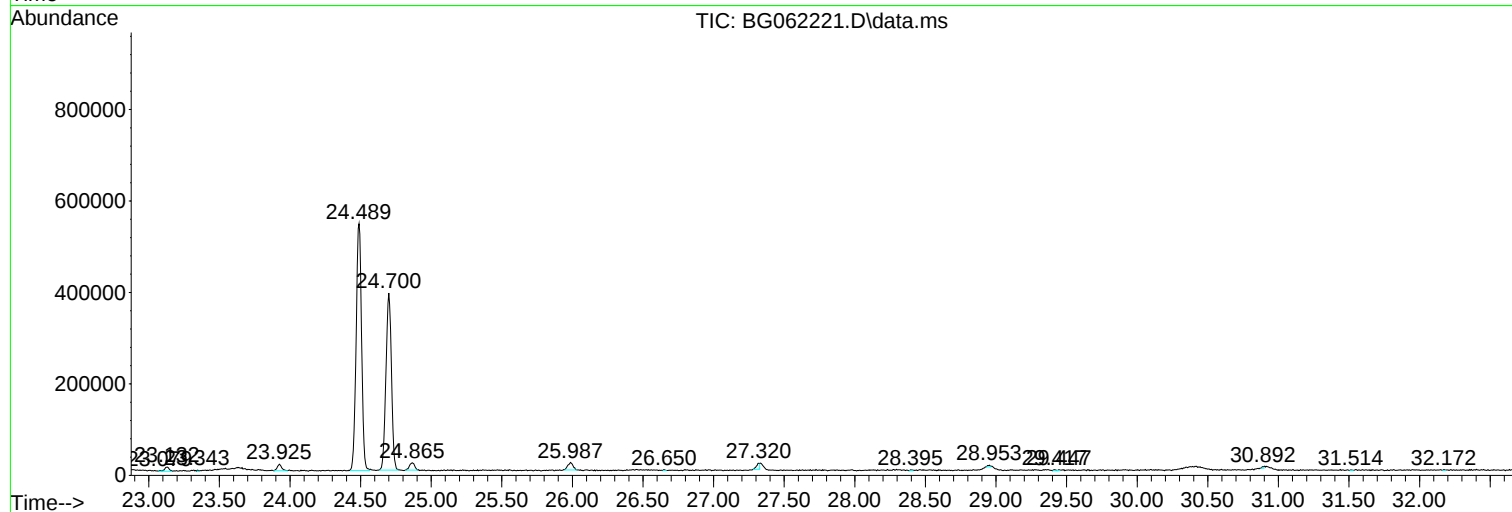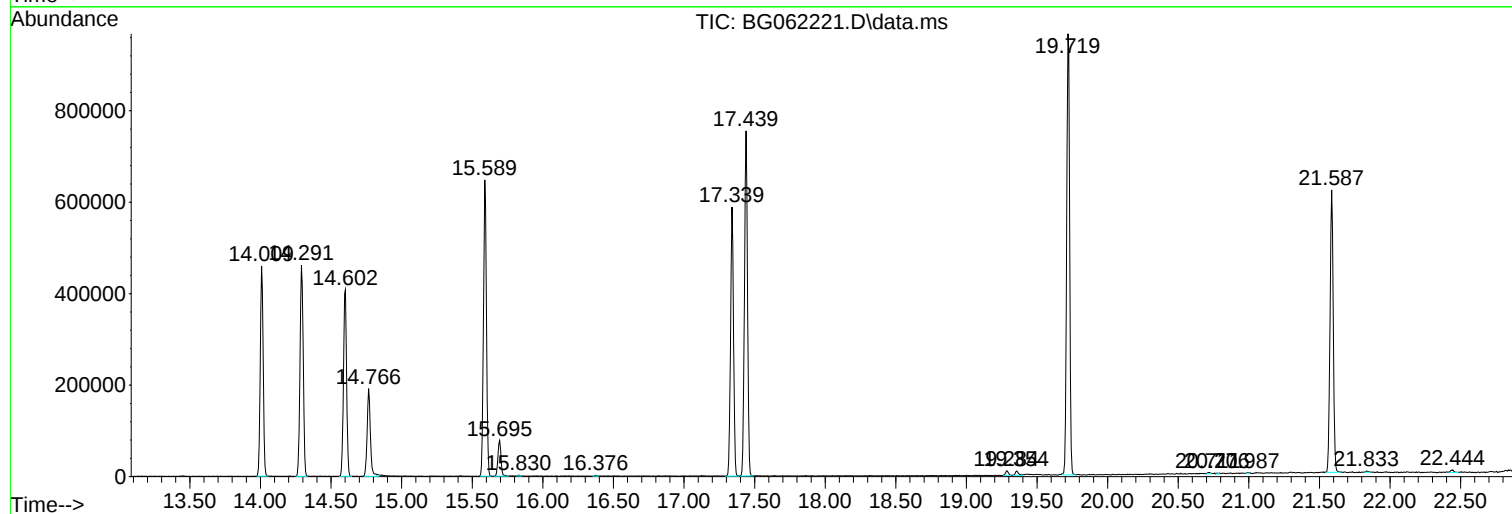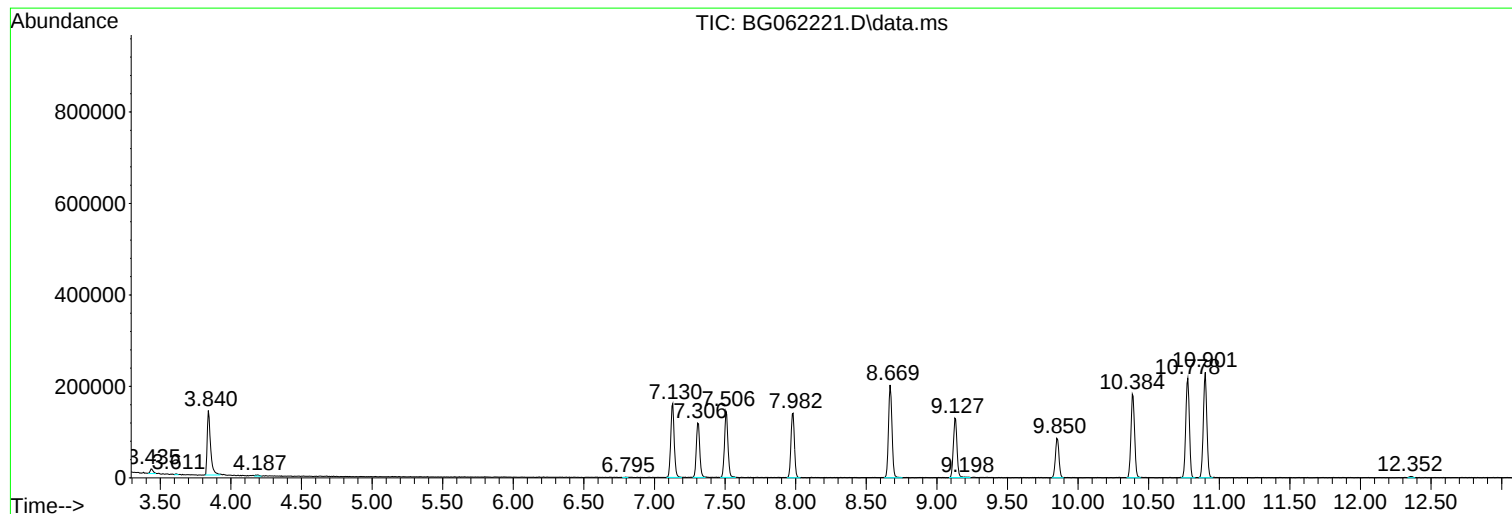

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
Data File : BG062221.D
Acq On : 31 Jul 2024 17:01
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073124\
Data File : BG062221.D
Acq On : 31 Jul 2024 17:01
Operator : MA/JU
Sample : PB162104BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG073124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc