




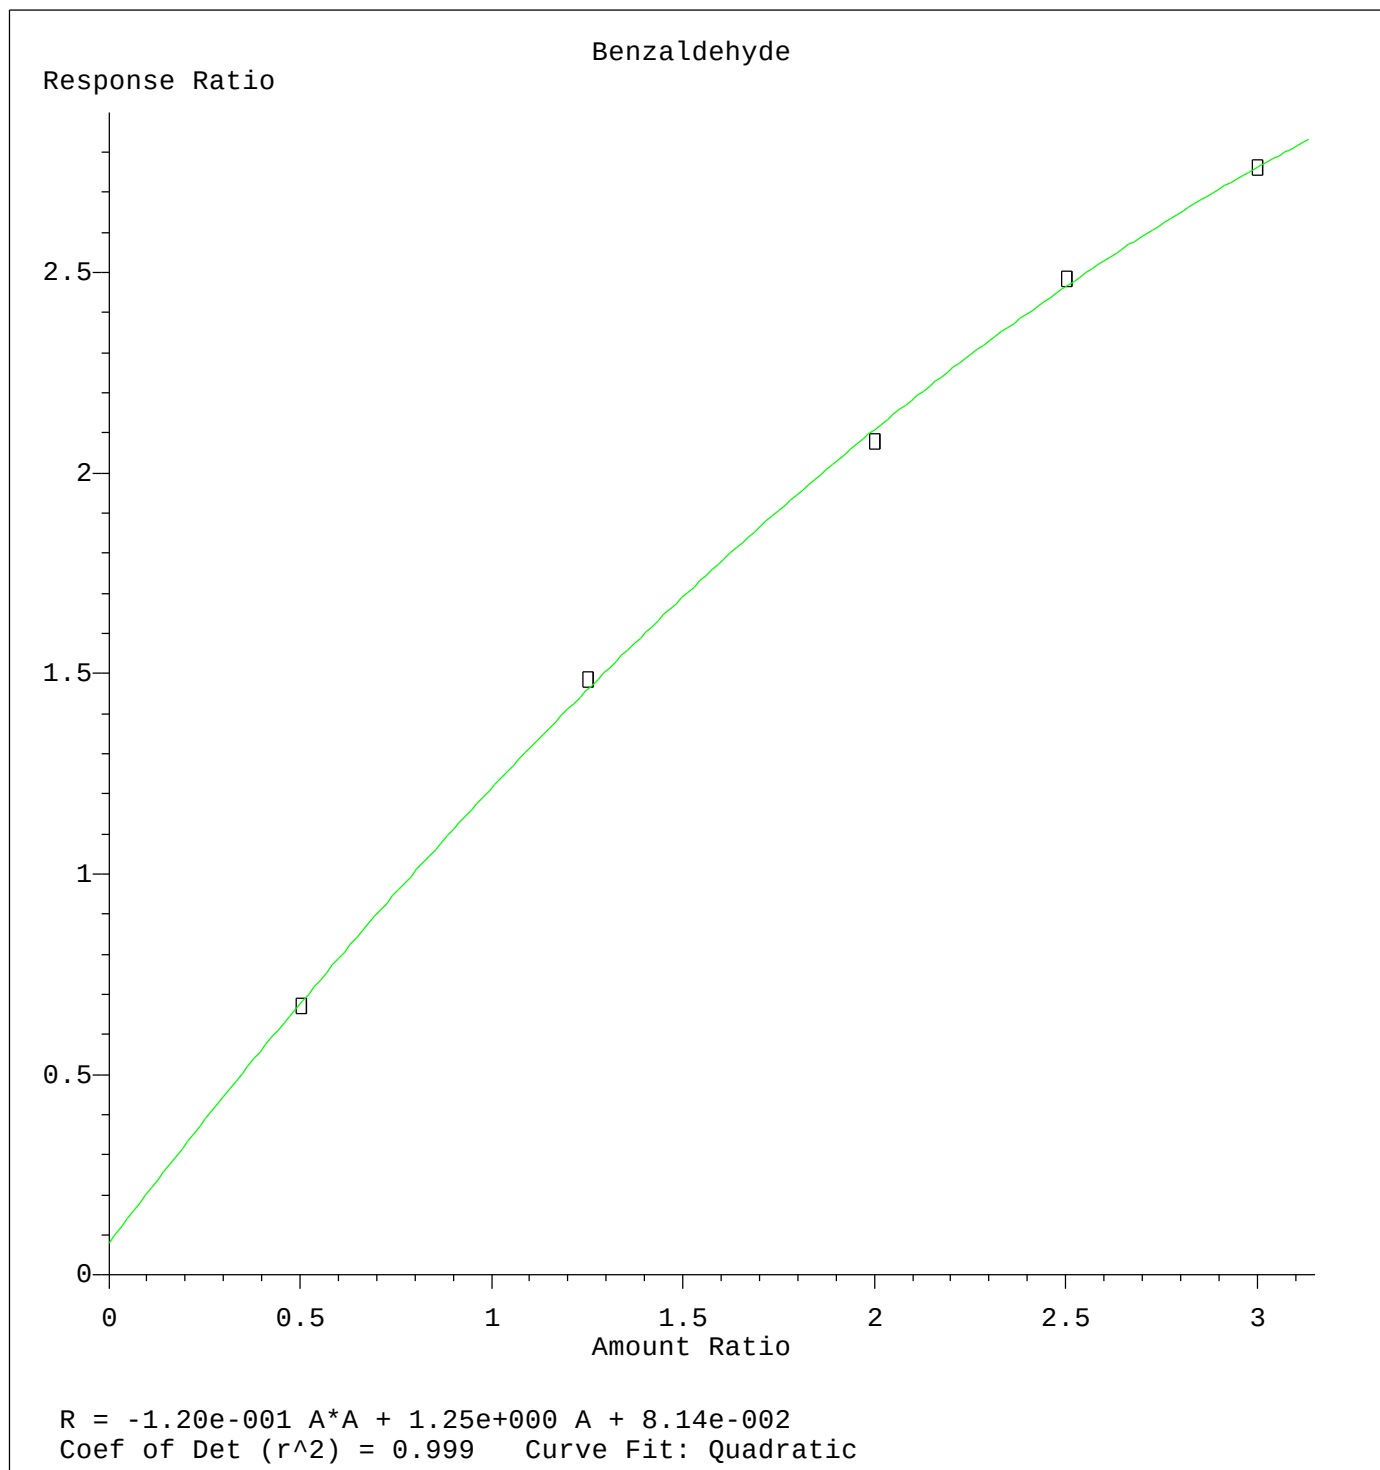


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016

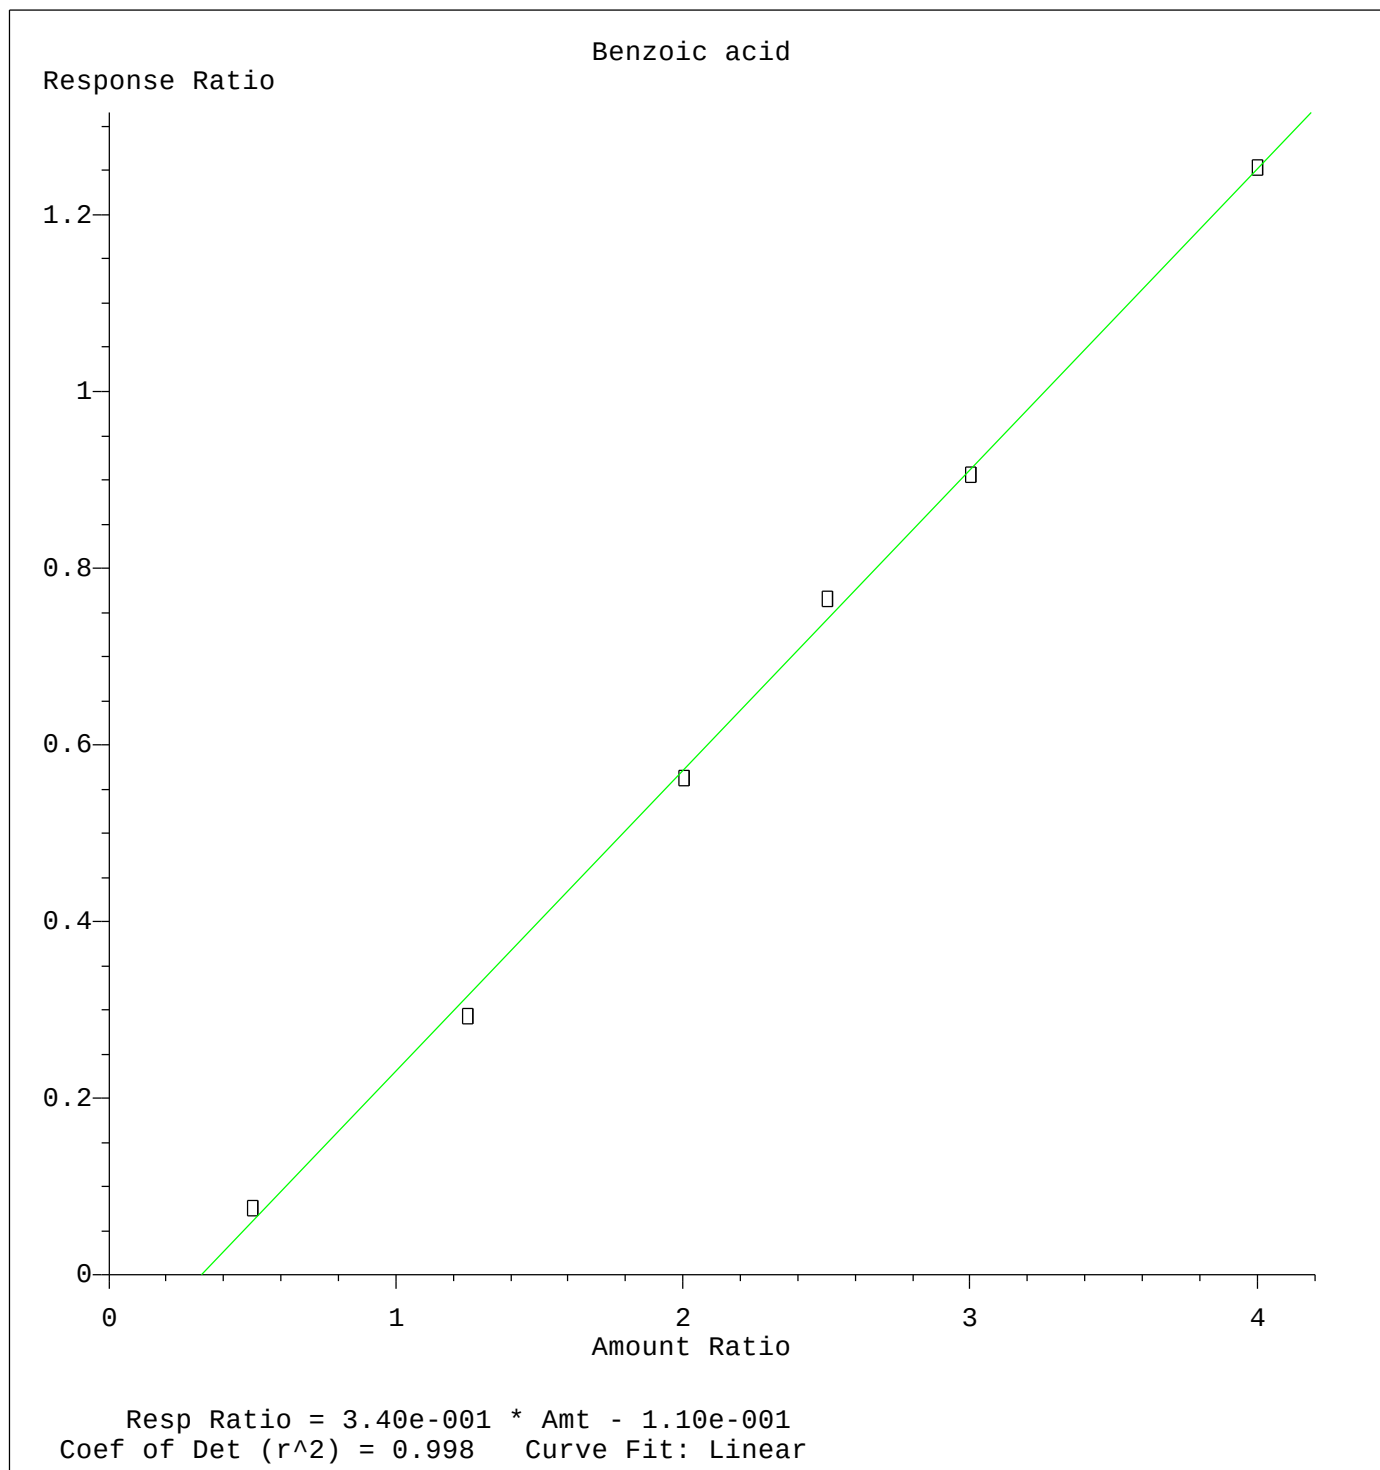


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016

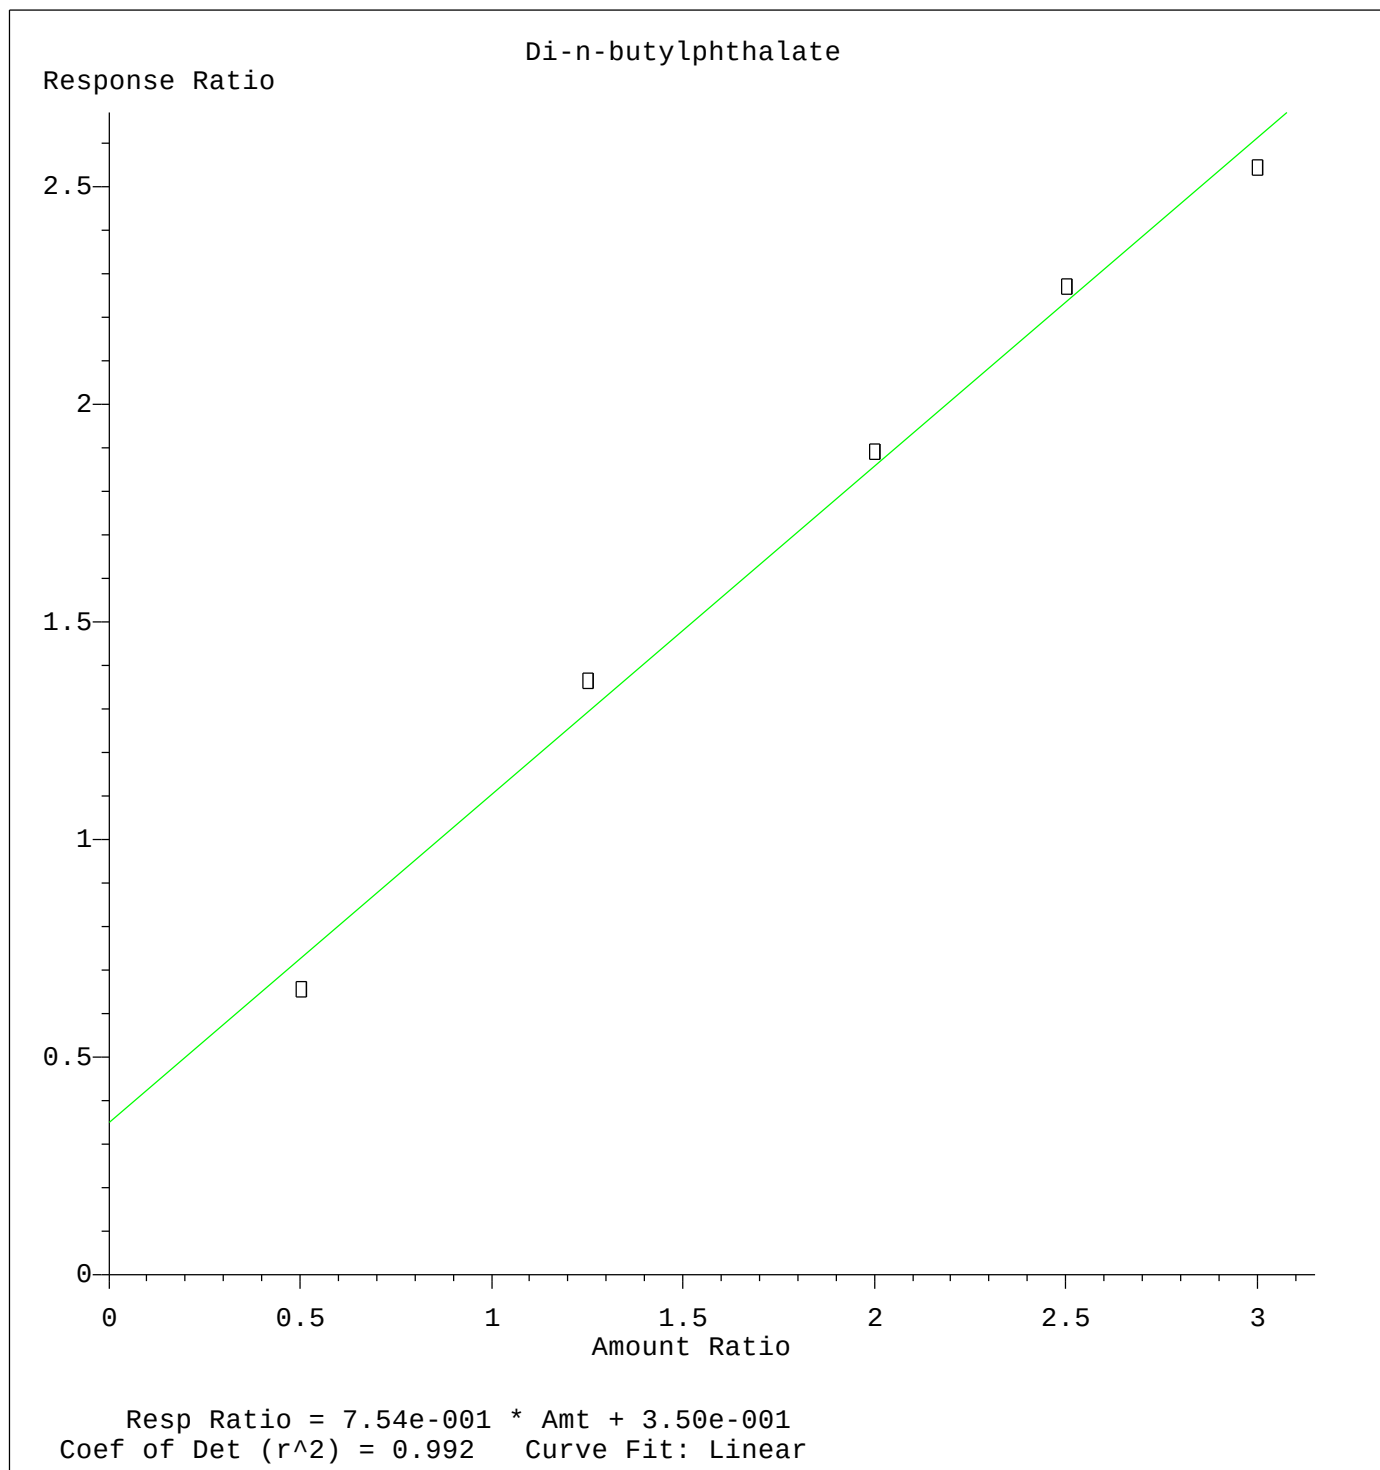


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016

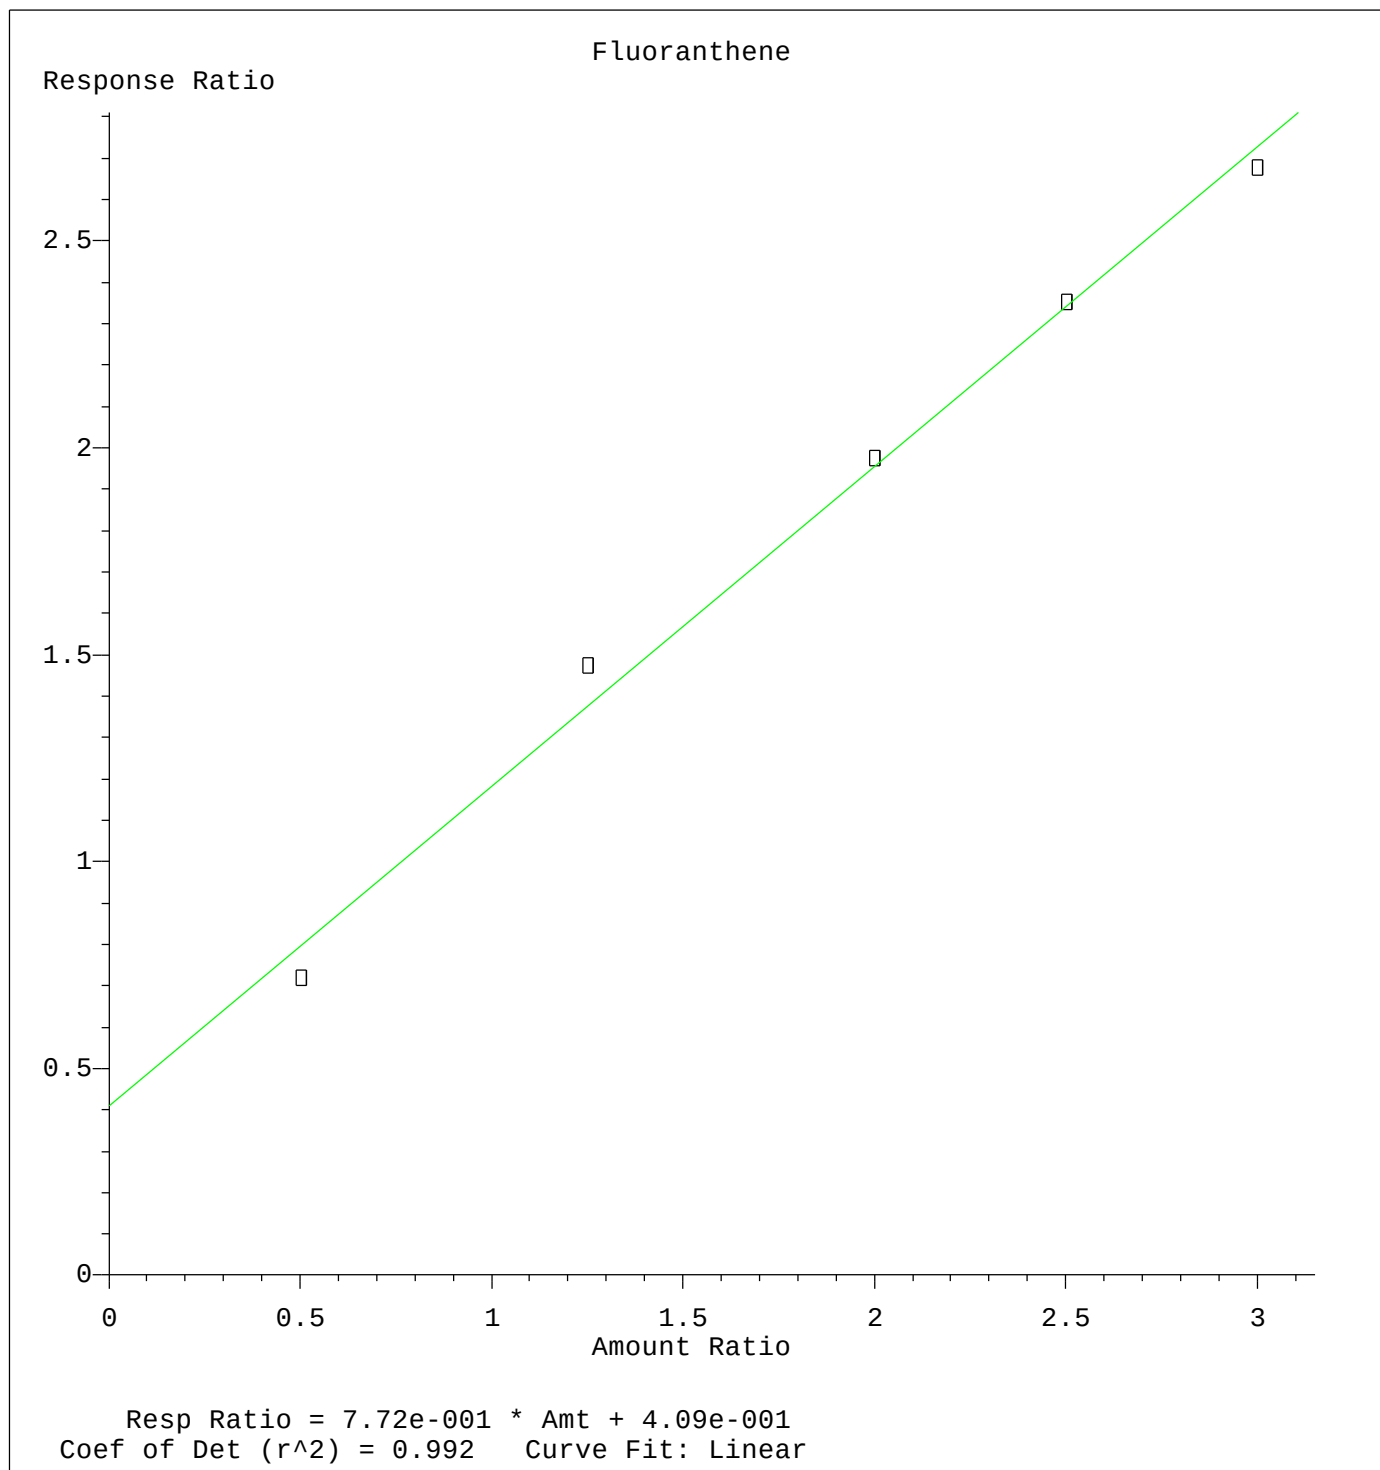

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016

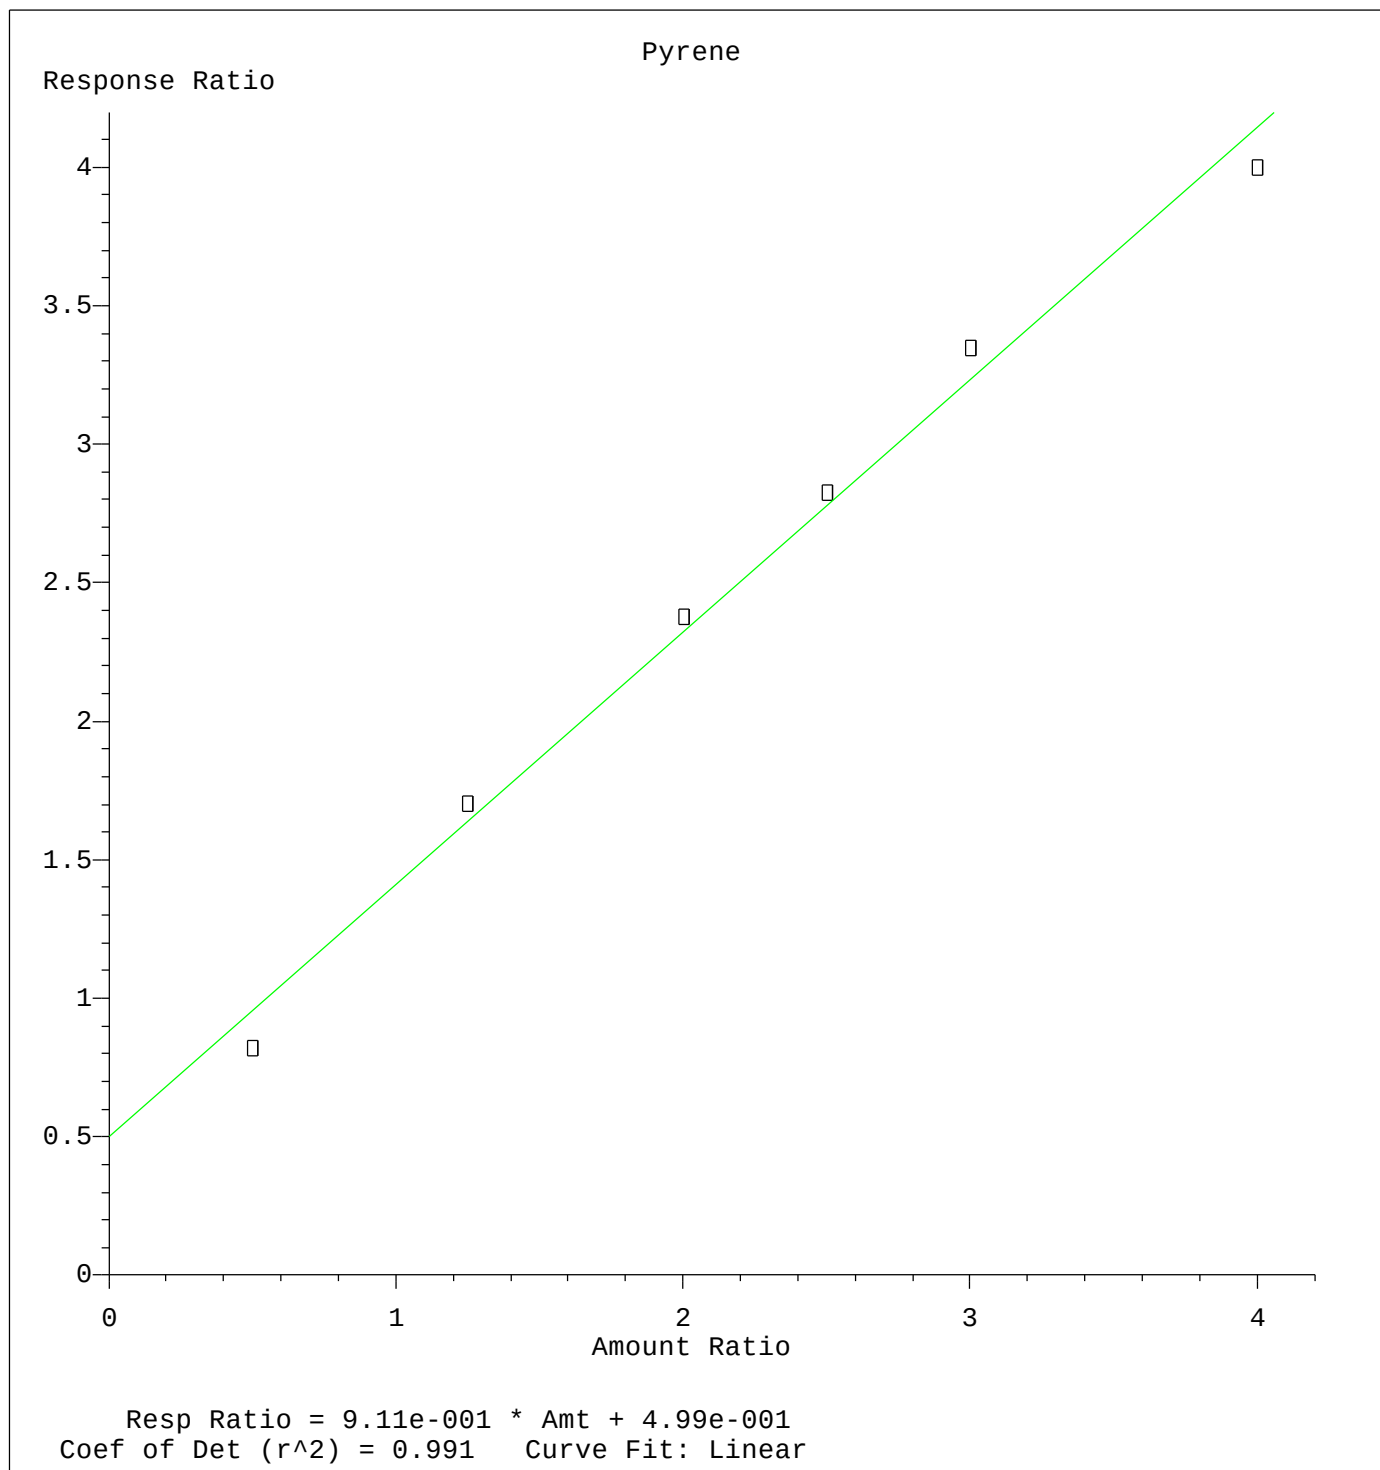

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016

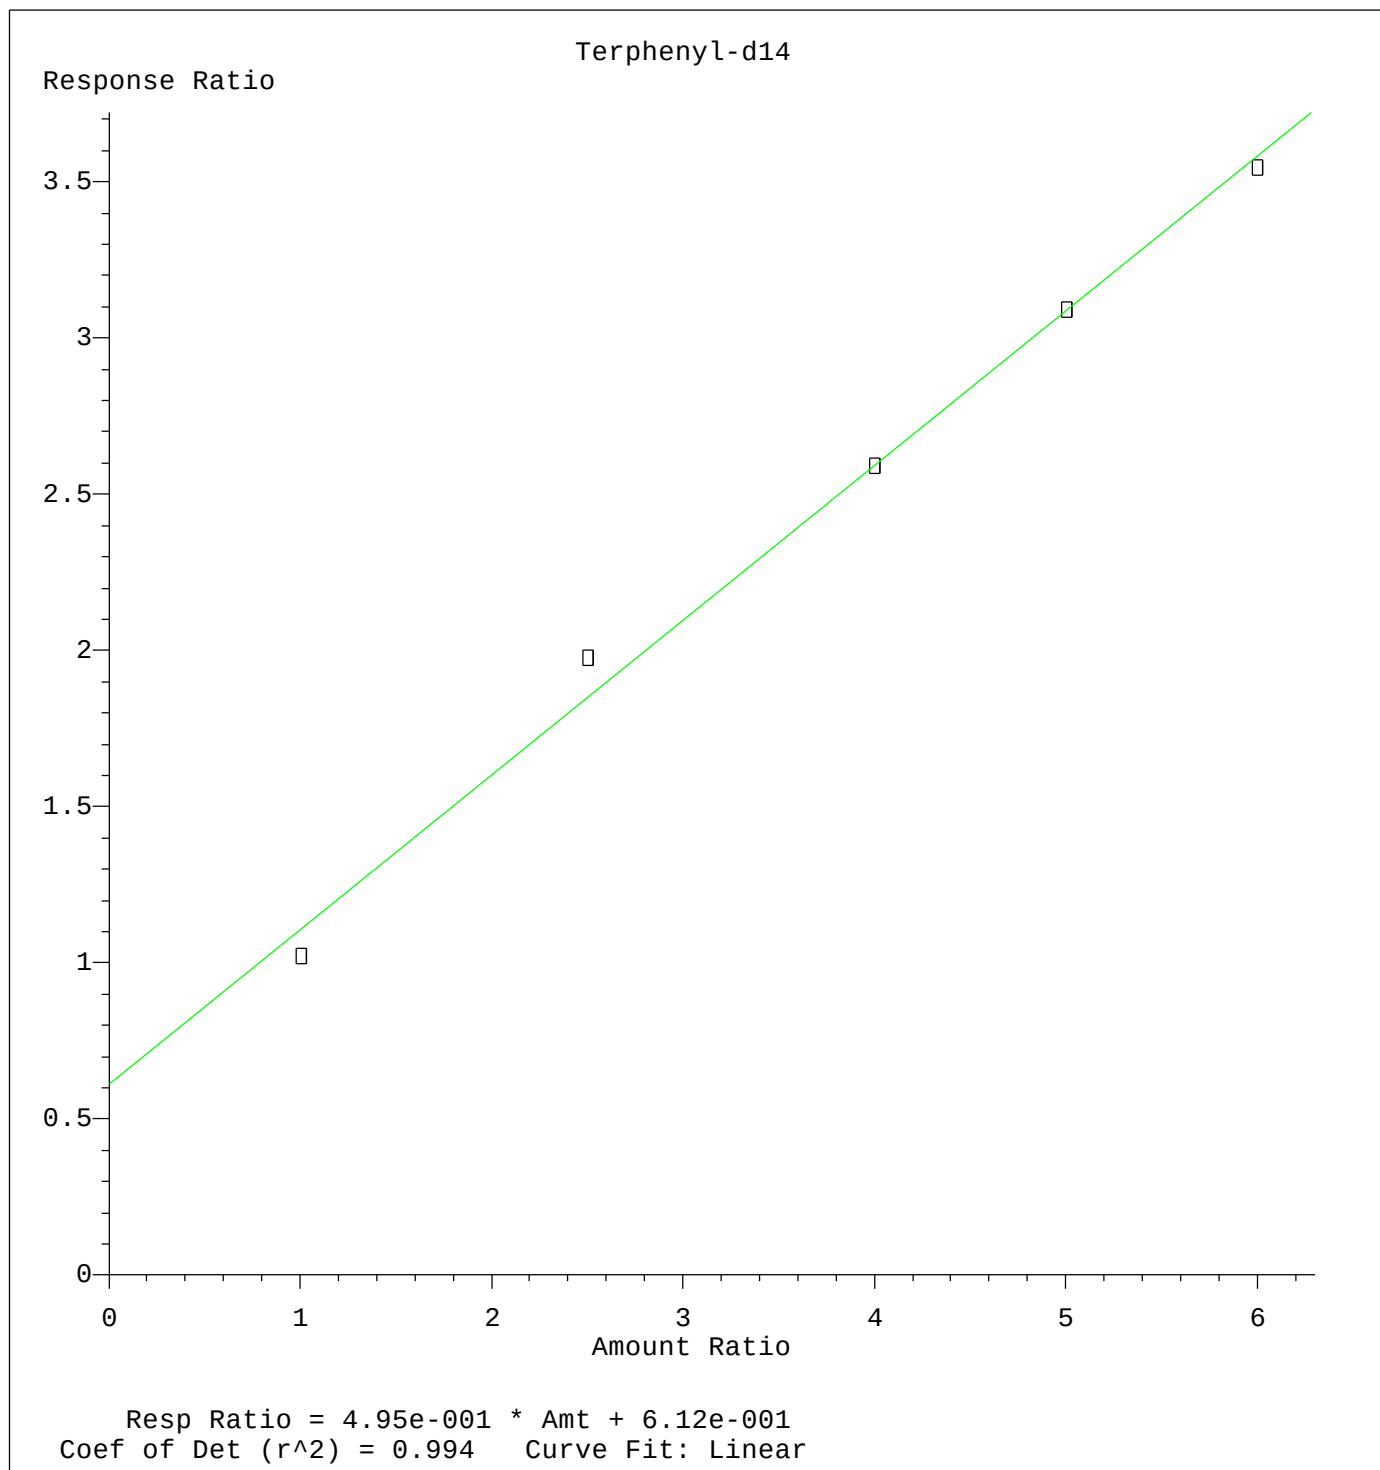

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Calibration Table Last Updated: Mon Aug 01 19:22:14 2016