
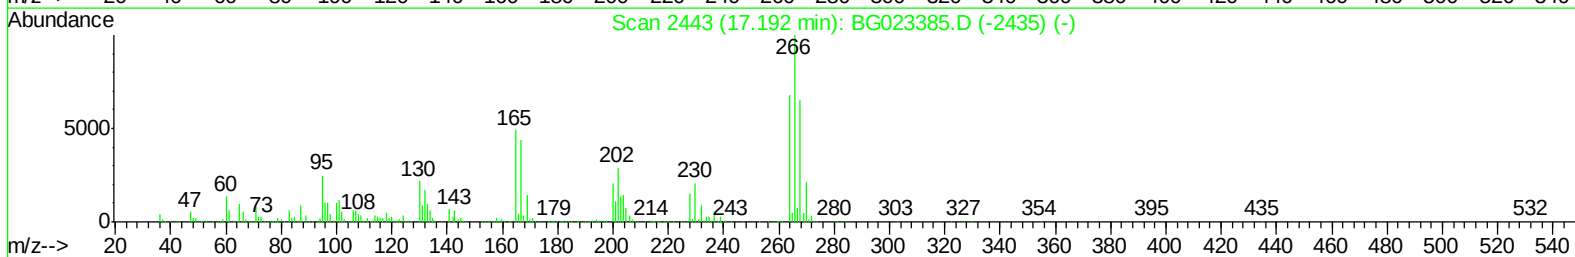
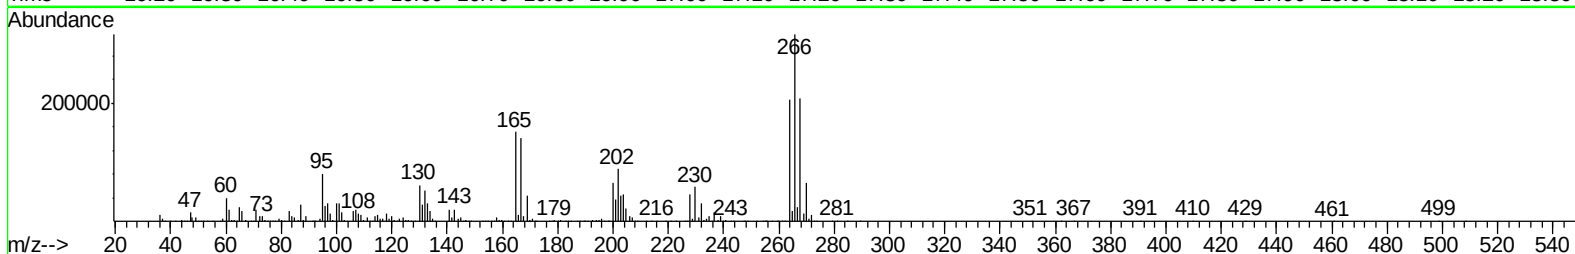


Data Path : Z:\HPCHEM1\BNA G\Data\BG080116\
Data File : BG023380.D
Acq On : 1 Aug 2016 10:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 17:42:20 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

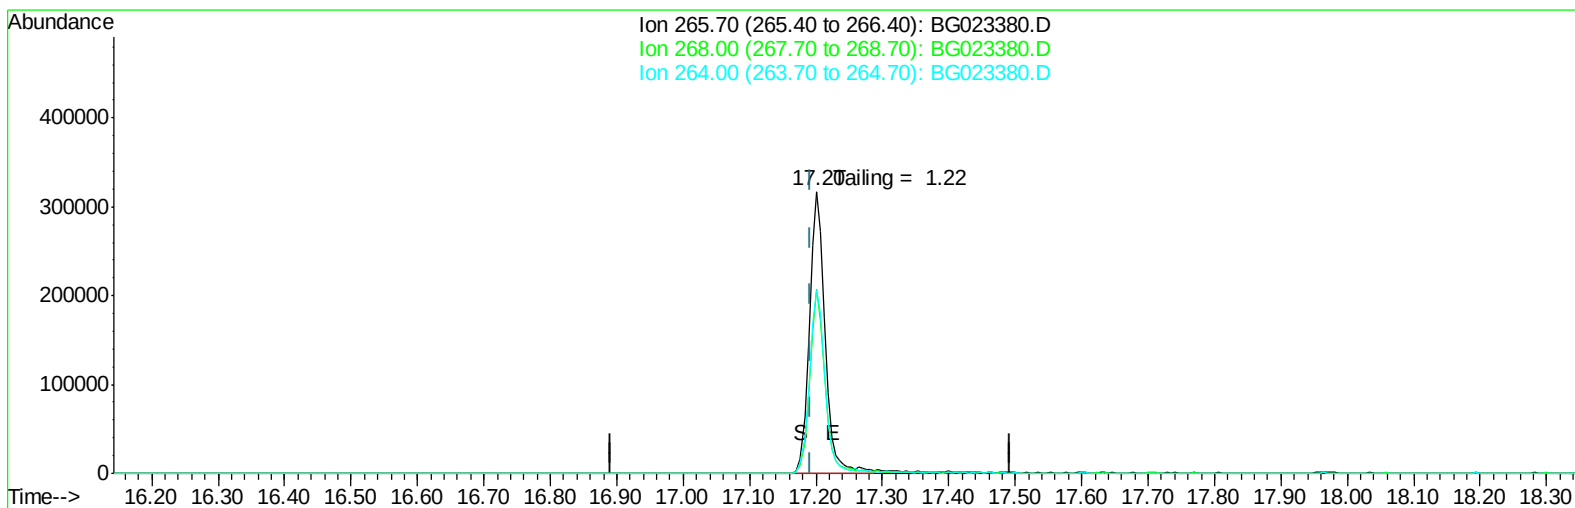

TIC: BG023380.D

(69) Pentachlorophenol (C)




17.200min (+0.008) 948416.79ng

response 528784

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.56
264.00	63.20	65.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG080116\
 Data File : BG023380.D
 Acq On : 1 Aug 2016 10:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 17:42:20 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 19:22:14 2016
 Response via : Initial Calibration

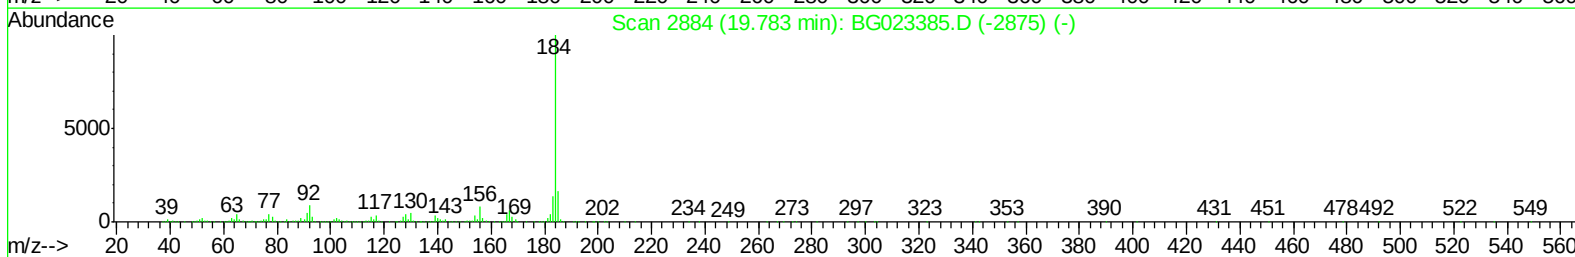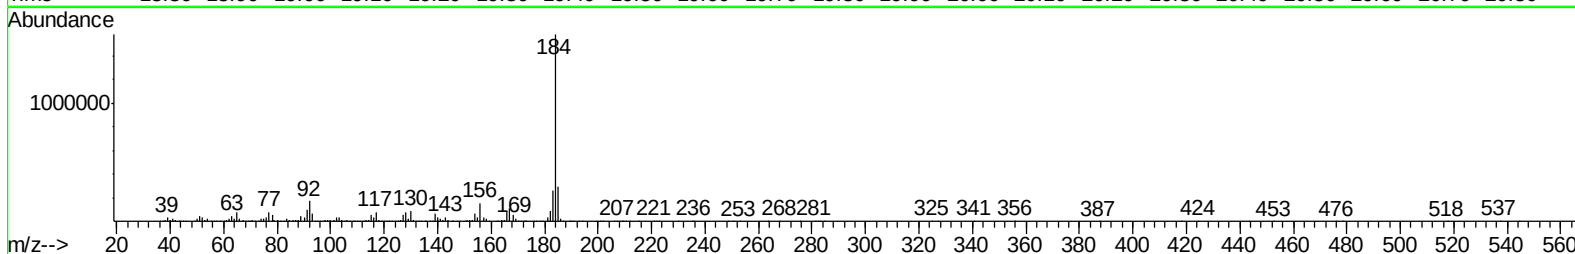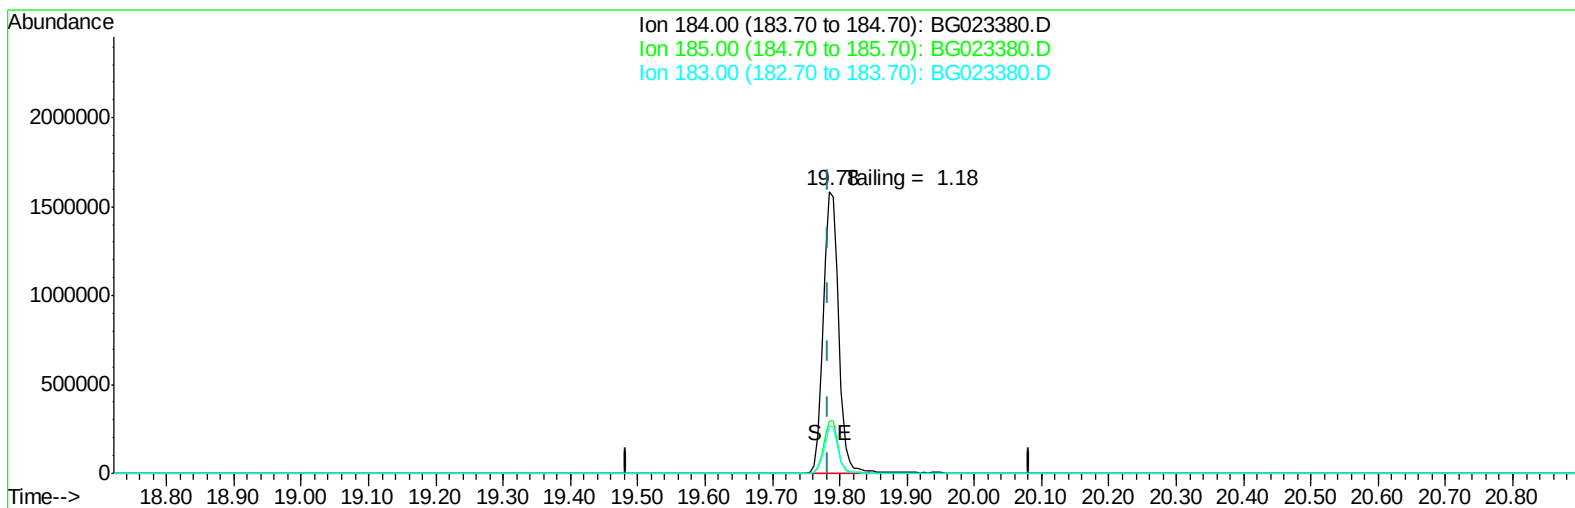

TIC: BG023380.D

(76) Benzidine

19.785min (+0.002) 1589216.36ng

response 2562322

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	18.82
183.00	13.40	16.71#
0.00	0.00	0.00