


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080116\
Data File : BG023380.D
Acq On : 1 Aug 2016 10:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 01 19:22:14 2016

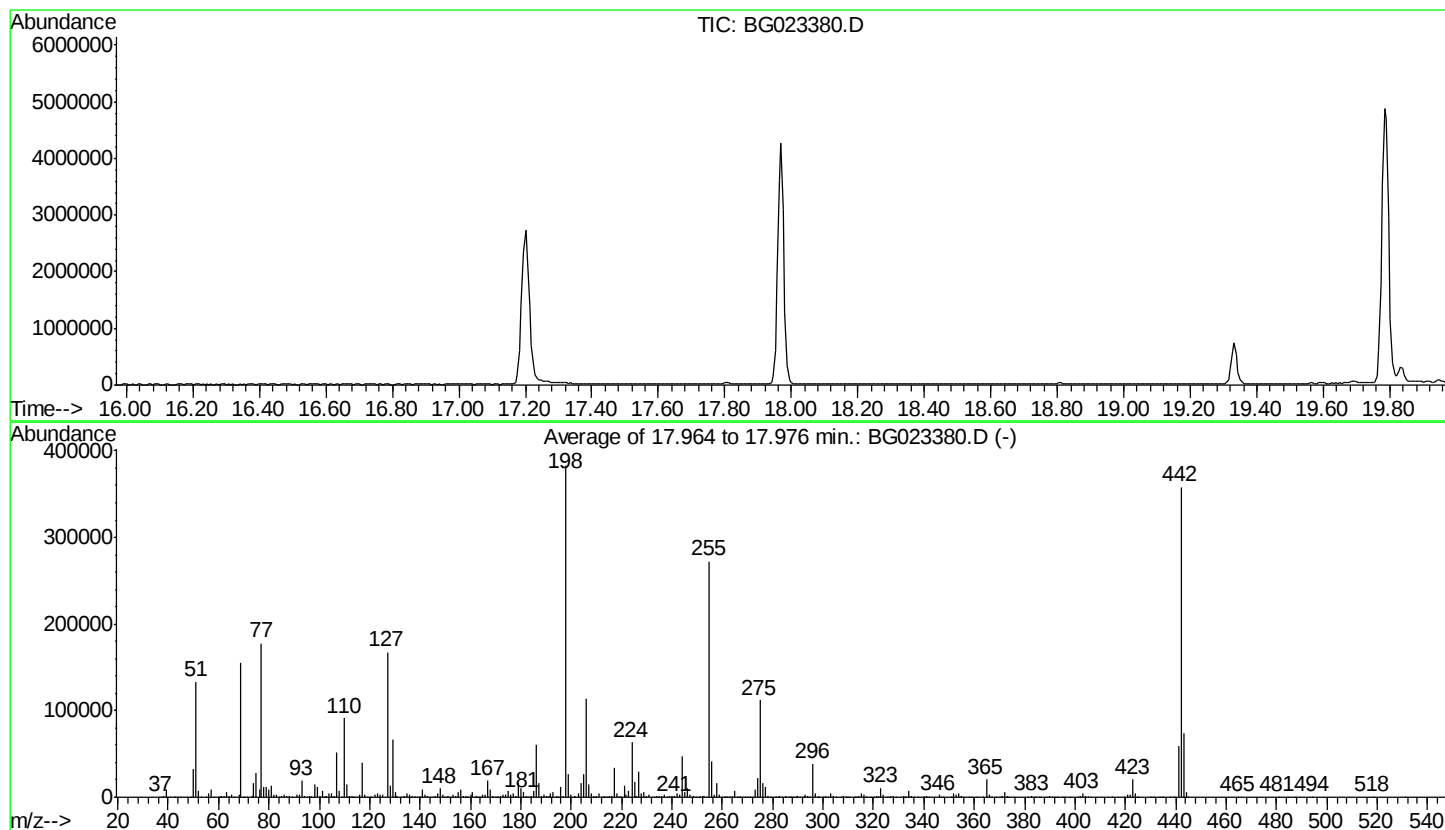

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	133047	PASS
68	69	0.00	2	2.0	3035	PASS
69	198	0.00	100	40.6	155309	PASS
70	69	0.00	2	0.4	647	PASS
127	198	10	80	43.8	167608	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	382869	PASS
199	198	5	9	7.1	27261	PASS
275	198	10	60	29.3	112224	PASS
365	198	1	100	5.3	20269	PASS
441	442	0.01	24	16.7	59848	PASS
442	198	50	100	93.5	358080	PASS
443	442	15	24	20.5	73429	PASS