


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080215\
Data File : BG018220.D
Acq On : 2 Aug 2015 11:44
Operator : TP
Sample : DFTPP23
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP23

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Title : SVOA CALIBRATION
Last Update : Tue Aug 04 02:54:30 2015

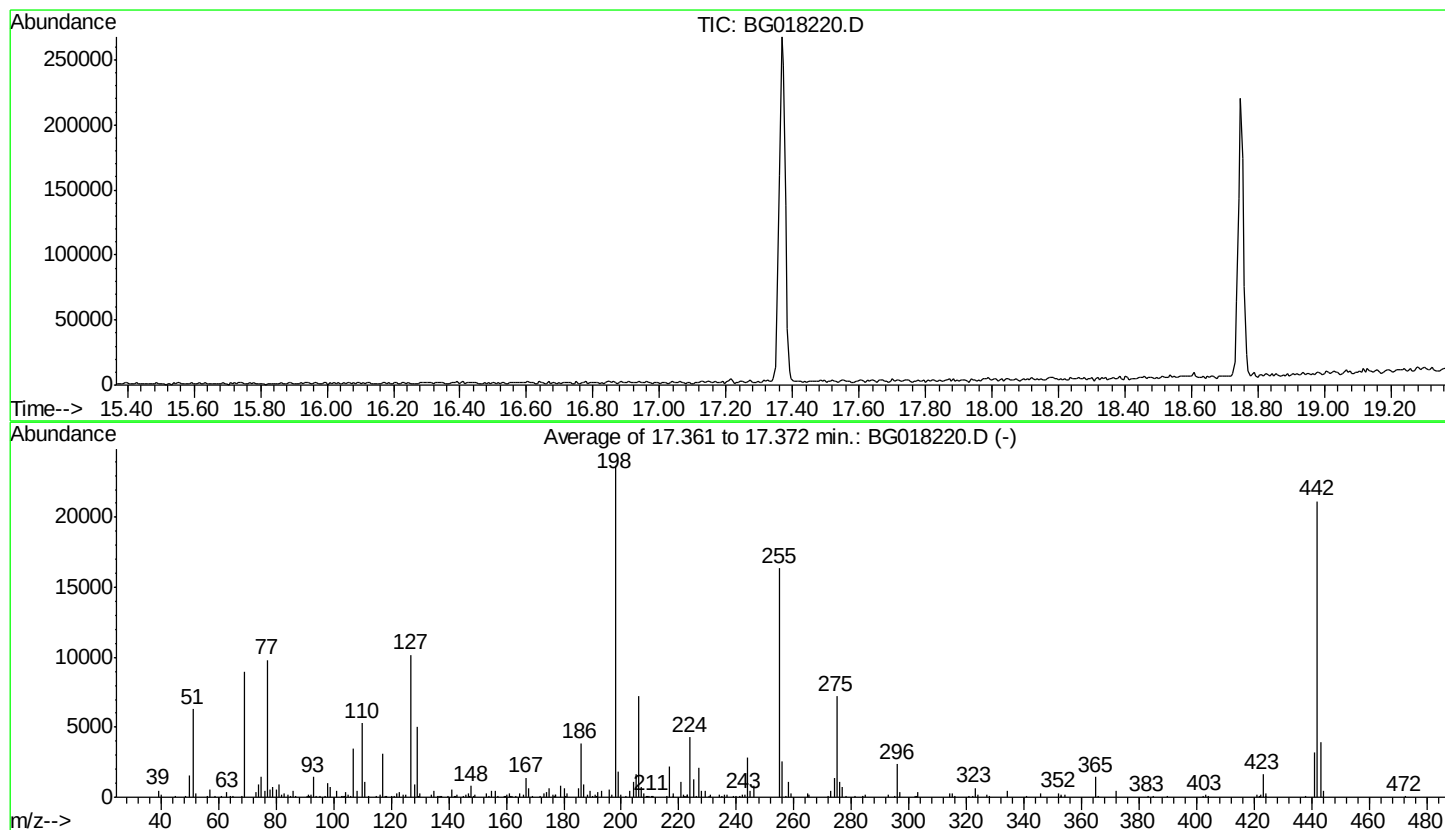

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	6281	PASS
68	69	0.00	2	1.1	98	PASS
69	198	0.00	100	37.9	8984	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	10193	PASS
197	198	0.00	2	0.9	207	PASS
198	198	100	100	100.0	23698	PASS
199	198	5	9	7.8	1854	PASS
275	198	10	60	30.5	7221	PASS
365	198	1	100	6.1	1440	PASS
441	442	0.01	24	14.9	3165	PASS
442	198	50	100	89.3	21172	PASS
443	442	15	24	18.5	3909	PASS

m/z	Abundance
38.90	542.0
39.90	233.0
50.00	1260.0
51.00	5509.0
52.00	278.0
55.90	158.0
57.00	468.0
58.90	159.0
62.80	311.0
63.90	162.0
68.00	295.0
69.00	8216.0
72.90	449.0
74.00	915.0
75.00	1264.0
75.90	251.0
77.00	8430.0
78.00	425.0
79.00	771.0
79.90	570.0
81.00	723.0
82.10	187.0
82.90	244.0
86.00	418.0
90.70	214.0
93.00	1211.0
98.00	752.0
98.90	768.0
100.90	499.0
103.80	322.0
105.00	286.0
107.00	3480.0
107.90	291.0
109.90	4420.0
110.90	896.0
115.00	161.0
116.00	215.0
116.90	2353.0
118.30	264.0
123.00	471.0
124.00	277.0
124.90	189.0
127.00	8345.0
128.00	728.0
129.00	3531.0
130.00	243.0
131.00	207.0
135.00	444.0
137.10	211.0
140.80	490.0
143.00	274.0
147.30	261.0
147.80	394.0
148.70	164.0
153.00	285.0
154.90	385.0
156.00	449.0
157.20	174.0
159.50	198.0
160.10	168.0
161.00	239.0
164.80	160.0
166.90	1005.0
167.90	524.0
174.00	341.0
175.00	502.0
176.60	198.0
177.20	177.0
178.90	721.0
180.00	399.0
181.00	214.0
185.00	428.0
186.00	3051.0
186.90	531.0
188.20	217.0
189.10	311.0
191.30	184.0
191.90	290.0
192.90	336.0
196.00	432.0
197.90	16800.0
199.00	1466.0
203.00	529.0
204.10	941.0
204.90	1332.0
206.00	5598.0
207.00	1007.0
216.80	1567.0
217.90	416.0
221.00	713.0
222.10	230.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

222.30	237.0
222.90	225.0
224.00	3064.0
224.90	1026.0
227.00	1367.0
228.00	202.0
229.00	405.0
231.10	274.0
235.90	237.0
240.00	164.0
241.00	151.0
244.00	2186.0
245.00	420.0
245.90	513.0
255.00	11281.0
256.00	1830.0
258.00	683.0
264.90	348.0
271.80	155.0
273.00	222.0
273.90	647.0
274.90	4554.0
276.00	748.0
276.90	521.0
292.90	236.0
296.00	1583.0
297.10	223.0
302.80	177.0
314.00	255.0
315.00	198.0
323.00	607.0
334.00	239.0
345.90	169.0
352.00	223.0
352.80	158.0
365.00	748.0
372.00	298.0
404.00	184.0
423.00	899.0
423.90	224.0
441.10	1625.0
442.10	12005.0
443.00	2076.0
444.00	255.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

m/z	Abundance
39.00	366.0
45.00	156.0
50.00	1962.0
51.00	7026.0
52.00	446.0
55.90	335.0
57.00	828.0
61.00	217.0
62.90	339.0
64.90	198.0
69.00	10417.0
73.00	313.0
74.00	891.0
75.00	2023.0
76.00	699.0
77.00	11440.0
78.00	777.0
79.00	680.0
80.00	586.0
81.00	1000.0
82.10	429.0
83.00	254.0
84.00	241.0
85.10	245.0
85.90	382.0
86.90	275.0
91.00	355.0
91.70	207.0
92.10	221.0
93.00	1924.0
98.00	1252.0
99.00	788.0
100.80	466.0
103.10	260.0
104.00	516.0
104.90	361.0
106.00	179.0
107.00	3827.0
108.00	542.0
110.00	5807.0
111.00	1376.0
112.00	353.0
115.90	231.0
116.90	3690.0
117.90	297.0
120.10	181.0
120.90	150.0
122.00	341.0
123.00	853.0
123.90	160.0
125.00	228.0
127.00	11938.0
128.00	918.0
129.00	6455.0
129.90	472.0
133.80	236.0
135.00	674.0
137.00	201.0
137.30	175.0
139.90	210.0
140.90	634.0
141.90	392.0
143.00	193.0
144.90	154.0
146.00	216.0
146.90	434.0
147.90	758.0
148.90	481.0
153.00	367.0
154.00	239.0
155.00	506.0
156.00	586.0
159.80	294.0
161.10	315.0
161.60	249.0
163.10	236.0
164.90	310.0
166.00	304.0
167.00	1716.0
167.90	791.0
168.90	296.0
172.90	283.0
174.00	391.0
175.00	692.0
176.00	460.0
177.10	345.0
178.90	1513.0
180.00	768.0
180.60	200.0
180.80	198.0
185.10	916.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

186.00	4586.0
186.90	828.0
188.10	272.0
188.90	527.0
190.90	228.0
191.90	451.0
193.00	579.0
195.90	469.0
196.70	203.0
197.90	28592.0
198.90	2006.0
199.90	266.0
201.50	234.0
203.10	482.0
204.00	1089.0
205.00	1786.0
206.00	8315.0
207.00	1460.0
208.00	298.0
208.80	188.0
209.10	172.0
209.80	273.0
210.90	331.0
216.90	2624.0
217.90	340.0
220.80	1677.0
221.80	438.0
223.10	579.0
224.00	5767.0
225.00	1165.0
226.00	310.0
226.90	2910.0
228.00	488.0
229.00	496.0
230.90	229.0
233.80	254.0
235.00	348.0
236.90	199.0
238.90	287.0
239.90	173.0
241.80	287.0
242.90	291.0
244.00	3073.0
245.00	459.0
246.00	1046.0
255.00	19648.0
256.00	2519.0
258.00	1076.0
258.90	333.0
264.90	492.0
272.90	718.0
274.00	1839.0
275.00	9010.0
276.00	1171.0
276.90	991.0
277.90	265.0
281.00	212.0
284.10	315.0
285.00	283.0
292.90	210.0
296.00	3151.0
296.90	557.0
302.10	156.0
303.00	423.0
314.00	196.0
315.10	387.0
315.90	186.0
323.00	845.0
324.10	176.0
327.00	264.0
327.90	174.0
333.90	608.0
340.90	175.0
346.00	247.0
352.00	320.0
353.00	228.0
354.10	323.0
364.90	1673.0
366.00	229.0
372.00	617.0
382.90	194.0
402.00	195.0
403.00	238.0
420.90	297.0
421.70	187.0
421.90	179.0
422.20	155.0
423.00	1956.0
424.10	290.0
437.70	150.0
441.10	3151.0
442.00	24336.0
443.00	4827.0
444.00	523.0
472.40	168.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

m/z	Abundance
39.00	516.0
40.00	276.0
43.90	172.0
48.70	268.0
50.00	1543.0
51.00	6799.0
51.90	238.0
55.10	195.0
55.90	248.0
57.00	915.0
63.00	402.0
66.90	280.0
68.90	8320.0
72.90	458.0
74.00	968.0
74.90	1157.0
76.00	437.0
77.00	9561.0
78.00	472.0
78.90	657.0
80.00	515.0
81.00	954.0
83.00	299.0
83.90	225.0
85.90	447.0
91.10	176.0
92.00	230.0
92.90	1224.0
93.80	163.0
95.10	307.0
97.00	204.0
97.90	1021.0
98.90	605.0
100.90	470.0
102.80	240.0
104.10	492.0
105.00	417.0
107.00	3181.0
108.00	501.0
110.00	5680.0
111.00	939.0
117.00	3222.0
122.00	581.0
123.00	945.0
124.00	252.0
125.00	273.0
127.00	10296.0
127.90	1020.0
129.00	5115.0
129.70	243.0
131.10	212.0
133.80	368.0
135.00	357.0
136.00	185.0
136.80	343.0
140.90	594.0
142.20	265.0
143.00	179.0
145.90	225.0
147.00	490.0
148.00	1268.0
149.00	165.0
152.90	269.0
155.00	407.0
156.00	428.0
160.10	299.0
160.90	361.0
161.90	157.0
164.90	362.0
166.10	246.0
167.00	1438.0
168.00	507.0
171.70	156.0
172.90	429.0
173.90	313.0
174.90	767.0
176.90	435.0
178.90	950.0
180.00	701.0
181.00	321.0
185.00	526.0
186.00	3789.0
187.00	1439.0
188.90	452.0
189.80	151.0
190.80	229.0
191.90	415.0
192.90	512.0
195.90	803.0
196.80	419.0
197.90	25704.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

198.80	2091.0
199.90	166.0
203.00	282.0
204.00	1395.0
205.00	1924.0
206.00	7657.0
207.00	1244.0
207.90	502.0
208.90	203.0
210.50	252.0
211.10	326.0
215.80	192.0
217.00	2413.0
218.10	183.0
220.90	877.0
222.10	186.0
222.80	402.0
224.00	3946.0
225.00	1578.0
226.90	2068.0
227.80	608.0
228.90	502.0
230.70	218.0
233.90	240.0
236.00	224.0
236.90	265.0
241.90	270.0
242.90	296.0
244.00	3330.0
244.90	480.0
245.90	841.0
249.10	196.0
255.00	18160.0
256.00	3296.0
257.00	243.0
258.00	1642.0
258.80	435.0
265.10	580.0
273.00	506.0
274.00	1703.0
275.00	8099.0
276.00	1361.0
276.90	576.0
283.80	179.0
285.00	180.0
292.90	240.0
295.10	195.0
295.90	2400.0
296.90	442.0
303.00	610.0
314.10	374.0
315.00	316.0
316.00	215.0
321.00	222.0
322.00	170.0
323.10	482.0
323.90	258.0
326.90	283.0
334.00	510.0
345.90	287.0
352.00	403.0
353.00	314.0
354.20	205.0
364.90	1900.0
365.80	180.0
372.00	559.0
384.90	164.0
390.00	152.0
402.10	178.0
403.10	308.0
421.00	212.0
422.10	366.0
423.10	1988.0
424.10	456.0
441.10	4719.0
442.10	27176.0
443.10	4826.0
444.10	599.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23

Scan 2492 (17.331 min): BG018220.D
DFTPP23

m/z	Abundance
40.90	244.0
43.90	185.0
51.00	163.0
54.90	230.0
56.00	151.0
57.00	194.0
66.90	188.0
105.00	212.0
123.10	412.0
131.00	161.0
179.00	233.0
206.90	465.0
249.00	161.0

Instrument :
BNA_G
ClientSampleId :
DFTPP23