
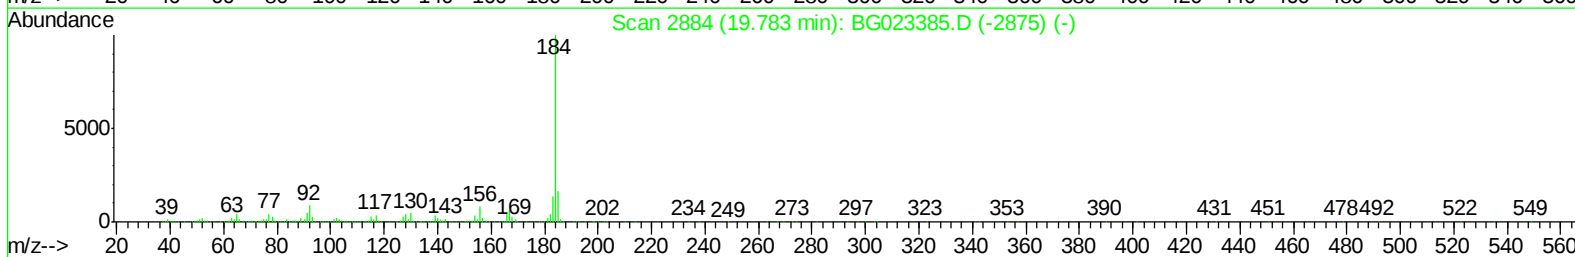
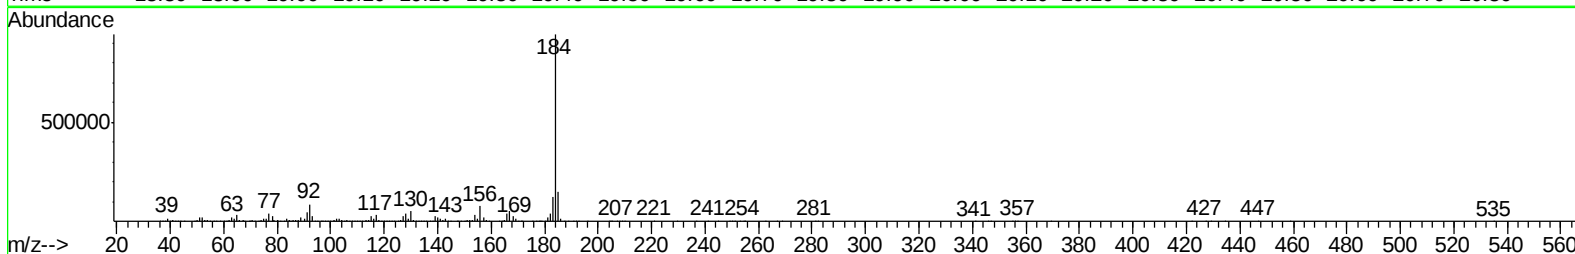


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080216\
Data File : BG023393.D
Acq On : 2 Aug 2016 8:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:10:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

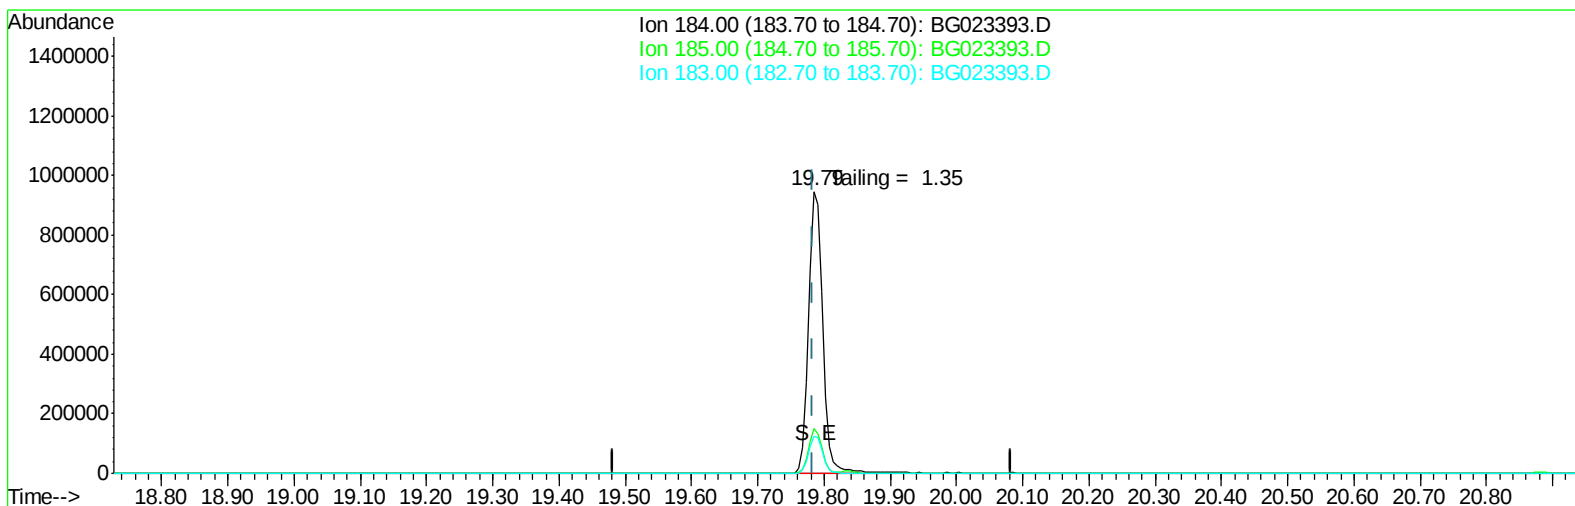

TIC: BG023393.D

(76) Benzidine




19.785min (+0.002) 36761.08ng

response 1435778

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.73
183.00	13.40	13.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG080216\
Data File : BG023393.D
Acq On : 2 Aug 2016 8:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:10:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

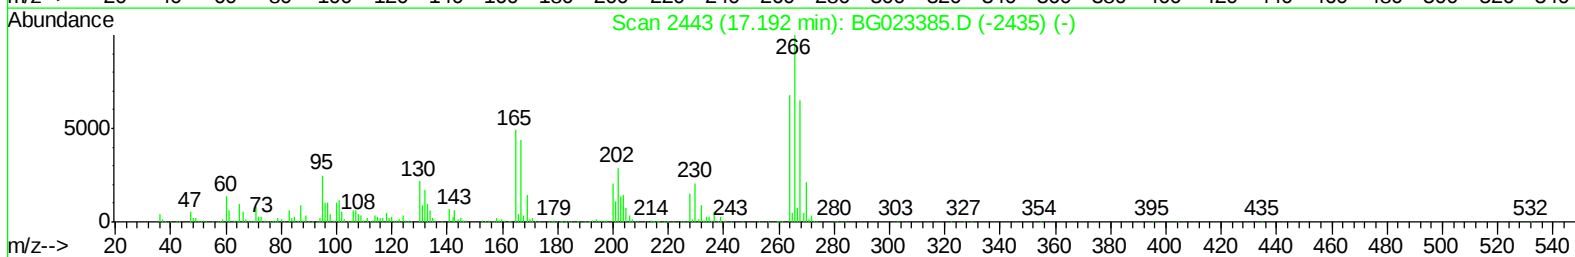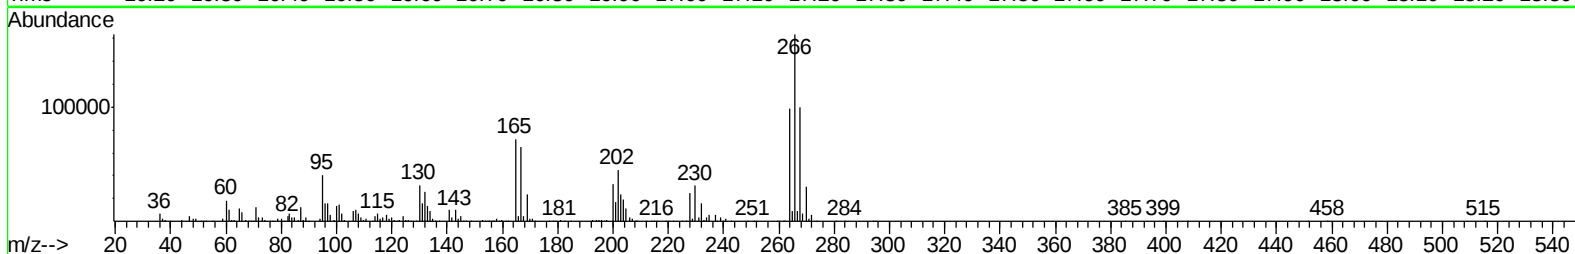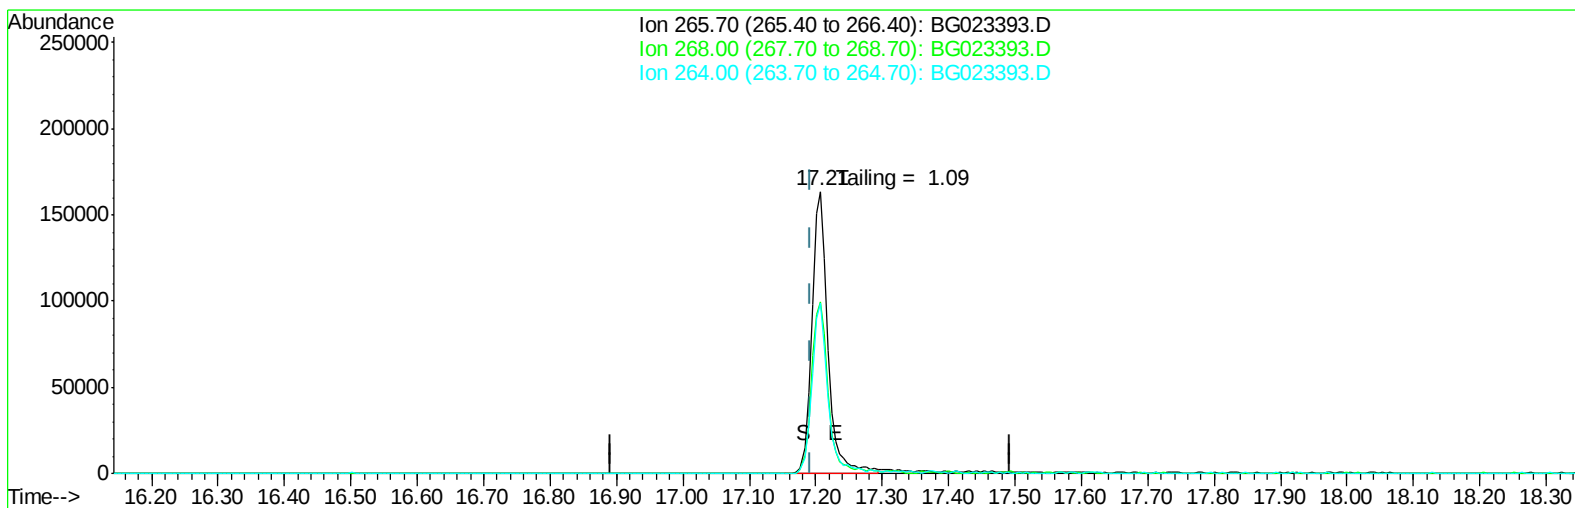

TIC: BG023393.D

(69) Pentachlorophenol (C)

17.206min (+0.014) 154659.40ng

response 280533

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	60.86
264.00	63.20	60.30
0.00	0.00	0.00