
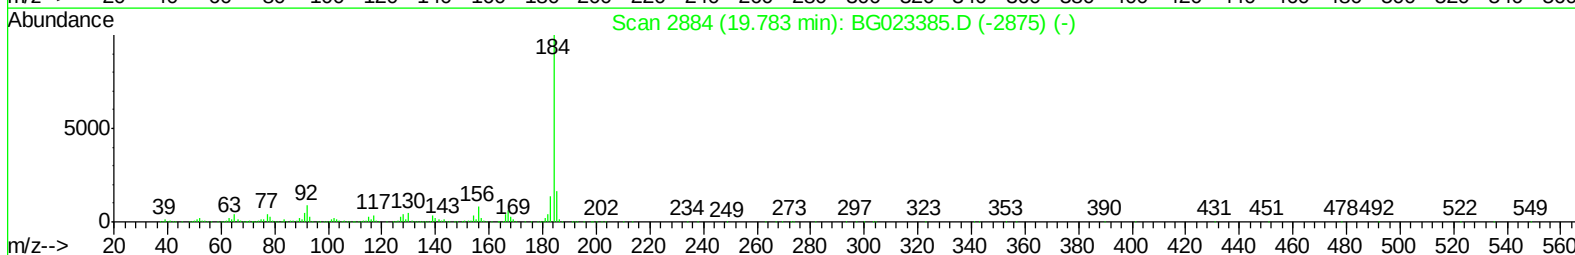
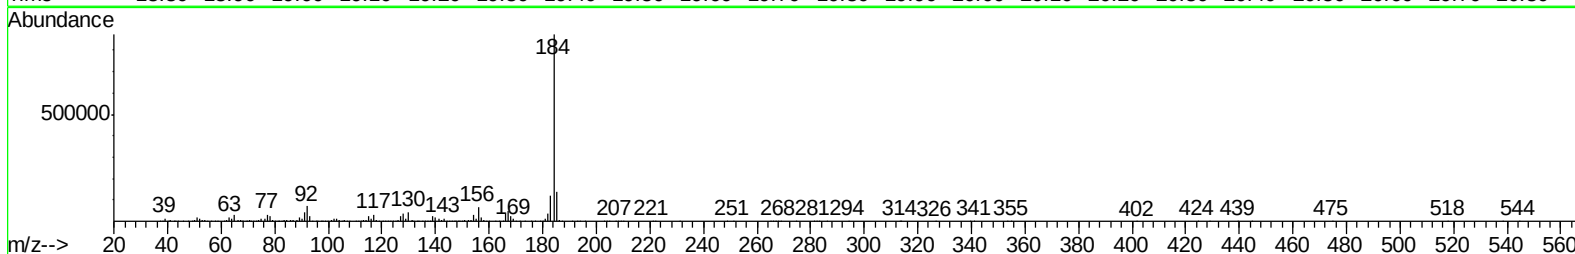


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080216\
Data File : BG023400.D
Acq On : 2 Aug 2016 17:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:11:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

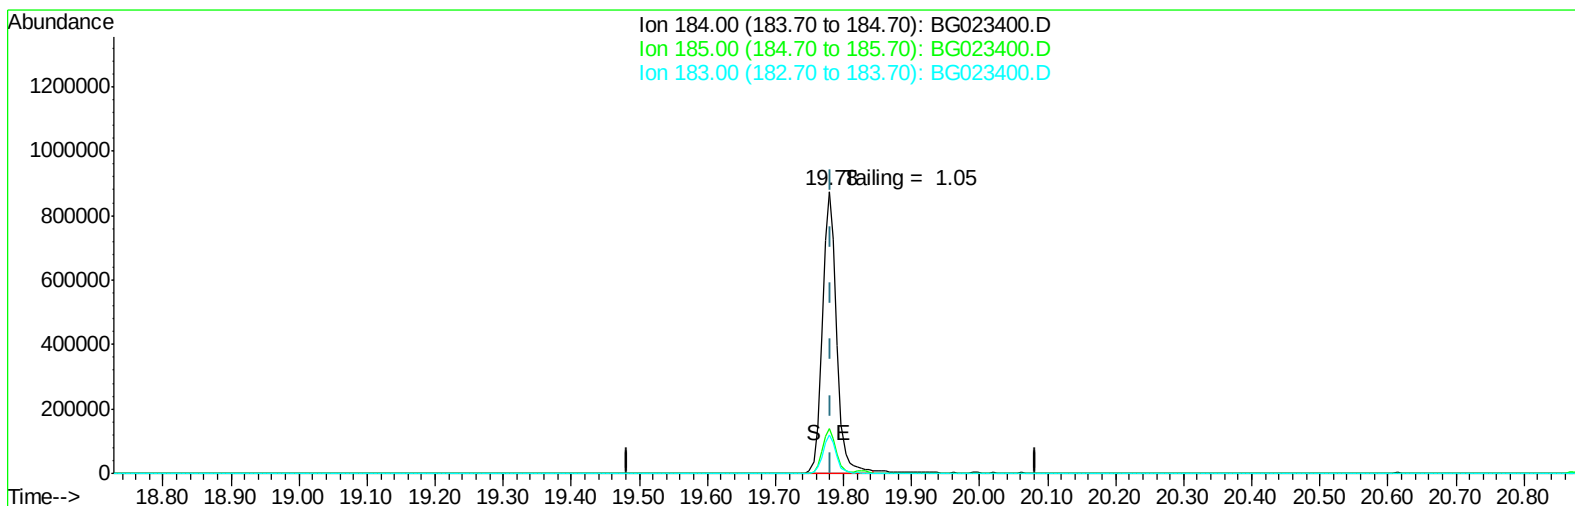

TIC: BG023400.D

(76) Benzidine




19.779min (-0.004) 49170.49ng

response 1305361

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.11
183.00	13.40	13.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG080216\
Data File : BG023400.D
Acq On : 2 Aug 2016 17:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:11:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

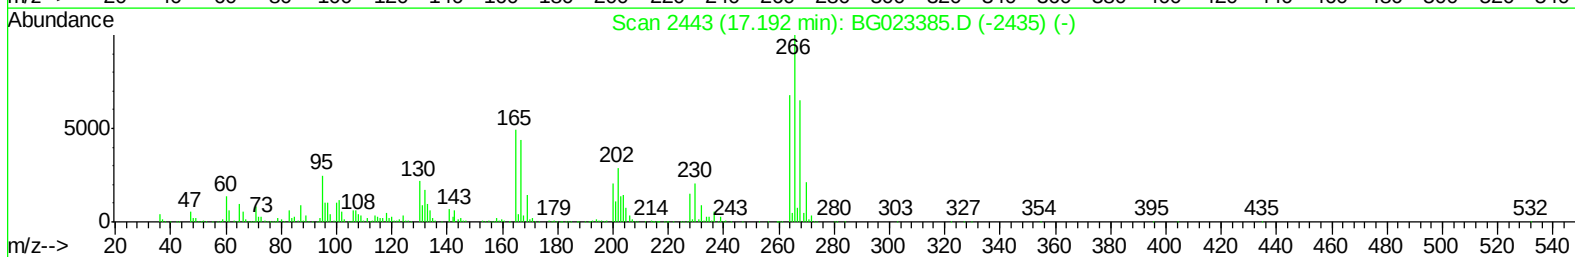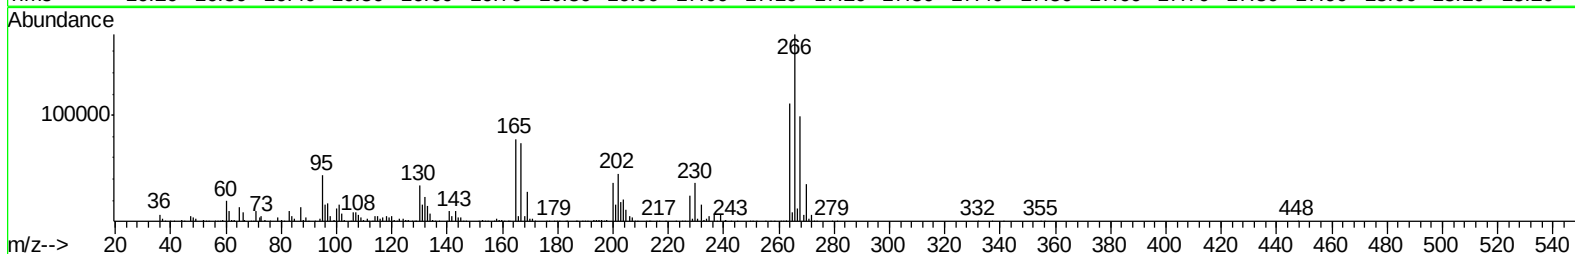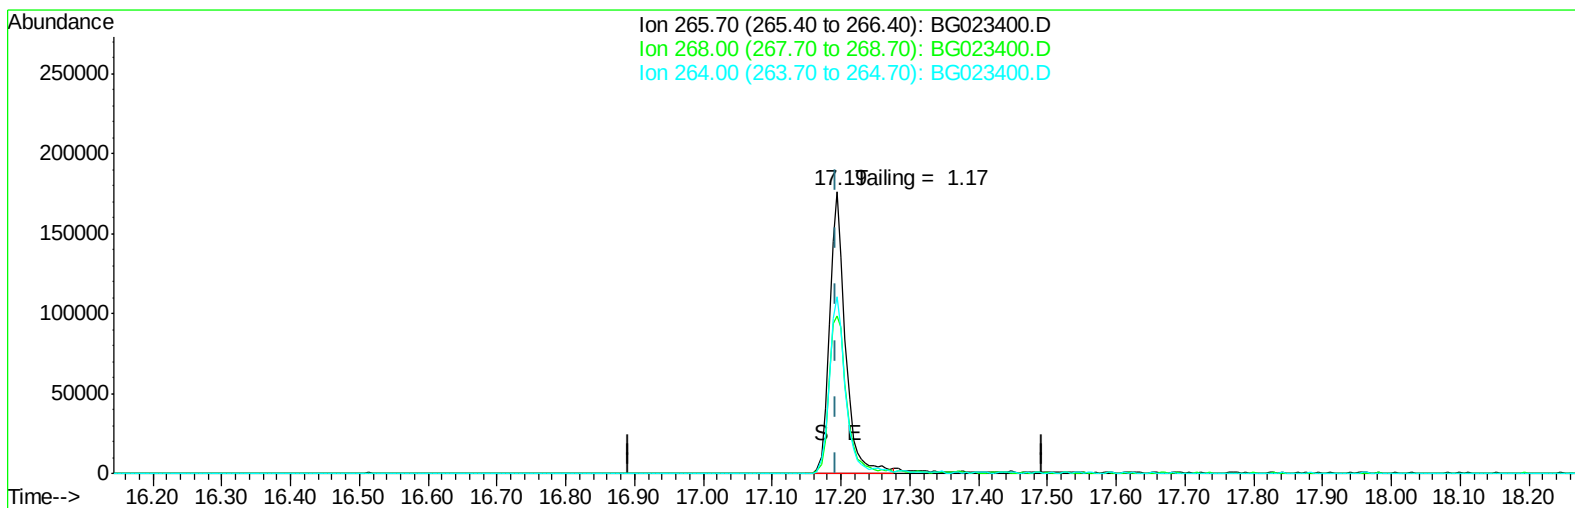

TIC: BG023400.D

(69) Pentachlorophenol (C)

17.195min (+0.002) 450615.00ng

response 284736

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	56.02
264.00	63.20	62.75
0.00	0.00	0.00