


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080216\
 Data File : BG023393.D
 Acq On : 2 Aug 2016 8:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

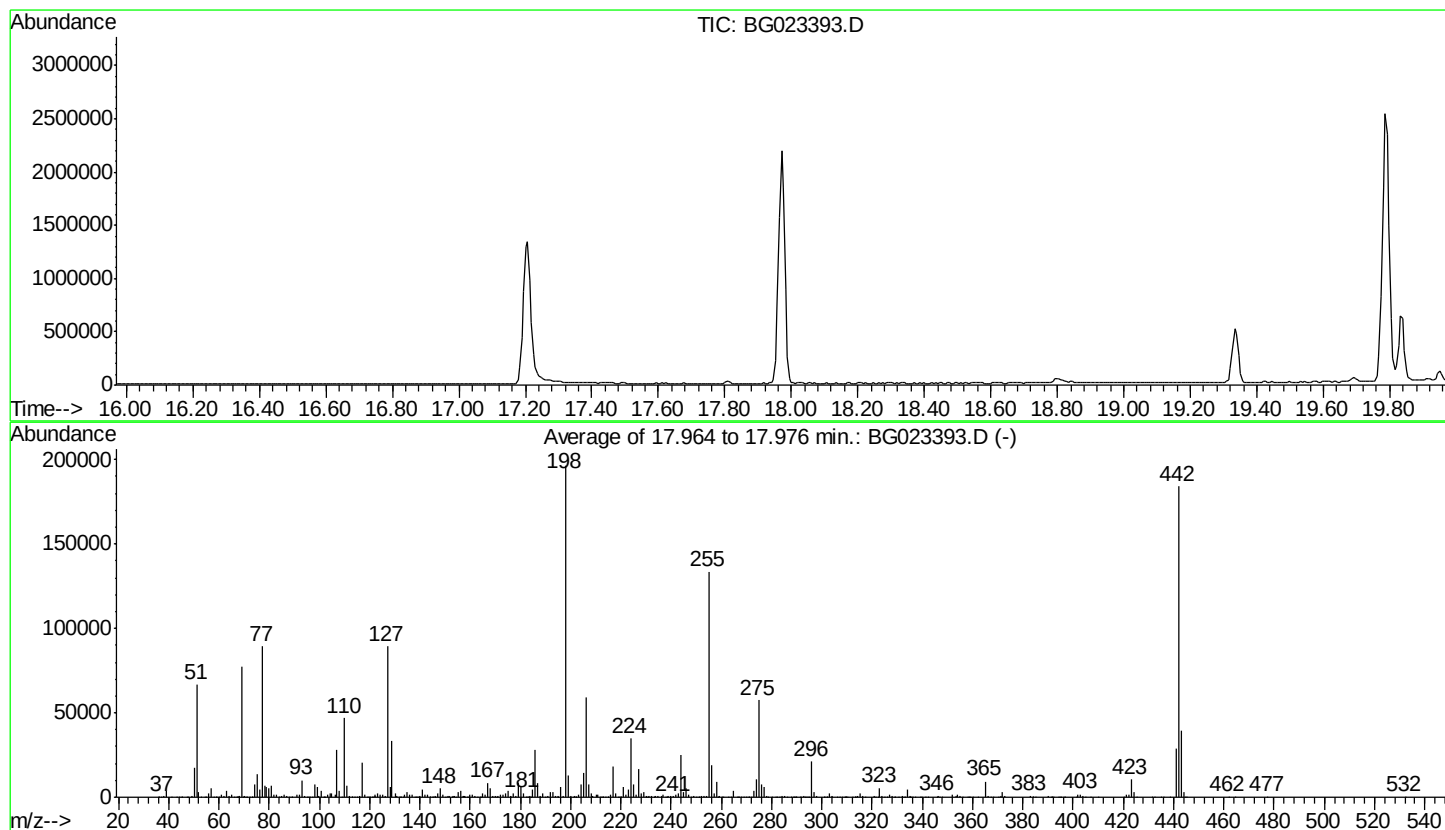

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	66674	PASS
68	69	0.00	2	1.1	839	PASS
69	198	0.00	100	39.5	77573	PASS
70	69	0.00	2	0.5	415	PASS
127	198	10	80	45.4	89165	PASS
197	198	0.00	2	0.4	743	PASS
198	198	100	100	100.0	196394	PASS
199	198	5	9	6.6	12992	PASS
275	198	10	60	29.3	57458	PASS
365	198	1	100	4.8	9486	PASS
441	442	0.01	24	15.5	28472	PASS
442	198	50	100	93.7	184002	PASS
443	442	15	24	21.5	39541	PASS