


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080216\
 Data File : BG023400.D
 Acq On : 2 Aug 2016 17:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

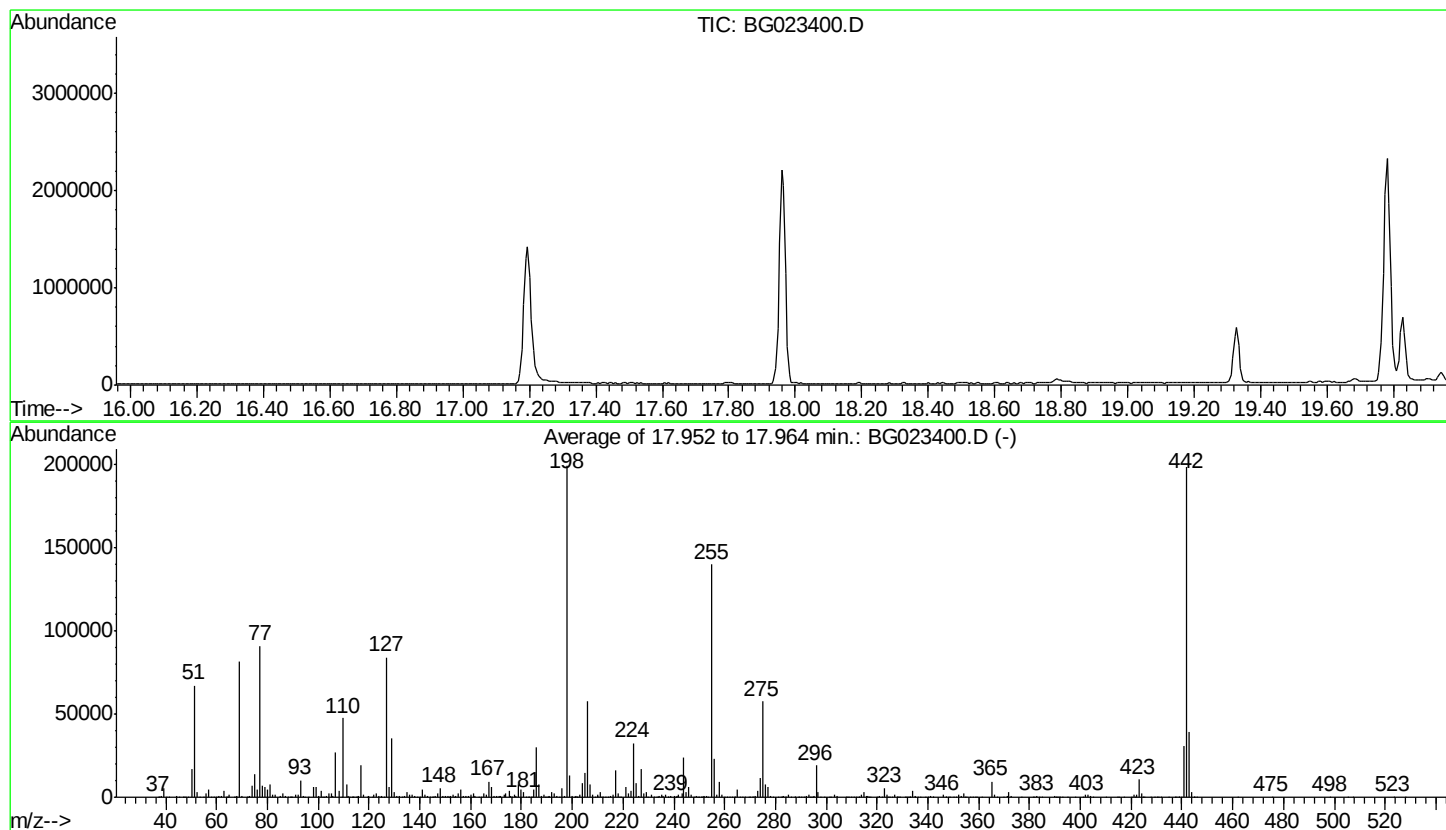

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	67128	PASS
68	69	0.00	2	0.7	566	PASS
69	198	0.00	100	41.1	81744	PASS
70	69	0.00	2	0.7	551	PASS
127	198	10	80	42.2	84030	PASS
197	198	0.00	2	0.5	929	PASS
198	198	100	100	100.0	199018	PASS
199	198	5	9	6.6	13198	PASS
275	198	10	60	28.8	57416	PASS
365	198	1	100	4.7	9329	PASS
441	442	0.01	24	15.6	30917	PASS
442	198	50	100	99.5	198040	PASS
443	442	15	24	19.7	39034	PASS