

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080217\
 Data File : BG028110.D
 Acq On : 2 Aug 2017 15:59
 Operator : SJ/JU
 Sample : PB100940BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.845	41	44	55	rVB6	7871	14786	1.11%	0.121%
2	4.327	122	126	129	rBV5	1326	1969	0.15%	0.016%
3	4.409	135	140	143	rVB3	1045	1978	0.15%	0.016%
4	4.767	198	201	204	rBV2	1276	1792	0.13%	0.015%
5	5.014	238	243	245	rVB3	1223	1926	0.14%	0.016%
6	5.619	342	346	350	rBV	1167	2076	0.16%	0.017%
7	6.571	505	508	511	rVB3	1370	1999	0.15%	0.016%
8	7.047	583	589	591	rBV	1012	1831	0.14%	0.015%
9	7.505	660	667	684	rBV	124438	236351	17.75%	1.927%
10	7.676	684	696	712	rBV	97192	173266	13.01%	1.413%
11	7.893	722	733	747	rBV	123034	224182	16.83%	1.828%
12	8.287	794	800	805	rBV2	1221	2884	0.22%	0.024%
13	8.363	805	813	825	rVV	98988	179613	13.49%	1.465%
14	9.051	920	930	947	rVB2	155234	300113	22.53%	2.447%
15	9.368	981	984	990	rVB	1131	1803	0.14%	0.015%
16	9.532	1002	1012	1024	rBV2	132297	257911	19.37%	2.103%
17	10.073	1101	1104	1107	rBV2	1417	1831	0.14%	0.015%
18	10.255	1127	1135	1151	rVB	113923	216484	16.26%	1.765%
19	10.713	1208	1213	1216	rBV	1207	1770	0.13%	0.014%
20	10.796	1220	1227	1242	rBV	148514	293205	22.02%	2.391%
21	11.183	1282	1293	1306	rVB	163199	304043	22.83%	2.479%
22	11.313	1306	1315	1329	rBV	166487	334460	25.11%	2.727%
23	11.577	1358	1360	1371	rVB2	1358	3015	0.23%	0.025%
24	12.752	1554	1560	1566	rBV3	2131	4578	0.34%	0.037%
25	12.999	1597	1602	1606	rBV	901	1864	0.14%	0.015%
26	14.362	1824	1834	1848	rBV	409113	623352	46.81%	5.083%
27	14.668	1877	1886	1895	rBV	375451	623343	46.81%	5.083%
28	14.967	1927	1937	1950	rVB2	290867	488345	36.67%	3.982%
29	15.085	1950	1957	1961	rVB2	1081	2080	0.16%	0.017%
30	15.149	1961	1968	1990	rBV	114006	266589	20.02%	2.174%
31	15.296	1990	1993	1998	rVV2	3519	5936	0.45%	0.048%
32	15.332	1998	1999	2004	rVB2	2158	2113	0.16%	0.017%
33	15.960	2097	2106	2114	rBV	572003	885458	66.49%	7.220%
34	16.066	2118	2124	2139	rBV	198825	323401	24.28%	2.637%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080217\
 Data File : BG028110.D
 Acq On : 2 Aug 2017 15:59
 Operator : SJ/JU
 Sample : PB100940BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

35	16.201	2143	2147	2150	rVB2	6060	8248	0.62%	0.067%
36	16.918	2263	2269	2273	rBV	952	2581	0.19%	0.021%
37	17.505	2364	2369	2374	rBV	2410	3612	0.27%	0.029%
38	17.717	2398	2405	2413	rBV	459738	710847	53.38%	5.796%
39	17.817	2415	2422	2437	rVB	698454	1098427	82.48%	8.956%
40	17.964	2443	2447	2451	rVB2	1119	1845	0.14%	0.015%
41	18.087	2462	2468	2470	rBV	1521	1882	0.14%	0.015%
42	18.122	2470	2474	2475	rVB2	1355	1850	0.14%	0.015%
43	18.287	2496	2502	2505	rBV2	1168	2285	0.17%	0.019%
44	18.904	2602	2607	2612	rVB2	1019	2120	0.16%	0.017%
45	19.092	2634	2639	2646	rBV4	1971	3928	0.29%	0.032%
46	19.638	2728	2732	2733	rBV2	1411	1883	0.14%	0.015%
47	19.726	2742	2747	2752	rVB2	8117	9694	0.73%	0.079%
48	19.979	2784	2790	2795	rBV3	6626	11606	0.87%	0.095%
49	20.091	2801	2809	2820	rBV	917294	1331784	100.00%	10.859%
50	20.220	2826	2831	2834	rVB5	3292	4586	0.34%	0.037%
51	20.314	2844	2847	2853	rVB4	2426	4463	0.34%	0.036%
52	20.473	2873	2874	2878	rBV3	2390	3396	0.25%	0.028%
53	20.672	2903	2908	2912	rBV6	2164	3848	0.29%	0.031%
54	21.037	2967	2970	2972	rBV3	1942	2582	0.19%	0.021%
55	21.195	2994	2997	3001	rBV4	2975	3821	0.29%	0.031%
56	21.283	3007	3012	3015	rBV5	2411	4352	0.33%	0.035%
57	21.307	3015	3016	3020	rBV4	2120	2374	0.18%	0.019%
58	21.477	3043	3045	3051	rVB6	2006	2660	0.20%	0.022%
59	21.636	3069	3072	3075	rBV5	2145	2948	0.22%	0.024%
60	22.053	3134	3143	3154	rBV	465764	820476	61.61%	6.690%
61	22.212	3163	3170	3173	rBV7	5463	10077	0.76%	0.082%
62	22.541	3221	3226	3228	rBV4	1572	2592	0.19%	0.021%
63	22.864	3278	3281	3285	rVB6	5234	8346	0.63%	0.068%
64	23.169	3331	3333	3335	rBV3	3483	4099	0.31%	0.033%
65	23.616	3403	3409	3415	rBV5	11145	19546	1.47%	0.159%
66	23.728	3427	3428	3432	rVB3	2758	2768	0.21%	0.023%
67	23.792	3438	3439	3443	rBV4	3876	3884	0.29%	0.032%
68	24.004	3474	3475	3479	rVB3	4191	2537	0.19%	0.021%
69	24.045	3479	3482	3485	rVB5	2980	3413	0.26%	0.028%
70	24.133	3495	3497	3500	rBV4	1937	2575	0.19%	0.021%
71	24.356	3527	3535	3540	rBV6	3239	6536	0.49%	0.053%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080217\
 Data File : BG028110.D
 Acq On : 2 Aug 2017 15:59
 Operator : SJ/JU
 Sample : PB100940BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

72	24.497	3552	3559	3567	rVB4	15167	34120	2.56%	0.278%
73	24.709	3594	3595	3599	rBV4	2943	2794	0.21%	0.023%
74	24.885	3622	3625	3630	rVB5	1923	2740	0.21%	0.022%
75	25.326	3686	3700	3714	rBV	382580	1189353	89.31%	9.698%
76	25.567	3726	3741	3755	rBV	248559	834522	62.66%	6.805%
77	26.084	3827	3829	3832	rBV2	2612	2303	0.17%	0.019%
78	26.195	3847	3848	3851	rBV3	2115	2310	0.17%	0.019%
79	26.372	3875	3878	3879	rBV	2641	2714	0.20%	0.022%
80	26.759	3934	3944	3958	rVB4	24858	75148	5.64%	0.613%
81	27.082	3997	3999	4001	rBV2	3968	3586	0.27%	0.029%
82	27.247	4024	4027	4028	rVB3	2713	2338	0.18%	0.019%
83	28.234	4185	4195	4208	rVB3	21891	81435	6.11%	0.664%
84	28.763	4284	4285	4287	rBV2	3401	2281	0.17%	0.019%
85	29.762	4454	4455	4458	rBV3	2662	2609	0.20%	0.021%
86	30.026	4492	4500	4514	rVB9	15957	62764	4.71%	0.512%
87	30.825	4634	4636	4640	rVB4	1916	2031	0.15%	0.017%
88	32.182	4853	4867	4882	rVB4	12754	55448	4.16%	0.452%
89	32.394	4901	4903	4905	rBV2	3330	2730	0.20%	0.022%
90	32.459	4912	4914	4916	rBV	2107	1984	0.15%	0.016%


Sum of corrected areas: 12264028

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080217\
Data File : BG028110.D
Acq On : 2 Aug 2017 15:59
Operator : SJ/JU
Sample : PB100940BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

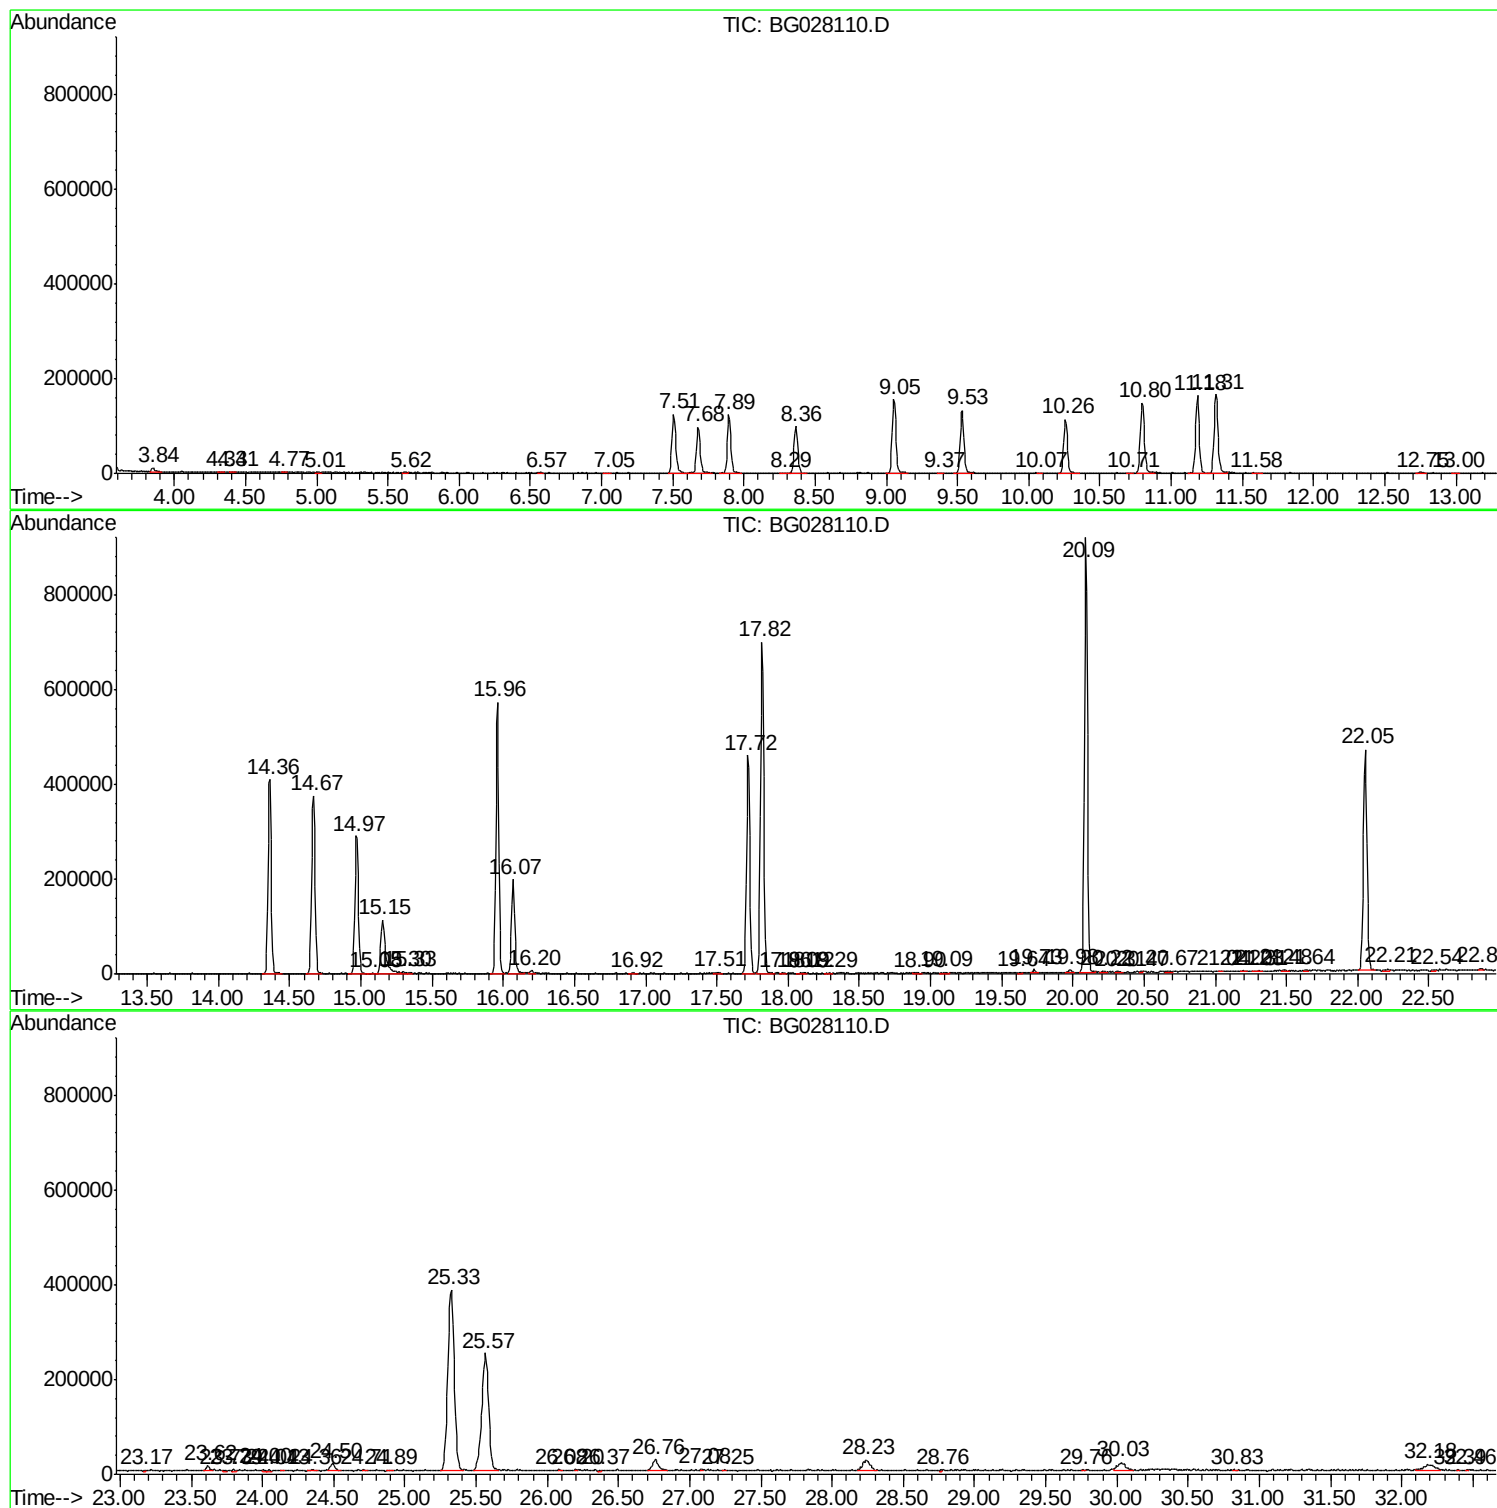

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080217\
Data File : BG028110.D
Acq On : 2 Aug 2017 15:59
Operator : SJ/JU
Sample : PB100940BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080217\
Data File : BG028110.D
Acq On : 2 Aug 2017 15:59
Operator : SJ/JU
Sample : PB100940BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc